

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103123\
 Data File : BM042506.D
 Acq On : 31 Oct 2023 11:48
 Operator : MA/JU
 Sample : PB156500BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB156500BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM042506.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.022	306	312	322	rBV	388240	535584	8.70%	1.690%
2	5.469	381	388	402	rBV	2614448	3823832	62.10%	12.064%
3	7.098	657	665	682	rBV	2486643	3937466	63.95%	12.422%
4	7.922	799	805	814	rBV	431792	682395	11.08%	2.153%
5	9.128	1002	1010	1023	rBV	1545131	2490095	40.44%	7.856%
6	10.745	1275	1285	1298	rBV	514443	869044	14.11%	2.742%
7	13.198	1695	1702	1715	rBV	3674583	5165266	83.89%	16.296%
8	14.574	1929	1936	1948	rBV	746092	1068041	17.35%	3.370%
9	16.068	2183	2190	2206	rBV	2974754	3951519	64.18%	12.466%
10	17.321	2397	2403	2418	rBV	777440	1129554	18.35%	3.564%
11	18.174	2544	2548	2562	rBV2	48367	109861	1.78%	0.347%
12	19.456	2762	2766	2774	rBV4	33374	61986	1.01%	0.196%
13	19.939	2842	2848	2860	rBV	5287279	6157076	100.00%	19.425%
14	21.503	3110	3114	3123	rBV	658964	899649	14.61%	2.838%
15	23.921	3520	3525	3536	rVB	393864	815768	13.25%	2.574%




Sum of corrected areas: 31697136

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103123\
Data File : BM042506.D
Acq On : 31 Oct 2023 11:48
Operator : MA/JU
Sample : PB156500BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB156500BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

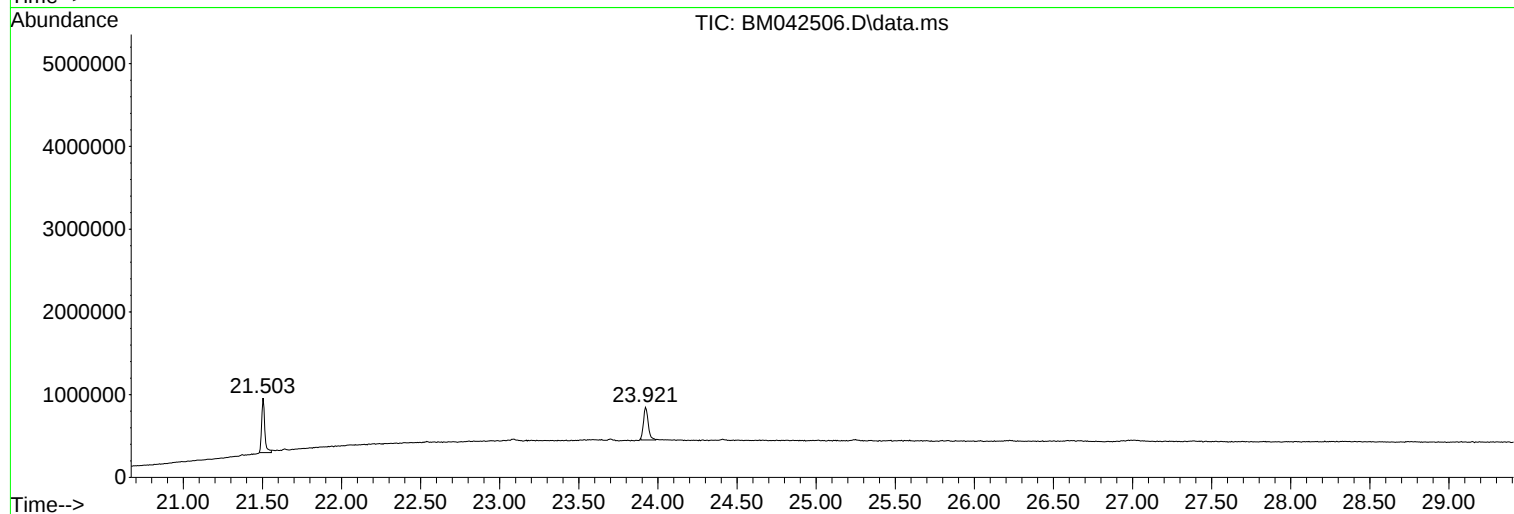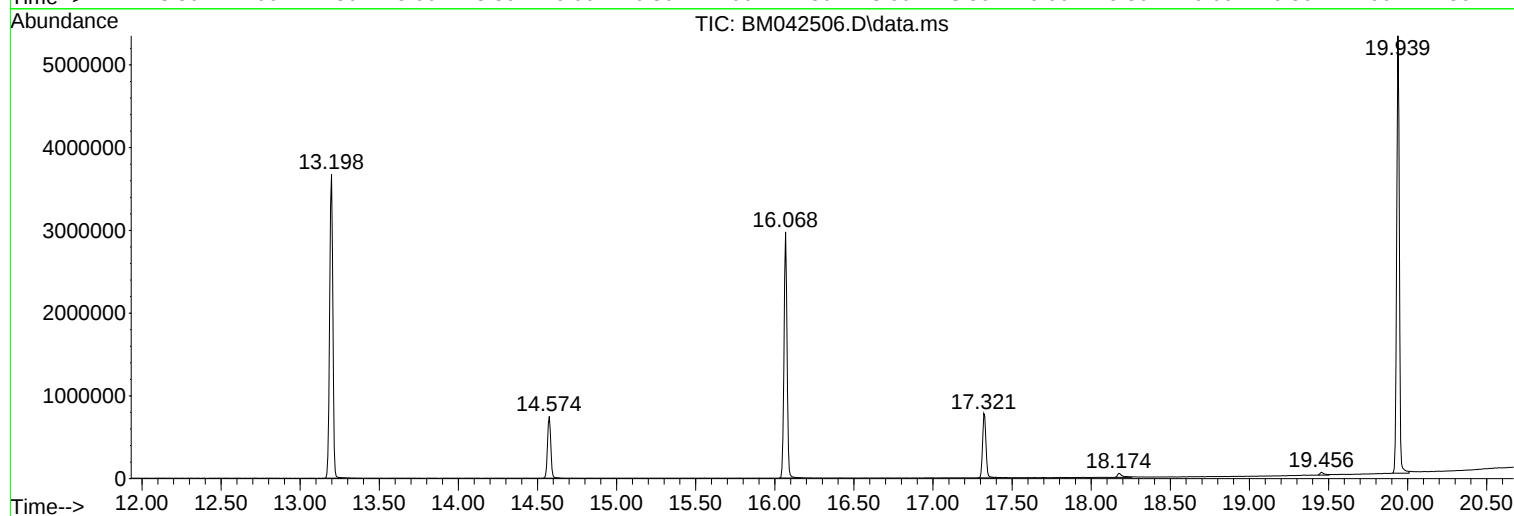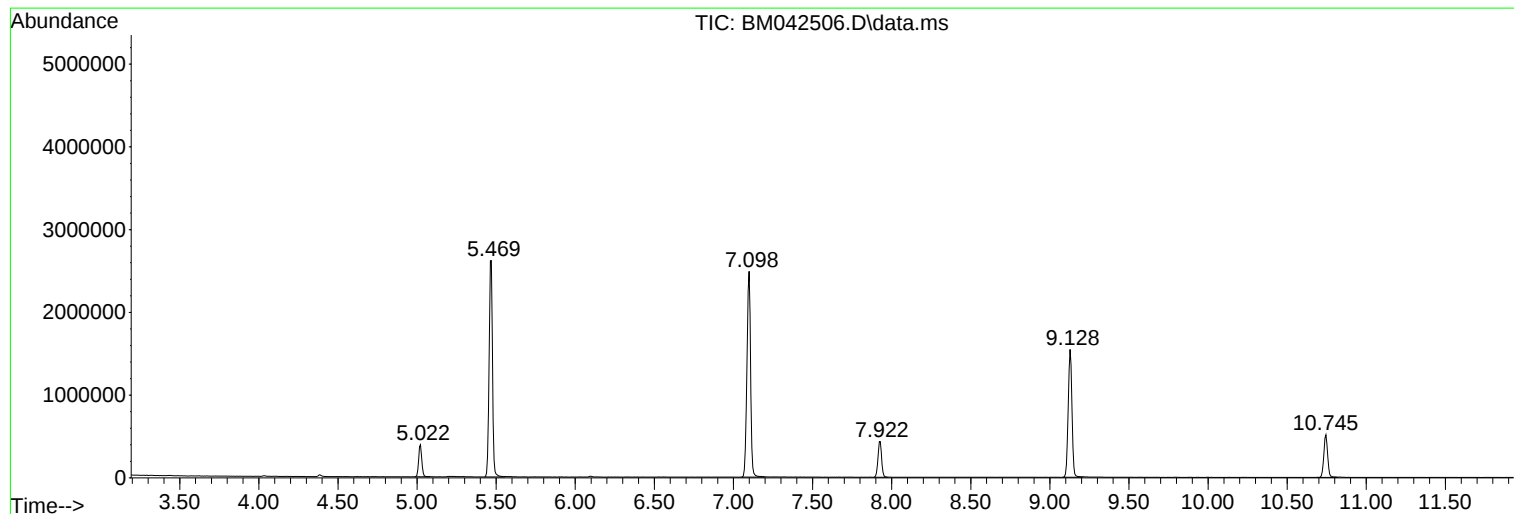

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103123\
Data File : BM042506.D
Acq On : 31 Oct 2023 11:48
Operator : MA/JU
Sample : PB156500BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB156500BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.022	15.70 ng	535584	1,4-Dichlorobenzene-d4	7.928

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25		
3	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	12		
4	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9		
5	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9		

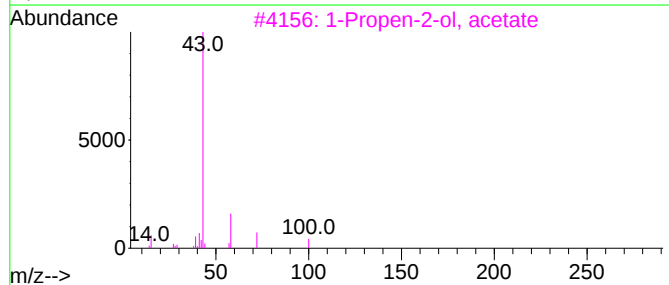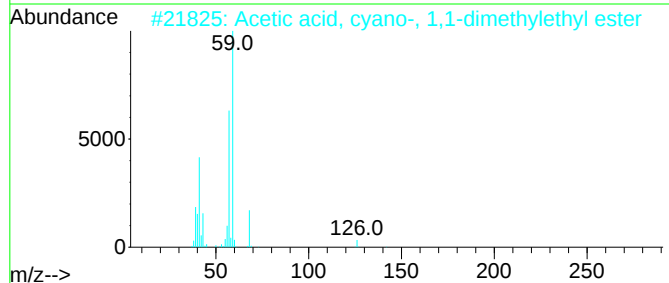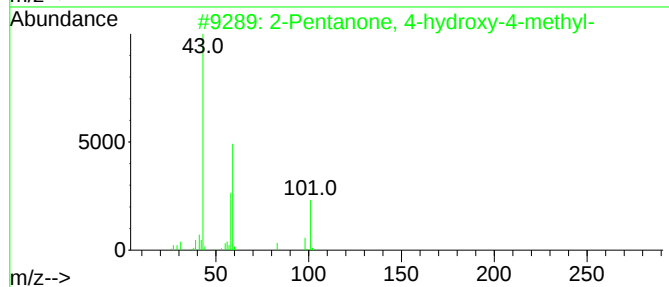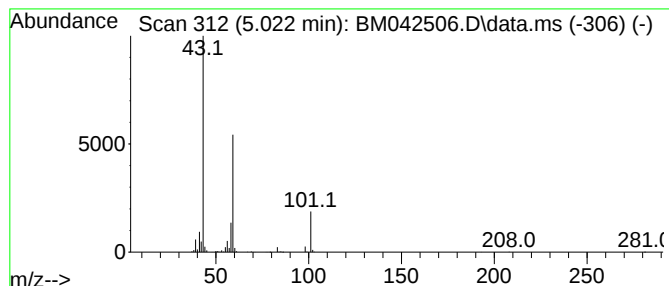

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103123\
Data File : BM042506.D
Acq On : 31 Oct 2023 11:48
Operator : MA/JU
Sample : PB156500BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB156500BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.022	15.7	ng	535584	1	7.928	682395	20.0