

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103123\
 Data File : BM042511.D
 Acq On : 31 Oct 2023 15:16
 Operator : MA/JU
 Sample : PB156527BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB156527BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM042511.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.016	306	311	318	rBV	208268	279048	5.04%	0.982%
2	5.463	380	387	401	rBV	2598362	3608366	65.12%	12.698%
3	7.093	656	664	683	rBV	2329823	3685571	66.52%	12.970%
4	7.922	798	805	816	rBV	401648	618168	11.16%	2.175%
5	9.128	1001	1010	1023	rBV	1429605	2307323	41.64%	8.120%
6	10.739	1278	1284	1297	rBV	453049	770643	13.91%	2.712%
7	13.198	1695	1702	1713	rBV	3315763	4725746	85.29%	16.631%
8	14.574	1929	1936	1948	rBV	644635	948585	17.12%	3.338%
9	16.068	2183	2190	2202	rBV	2614421	3565123	64.34%	12.546%
10	17.321	2397	2403	2415	rBV	682421	974984	17.60%	3.431%
11	19.939	2842	2848	2860	rBV	4860281	5540941	100.00%	19.499%
12	21.503	3110	3114	3124	rBV	531133	762278	13.76%	2.683%
13	23.921	3520	3525	3535	rVB	313249	629247	11.36%	2.214%




Sum of corrected areas: 28416023

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103123\
Data File : BM042511.D
Acq On : 31 Oct 2023 15:16
Operator : MA/JU
Sample : PB156527BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB156527BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

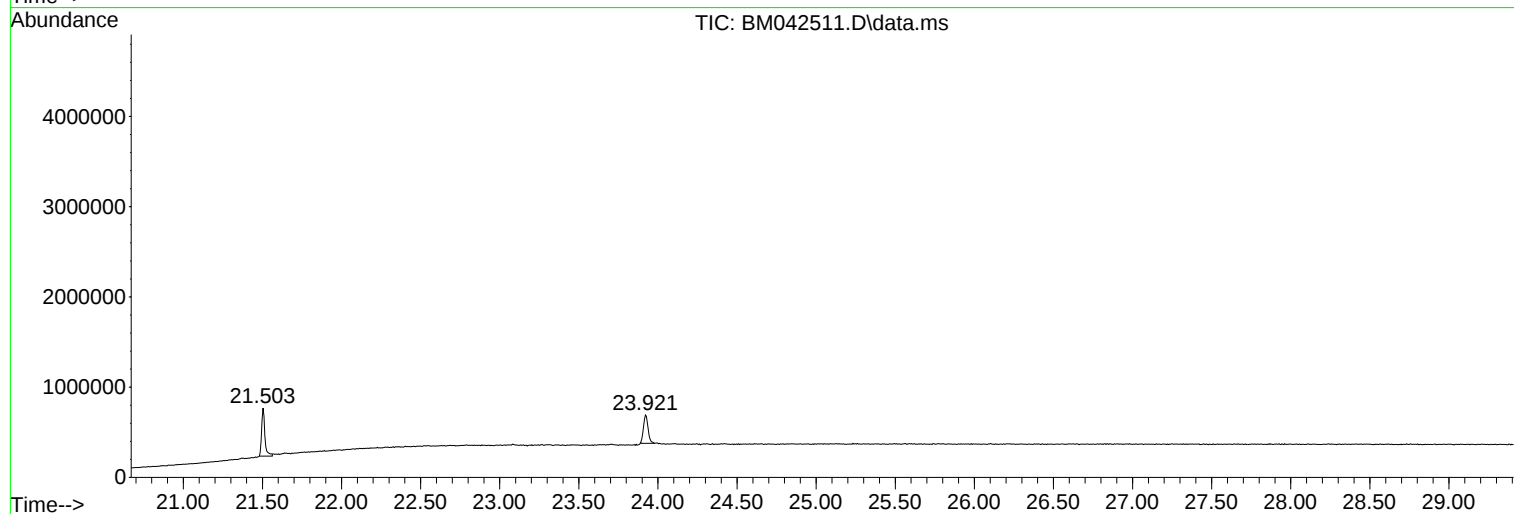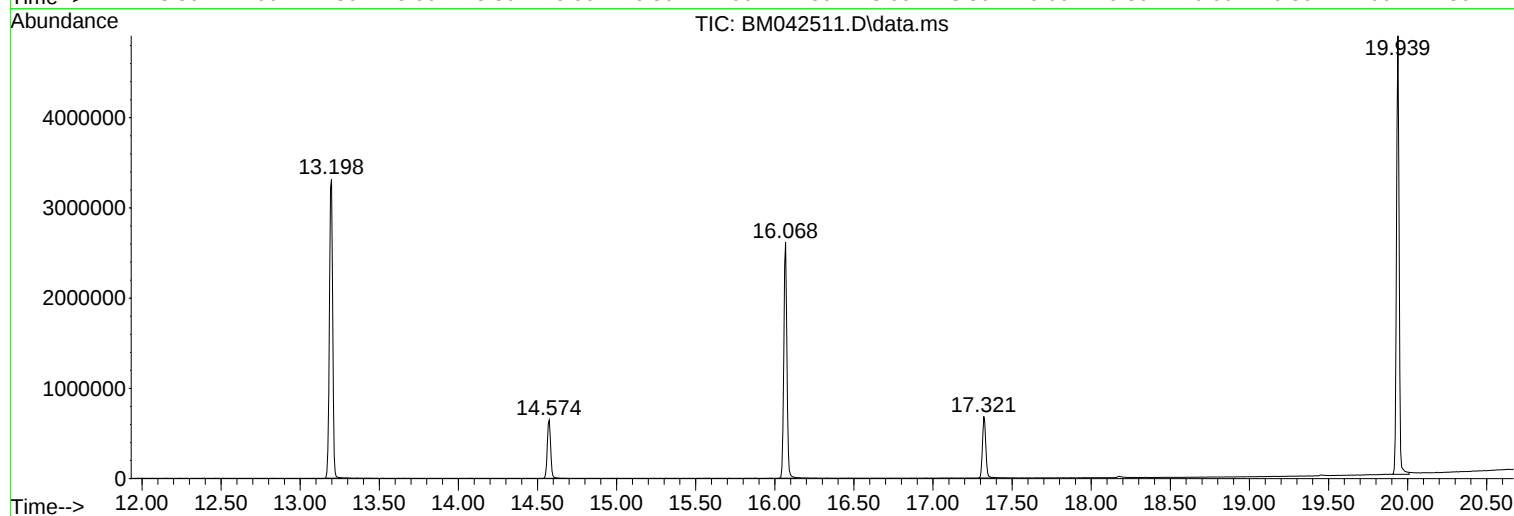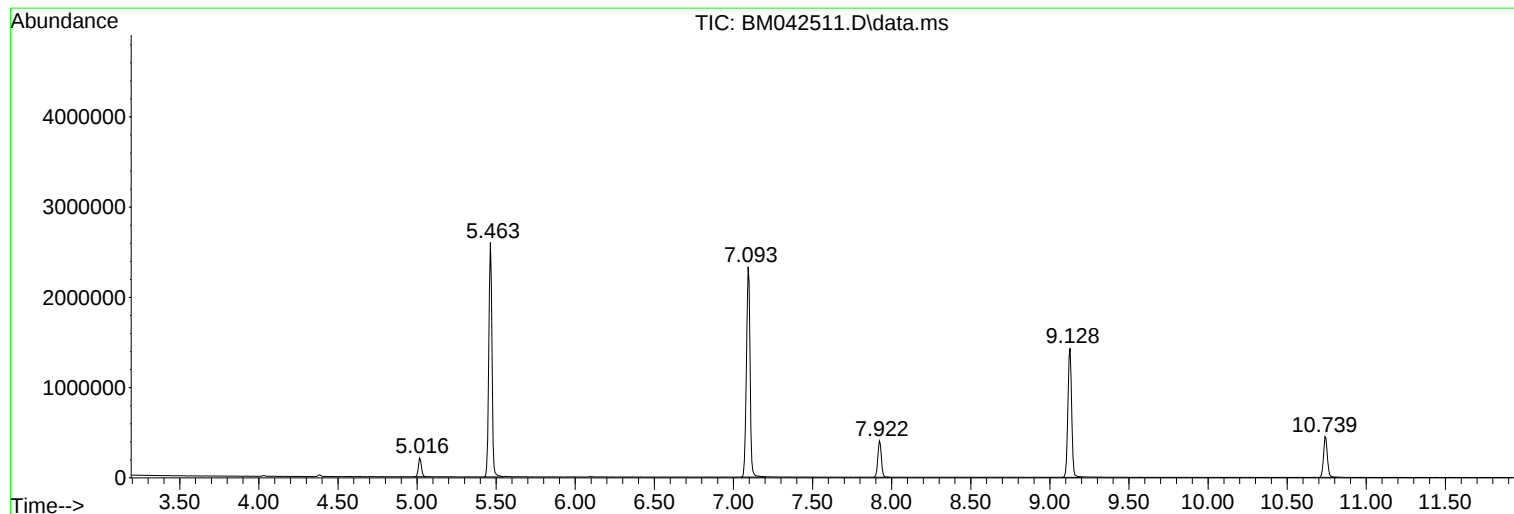

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103123\
Data File : BM042511.D
Acq On : 31 Oct 2023 15:16
Operator : MA/JU
Sample : PB156527BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB156527BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.016	9.03 ng	279048	1,4-Dichlorobenzene-d4	7.922

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56	
2	t-Butyl nitrite	103	C4H9NO2	000540-80-7	39	
3	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	16	
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	12	
5	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9	

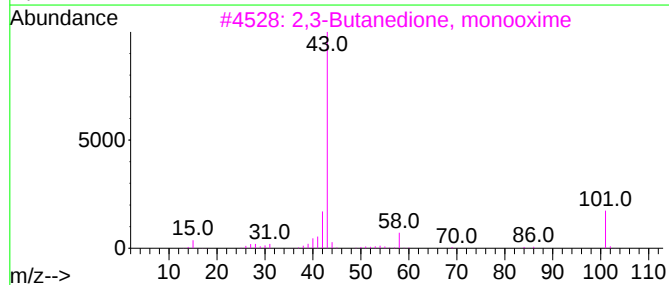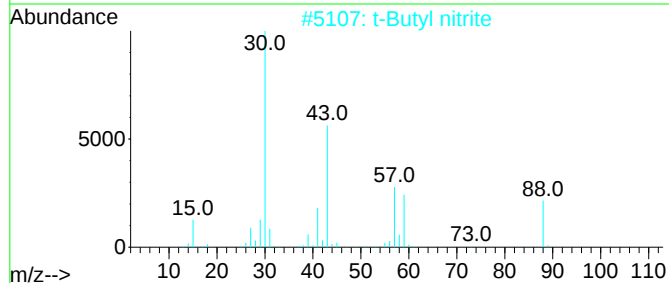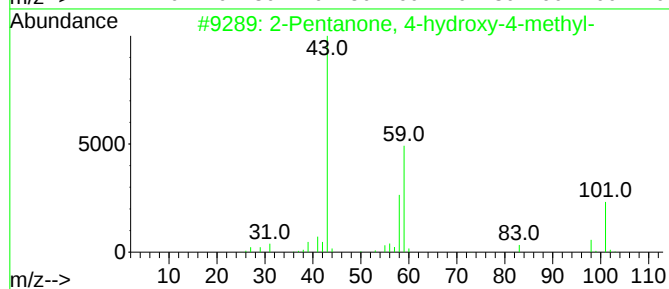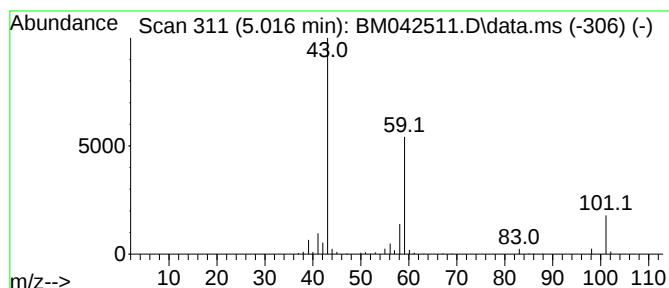

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103123\
Data File : BM042511.D
Acq On : 31 Oct 2023 15:16
Operator : MA/JU
Sample : PB156527BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB156527BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.016	9.0	ng	279048	1	7.922	618168	20.0