

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103123\
 Data File : BM042515.D
 Acq On : 31 Oct 2023 17:43
 Operator : MA/JU
 Sample : PB156565BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB156565BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM042515.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.016	305	311	318	rBV	403008	534726	8.94%	1.723%
2	5.463	380	387	401	rBV	2822421	3857956	64.47%	12.431%
3	7.093	656	664	687	rBV	2562636	4003022	66.89%	12.898%
4	7.922	798	805	817	rVB	441650	682228	11.40%	2.198%
5	9.128	1002	1010	1025	rBV	1494614	2412856	40.32%	7.775%
6	10.739	1276	1284	1295	rBV	505259	849585	14.20%	2.737%
7	13.198	1694	1702	1713	rBV	3509307	5046347	84.32%	16.260%
8	14.574	1929	1936	1950	rBV	710102	1052353	17.58%	3.391%
9	16.068	2183	2190	2205	rBV	2960762	3964864	66.25%	12.775%
10	17.321	2397	2403	2419	rBV	793974	1125512	18.81%	3.627%
11	19.939	2842	2848	2860	rBV	5233028	5984453	100.00%	19.283%
12	21.503	3109	3114	3122	rBV	582383	845280	14.12%	2.724%
13	23.921	3520	3525	3533	rVB	335685	675979	11.30%	2.178%




Sum of corrected areas: 31035161

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103123\
Data File : BM042515.D
Acq On : 31 Oct 2023 17:43
Operator : MA/JU
Sample : PB156565BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB156565BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

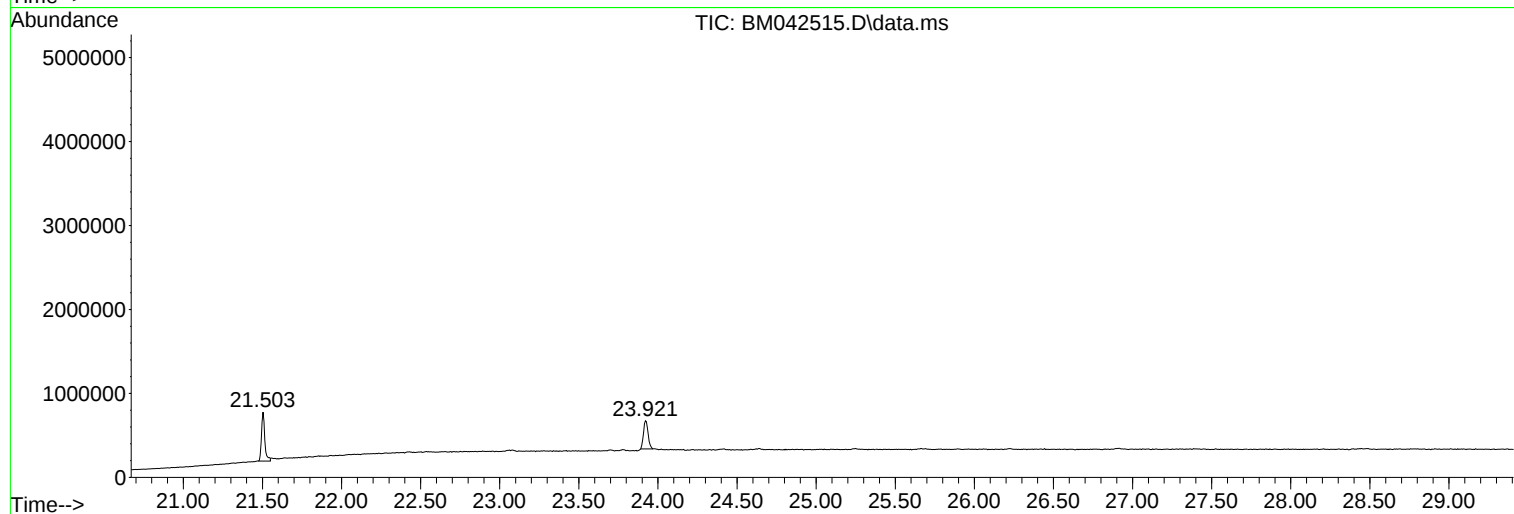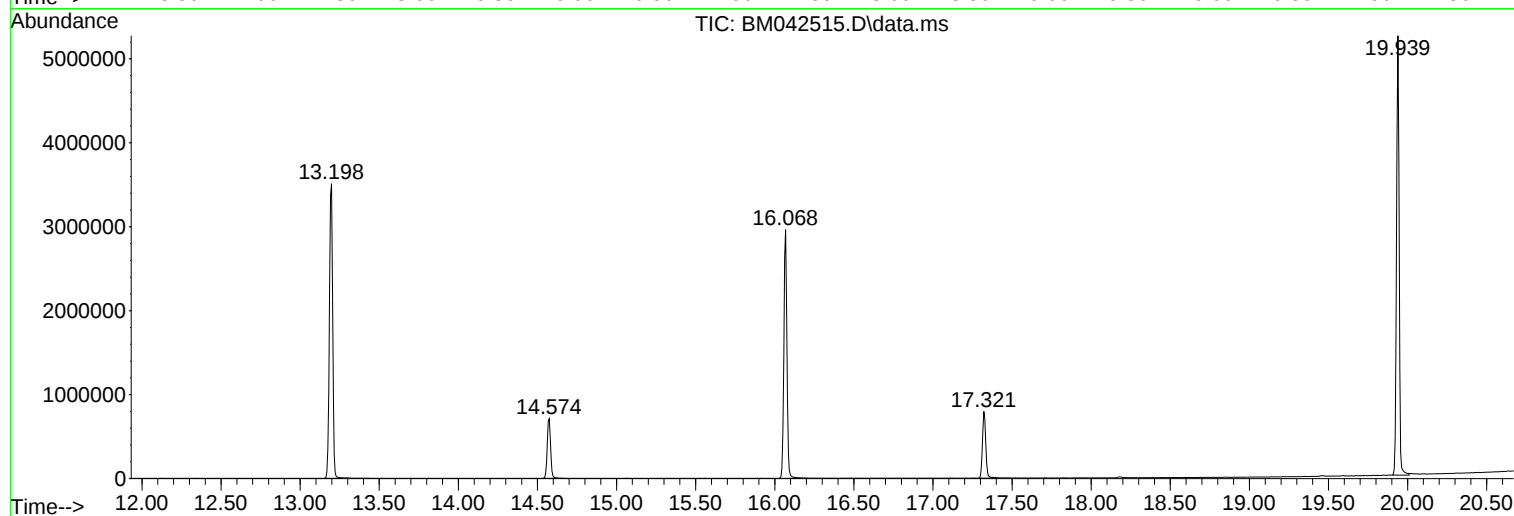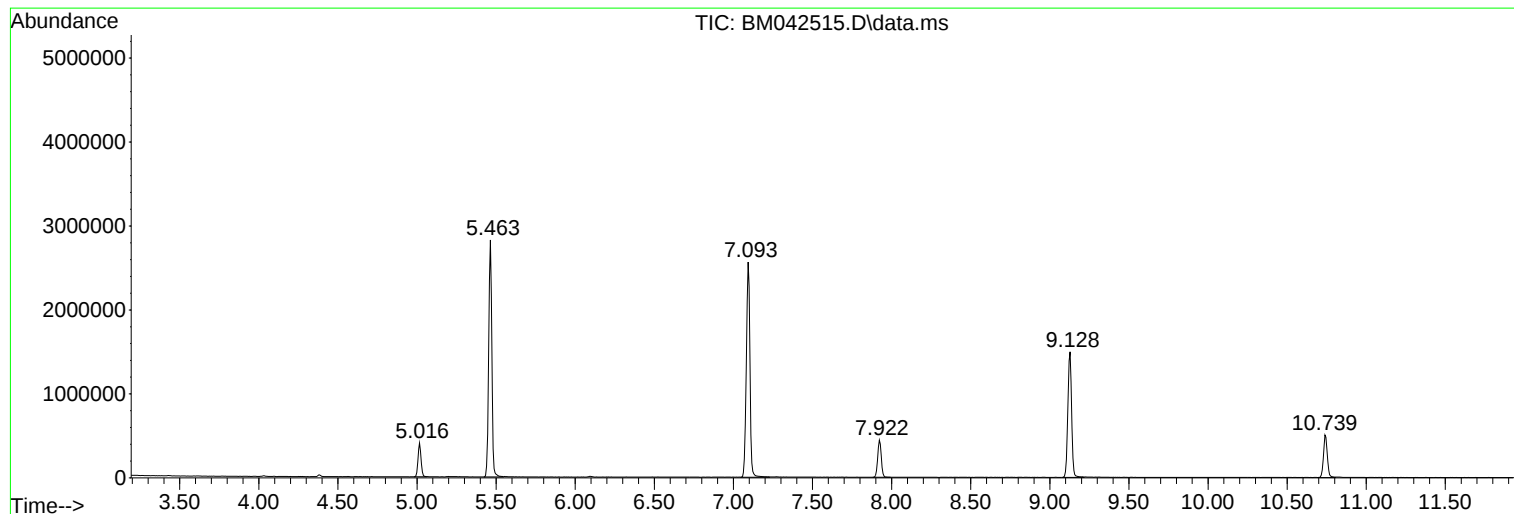

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103123\
Data File : BM042515.D
Acq On : 31 Oct 2023 17:43
Operator : MA/JU
Sample : PB156565BL
Misc :
ALS Vial : 4 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
PB156565BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD			R.T.
5.016	15.68 ng	534726	1,4-Dichlorobenzene-d4			7.922
Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2		000123-42-2	50
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2		001116-98-9	25
3	2,3-Butanedione, monooxime	101	C4H7NO2		000057-71-6	16
4	1-Propen-2-ol, acetate	100	C5H8O2		000108-22-5	12
5	n-Propyl t-butyl ether	116	C7H16O		1000334-81-9	9

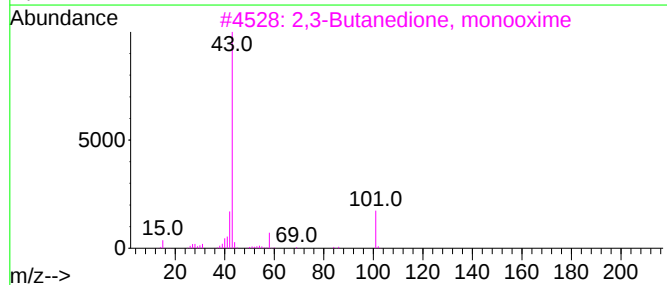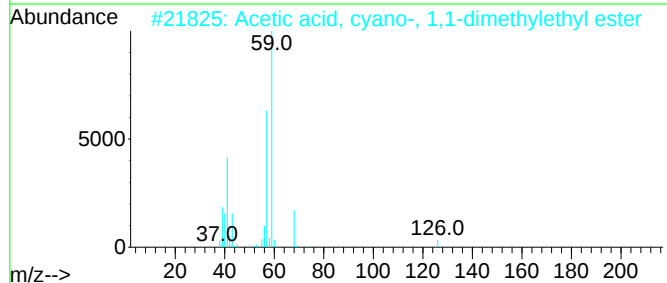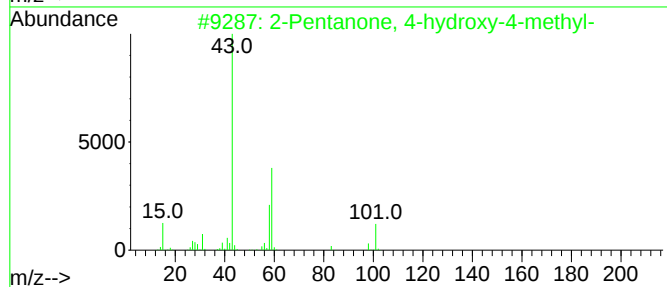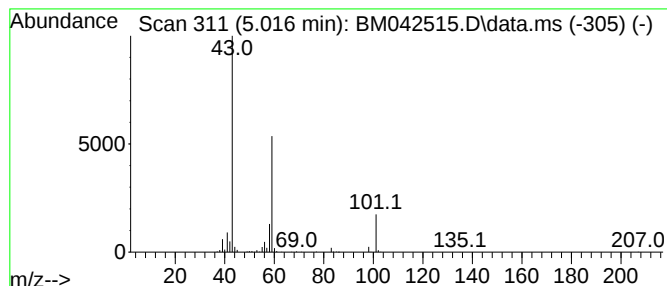

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103123\
Data File : BM042515.D
Acq On : 31 Oct 2023 17:43
Operator : MA/JU
Sample : PB156565BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB156565BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.016	15.7	ng	534726	1	7.922	682228	20.0