
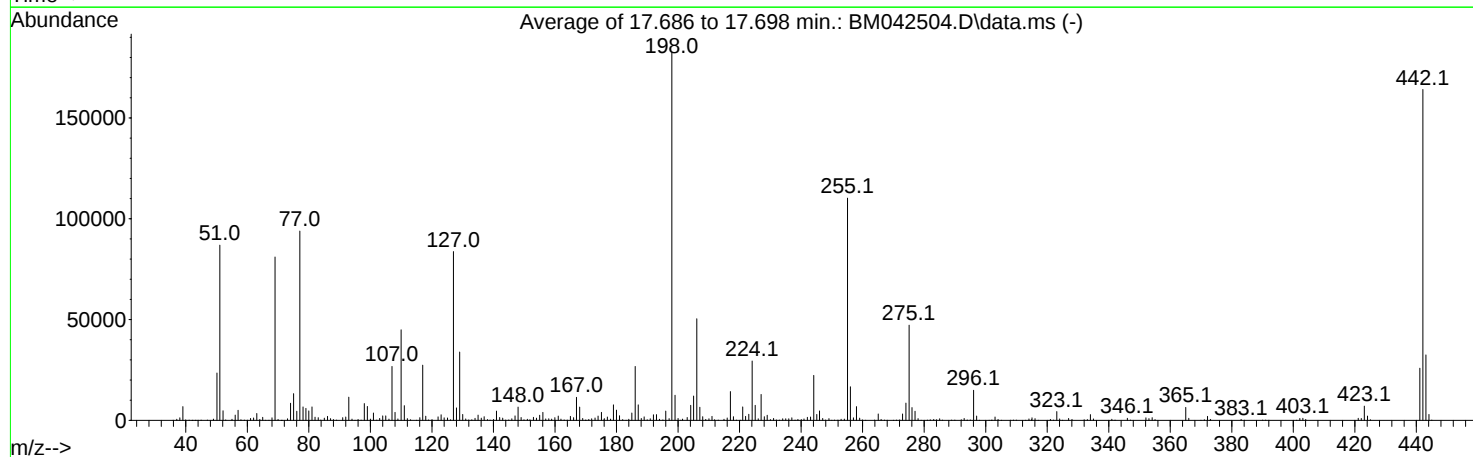


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103123\
 Data File : BM042504.D
 Acq On : 31 Oct 2023 10:36
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 31 02:55:18 2023



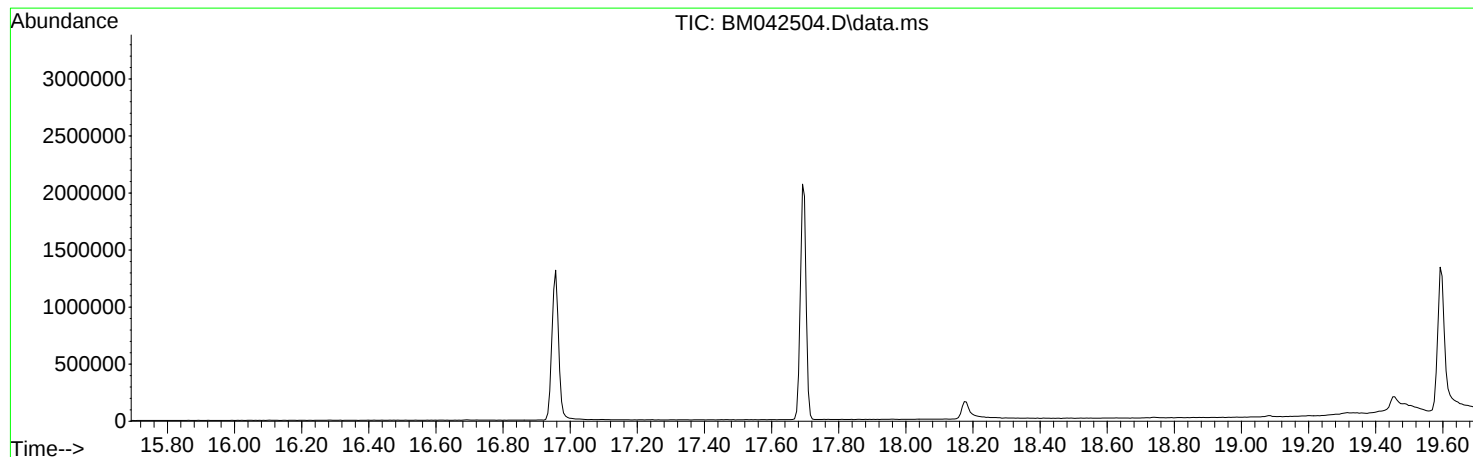


AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.6	86907	PASS
68	69	0.00	2	1.6	1318	PASS
69	198	0.00	100	44.4	81079	PASS
70	69	0.00	2	0.6	477	PASS
127	198	10	80	45.9	83765	PASS
197	198	0.00	2	0.5	842	PASS
198	198	100	100	100.0	182493	PASS
199	198	5	9	6.8	12500	PASS
275	198	10	60	25.9	47264	PASS
365	198	1	100	3.5	6452	PASS
441	198	0.01	100	14.2	25843	PASS
442	442	50	100	100.0	164160	PASS
443	442	15	24	19.8	32488	PASS

Instrument :
BNA_M
ClientSampleId :
DFTPP

lon 265.70 (265.40 to 266.40): BM042504.D\data.ms
lon 268.00 (267.70 to 268.70): BM042504.D\data.ms
lon 264.00 (263.70 to 264.70): BM042504.D\data.ms

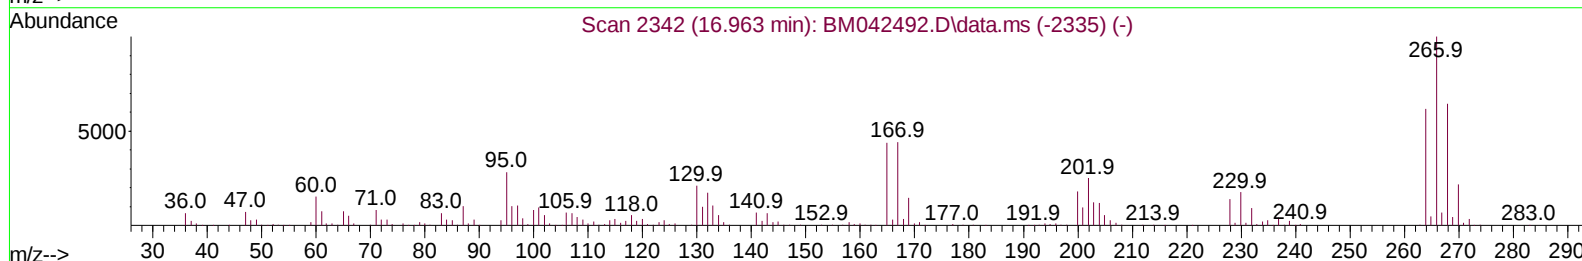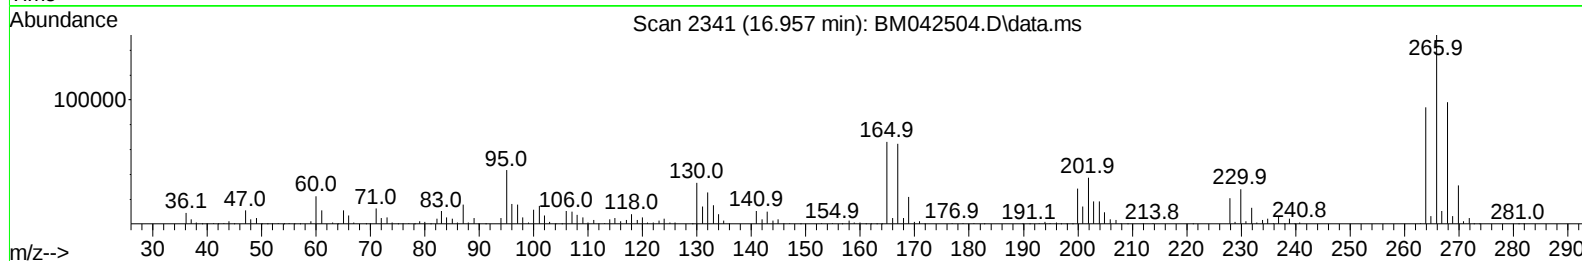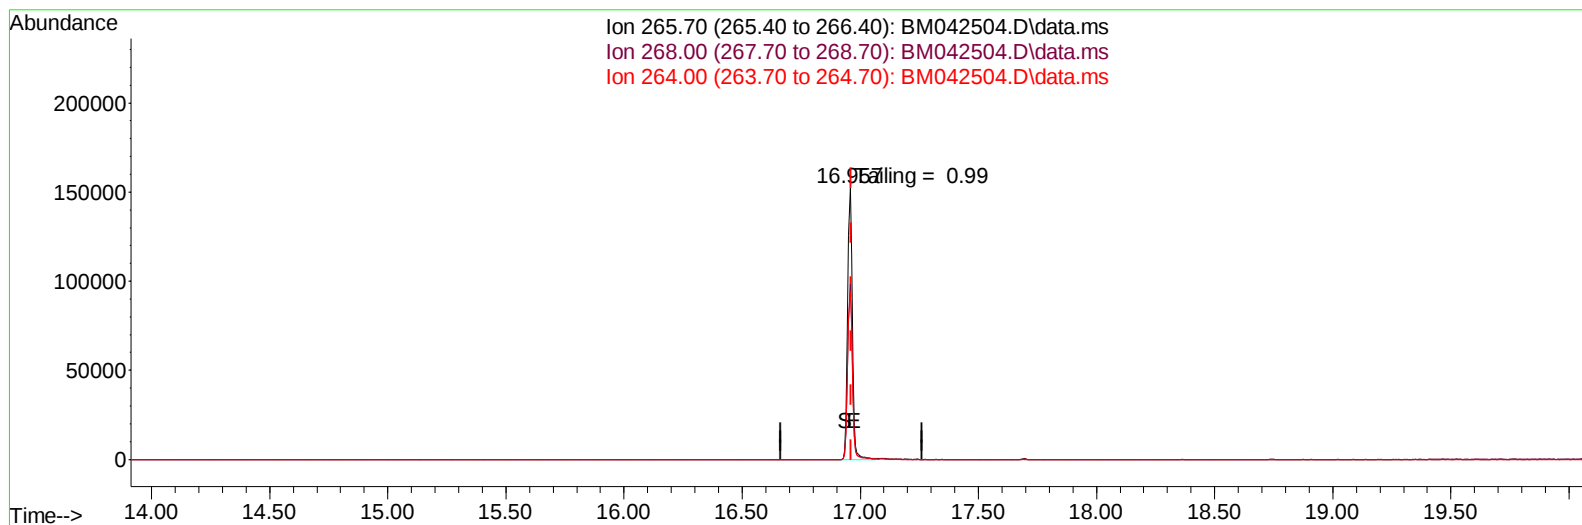

TIC: BM042504.D\data.ms




response **209574**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	64.41
264.00	61.80	61.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103123\
Data File : BM042504.D
Acq On : 31 Oct 2023 10:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 01 02:52:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 31 02:55:18 2023
Response via : Initial Calibration

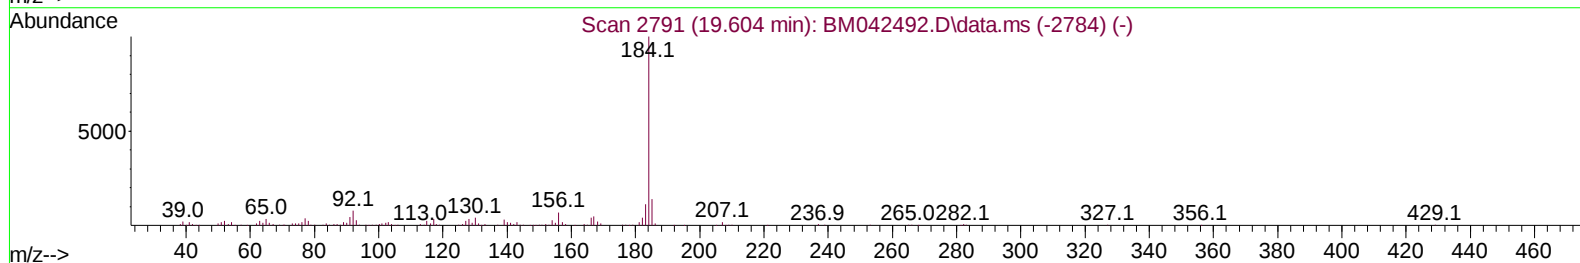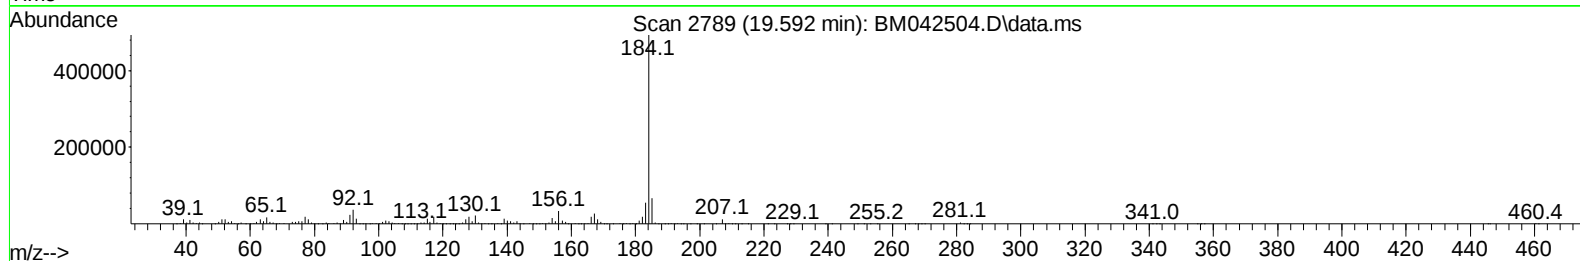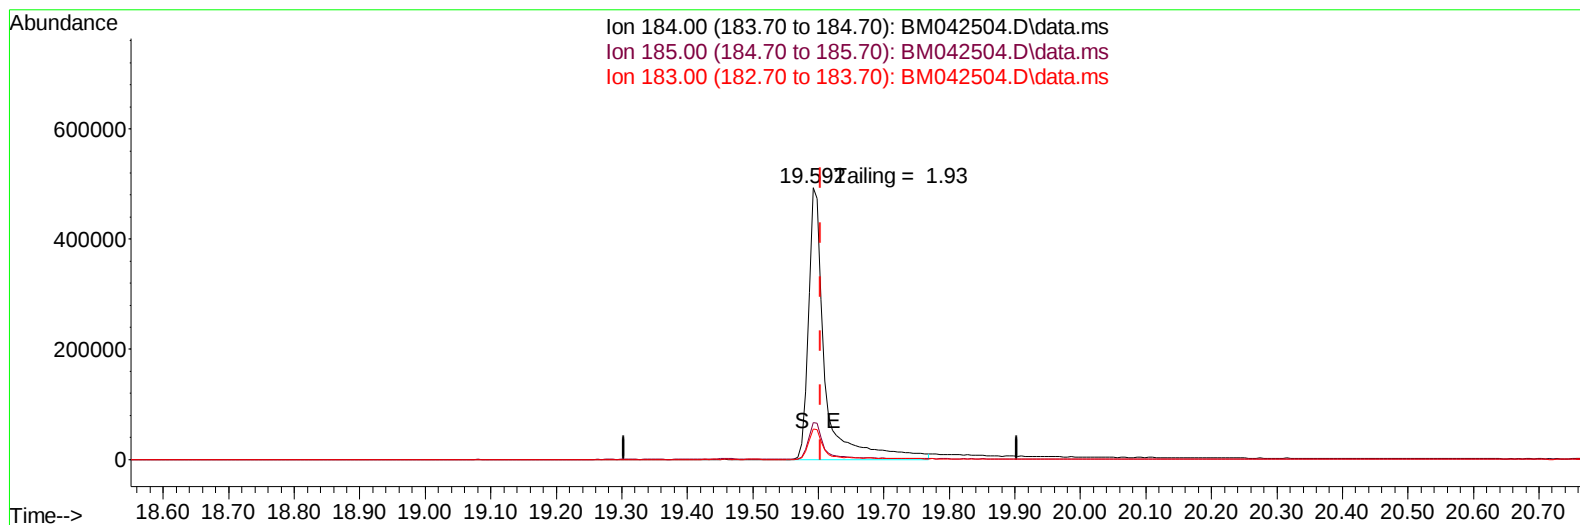

TIC: BM042504.D\data.ms

(77) Benzidine

19.592min (-0.012) 127426.24 ng

response 872728

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.54
183.00	11.20	11.18
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/31/2023	BNA_M	<u>BM042504.D</u>
Compound Name	Response	Retention Time
DDT	638248	20.78
DDD	11558	20.345
DDE	343	19.833
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11901	650149	1.83

Instrument :
BNA_M
ClientSampleId :
DFTPP