

Data File : BM017460.D

Acq On : 01 Nov 2018 11:53

Operator : MJ/SJ

Sample : J5701-19

Misc :

ALS Vial : 5 Sample Multiplier: 1




Quant Time: Nov 02 01:59:28 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Fri Nov 02 01:56:23 2018

Response via : Initial Calibration

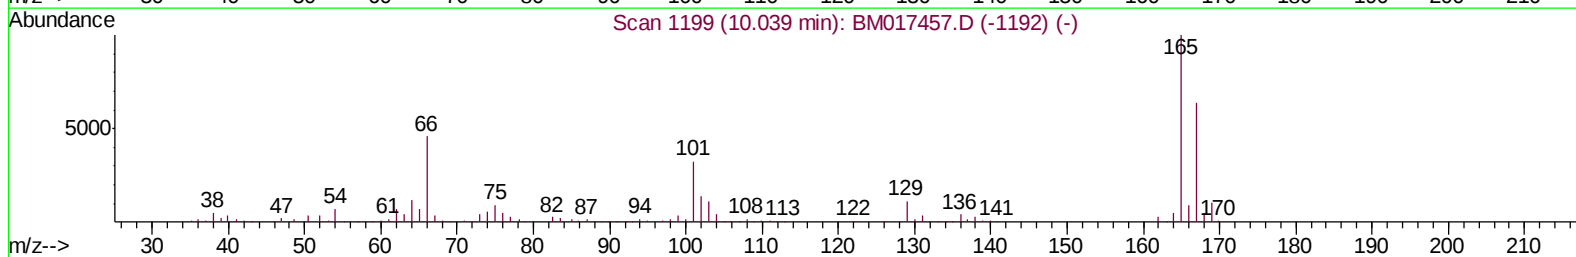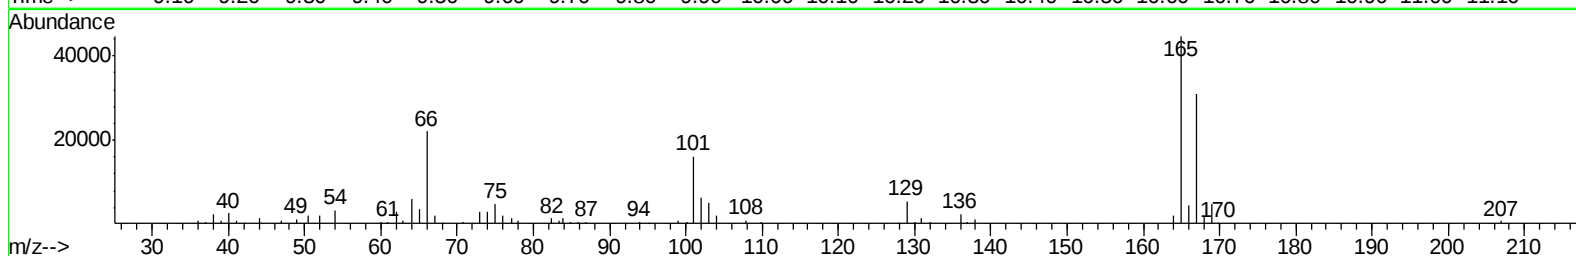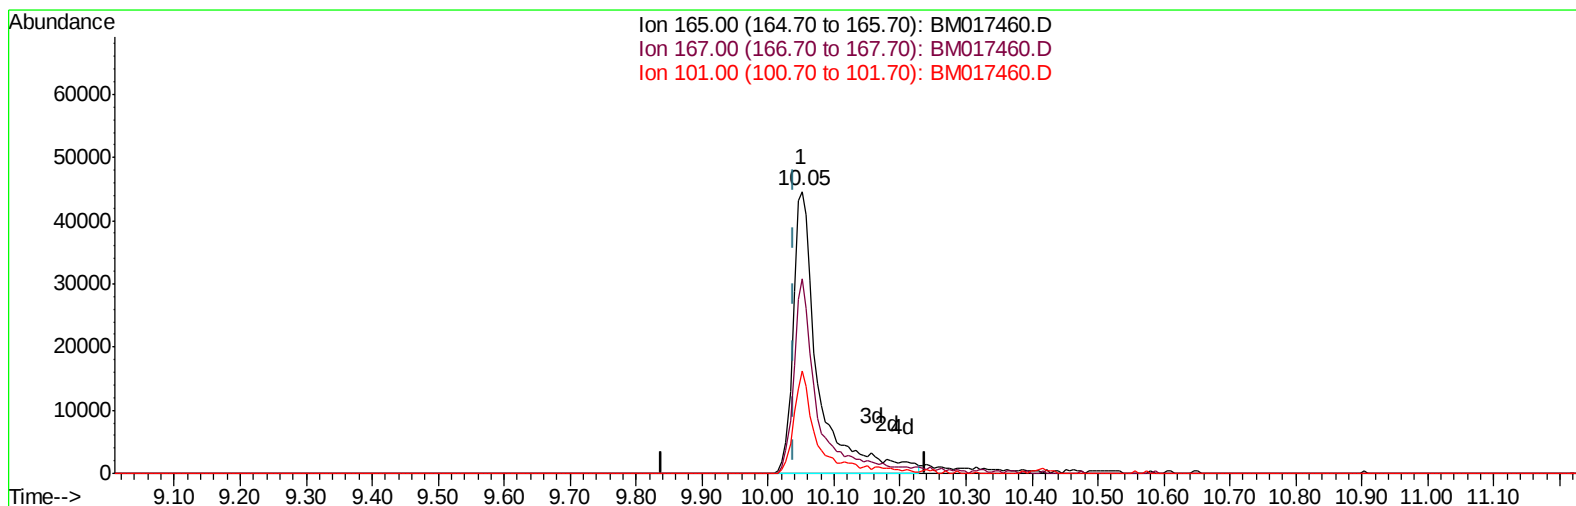

TIC: BM017460.D

(26) 2,4-Dichlorophenol-d3 (S)

10.051min (+0.012) 8.03ng/ul m

response 117854

Ion	Exp%	Act%
165.00	100	100
167.00	63.60	69.33
101.00	34.30	36.35
0.00	0.00	0.00