
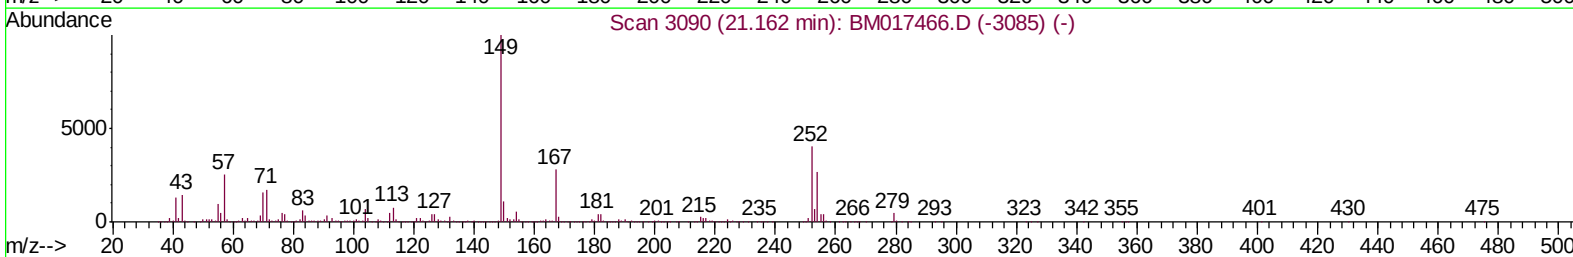
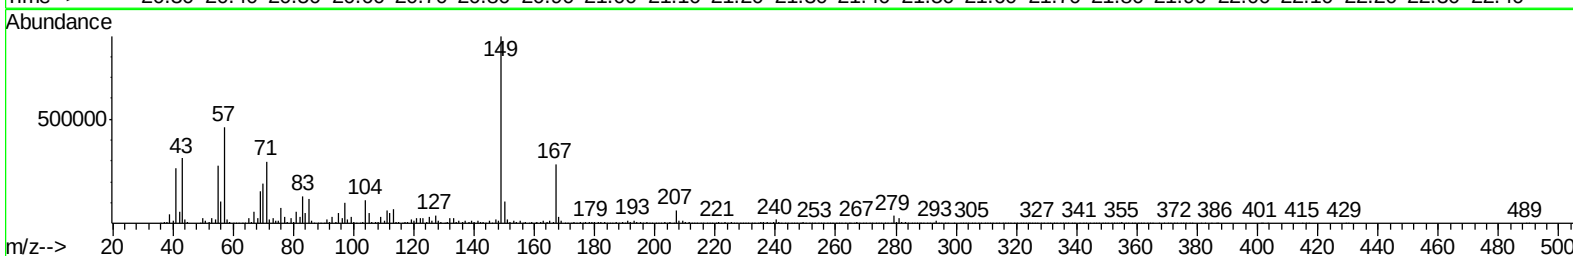


Data File : BM017471.D
Acq On : 01 Nov 2018 18:36
Operator : MJ/SJ
Sample : J5704-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Nov 02 03:05:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 02 02:41:22 2018
Response via : Initial Calibration

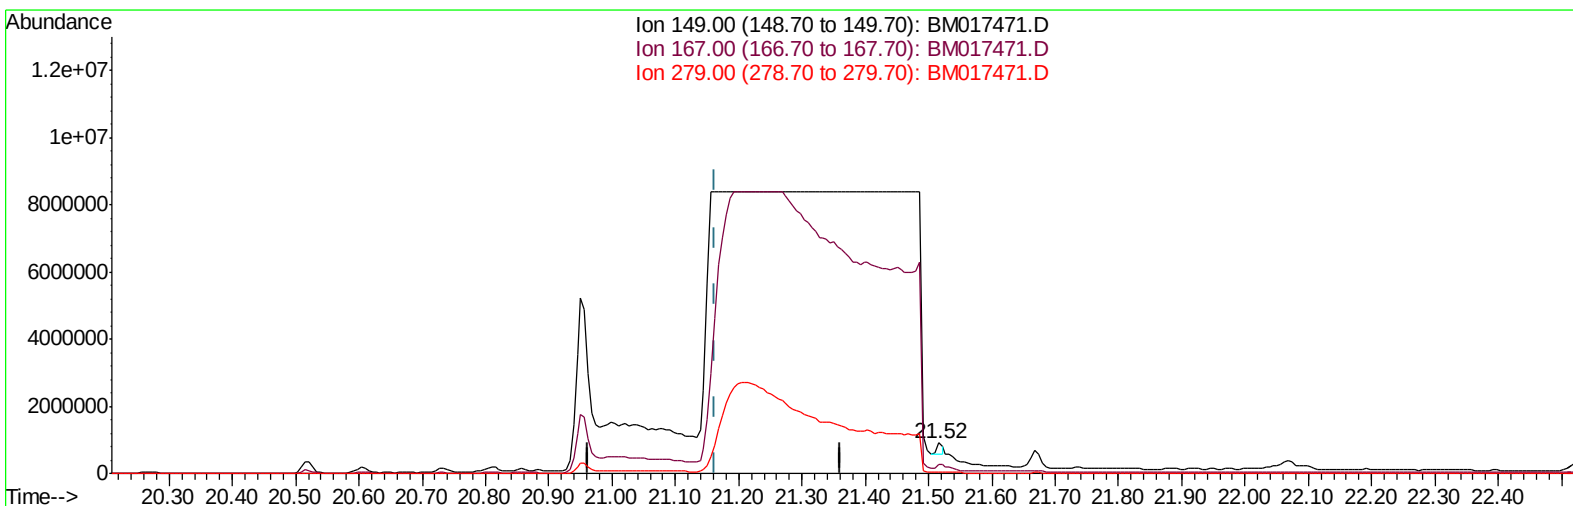

TIC: BM017471.D

(84) Bis(2-ethylhexyl)phthalate

21.515min (+0.353) 34.74ng/ul

response 218261

Ion	Exp%	Act%
149.00	100	100
167.00	28.80	31.77
279.00	5.10	4.02#
0.00	0.00	0.00