
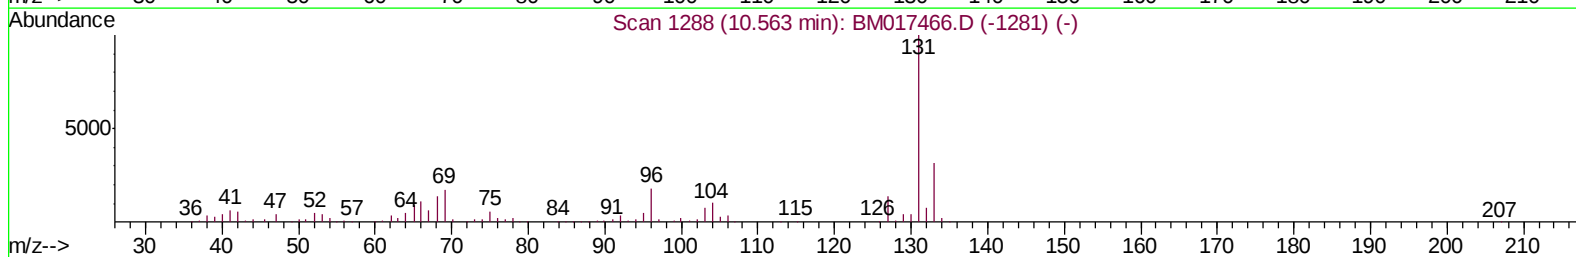
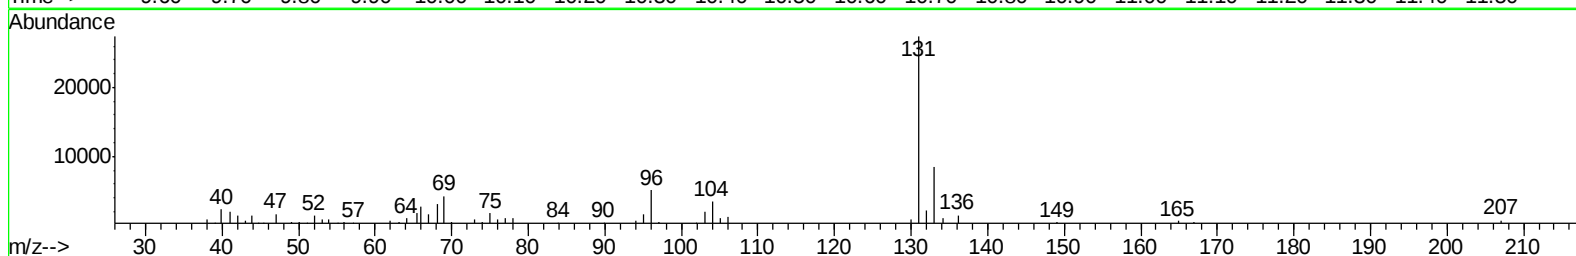


Data File : BM017475.D
Acq On : 01 Nov 2018 21:01
Operator : MJ/SJ
Sample : J5704-21
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Nov 02 02:45:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 02 02:41:22 2018
Response via : Initial Calibration

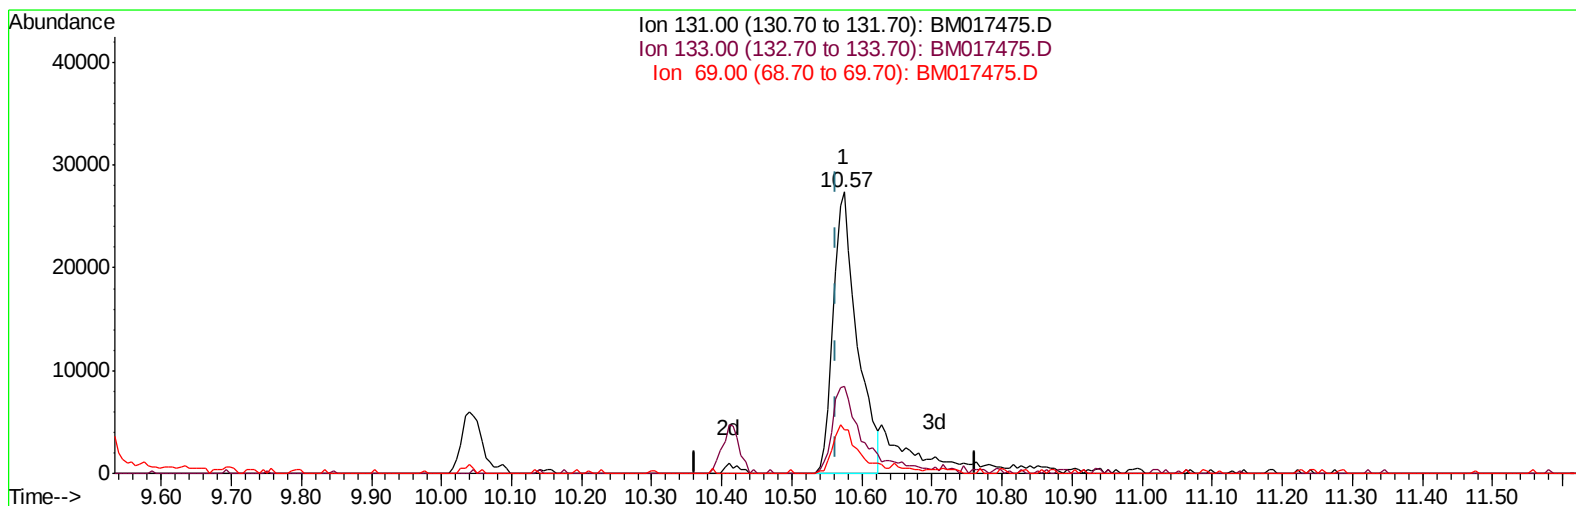

TIC: BM017475.D

(29) 4-Chloroaniline-d4 (S)
10.575min (+0.012) 4.53ng/ul
response 64383

Ion	Exp%	Act%
131.00	100	100
133.00	33.60	30.98
69.00	17.60	15.63
0.00	0.00	0.00