
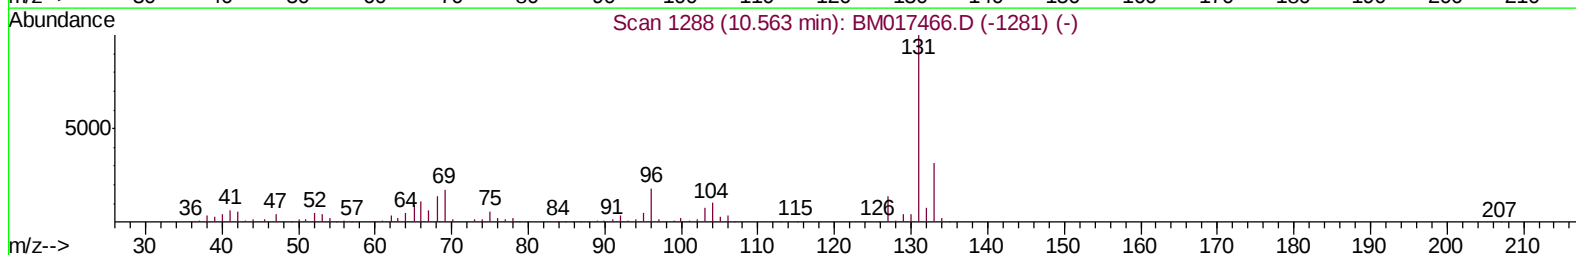
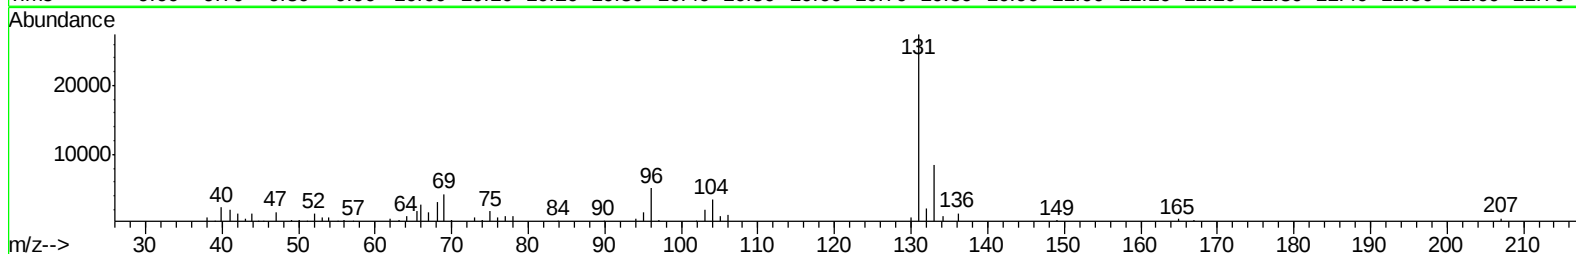


Data File : BM017475.D  
Acq On : 01 Nov 2018 21:01  
Operator : MJ/SJ  
Sample : J5704-21  
Misc :  
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Nov 02 02:45:28 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM102418MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Fri Nov 02 02:41:22 2018  
Response via : Initial Calibration

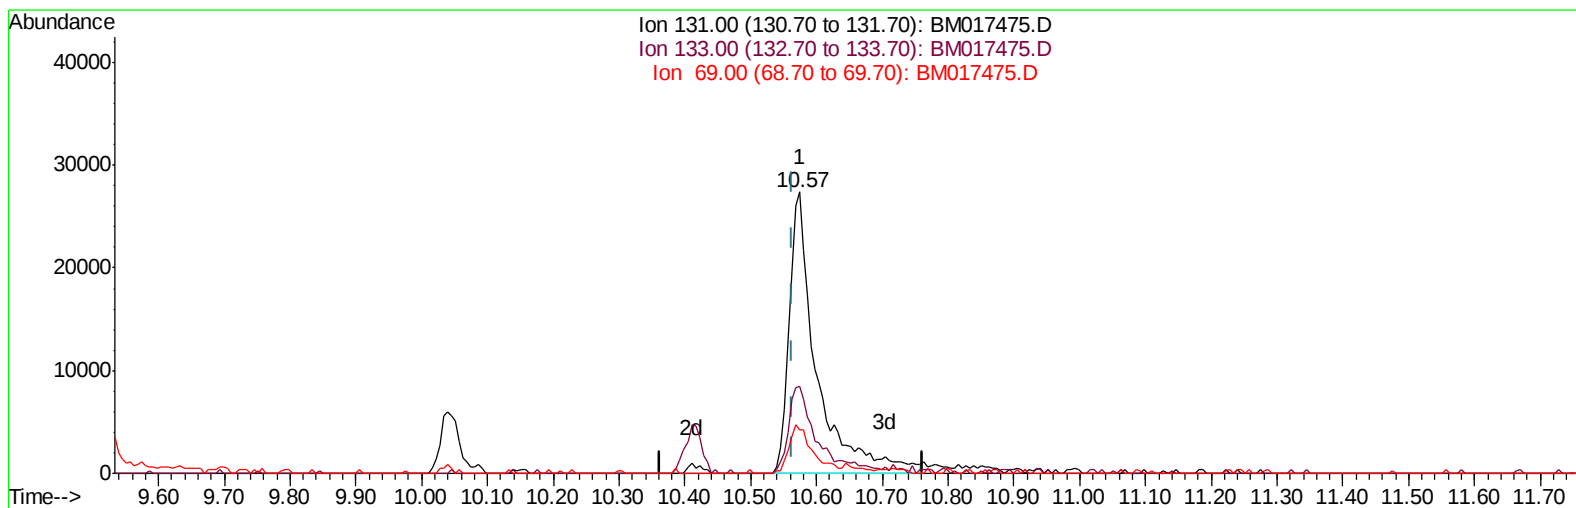

TIC: BM017475.D

(29) 4-Chloroaniline-d4 (S)

10.575min (+0.012) 5.59ng/ul m

response 79368

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 131.00 | 100   | 100   |
| 133.00 | 33.60 | 30.98 |
| 69.00  | 17.60 | 15.63 |
| 0.00   | 0.00  | 0.00  |