
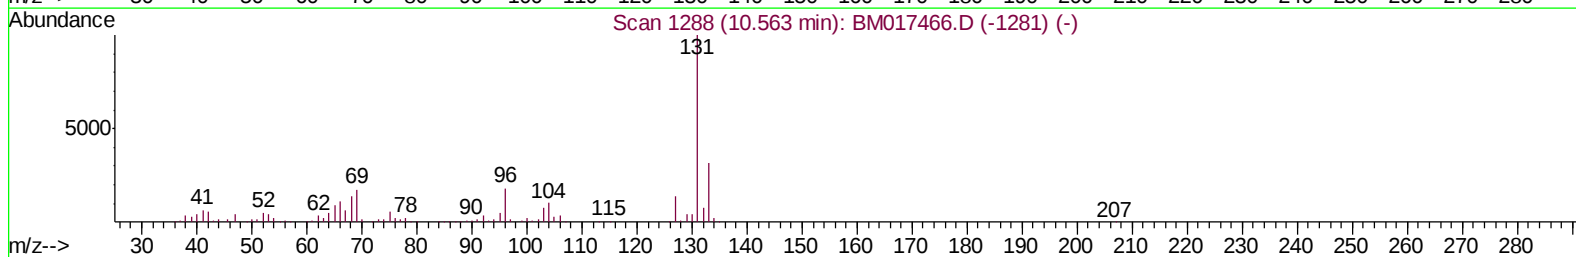
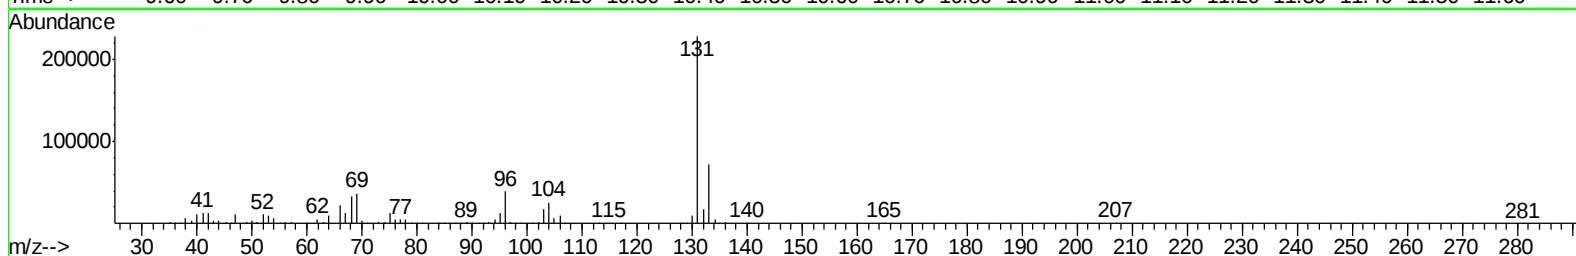


Data File : BM017481.D
Acq On : 02 Nov 2018 00:38
Operator : MJ/SJ
Sample : J5657-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Nov 02 02:46:36 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 02 02:41:22 2018
Response via : Initial Calibration

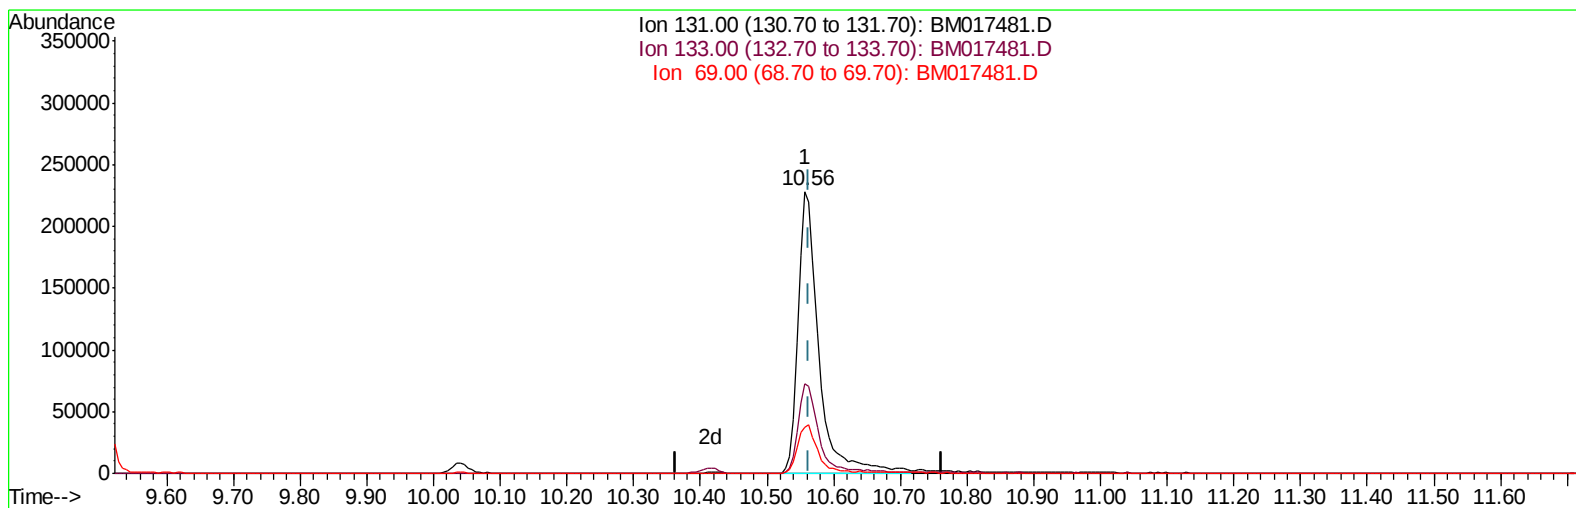

TIC: BM017481.D

(29) 4-Chloroaniline-d4 (S)
10.557min (-0.006) 34.10ng/ul m
response 486947

Ion	Exp%	Act%
131.00	100	100
133.00	33.60	31.81
69.00	17.60	16.20
0.00	0.00	0.00