
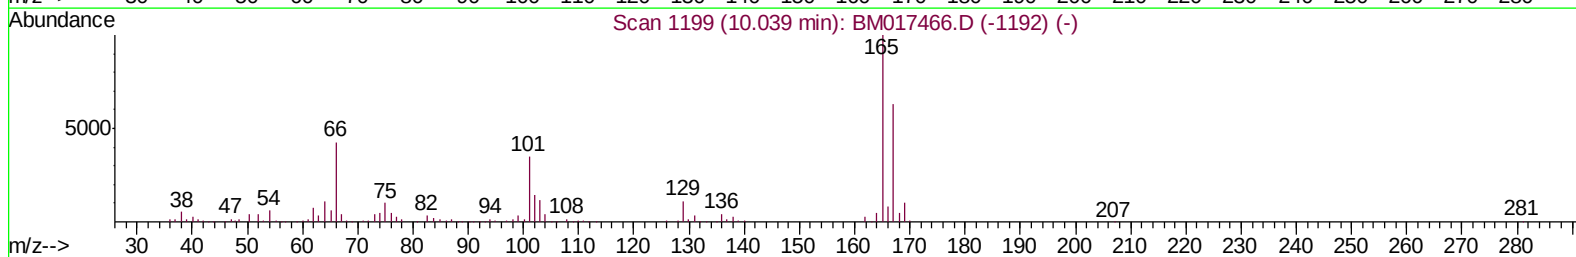
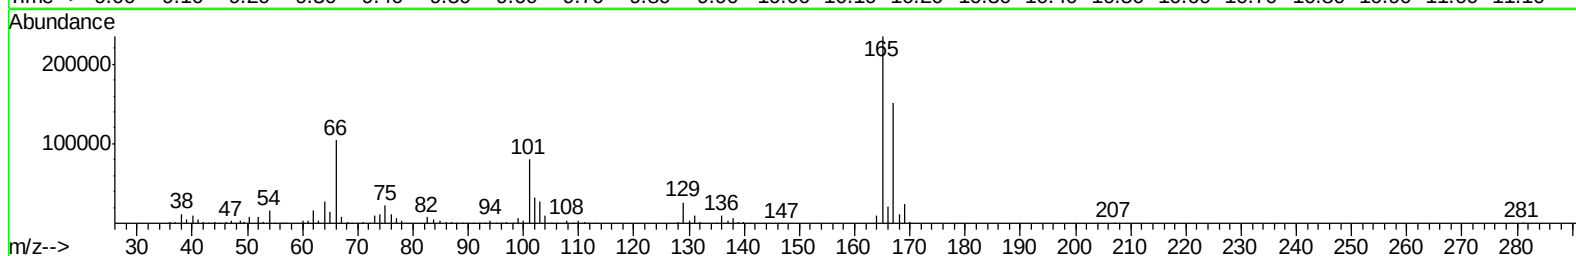


Data File : BM017482.D
Acq On : 02 Nov 2018 01:14
Operator : MJ/SJ
Sample : J5657-17MS
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Nov 02 04:23:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 02 02:41:22 2018
Response via : Initial Calibration

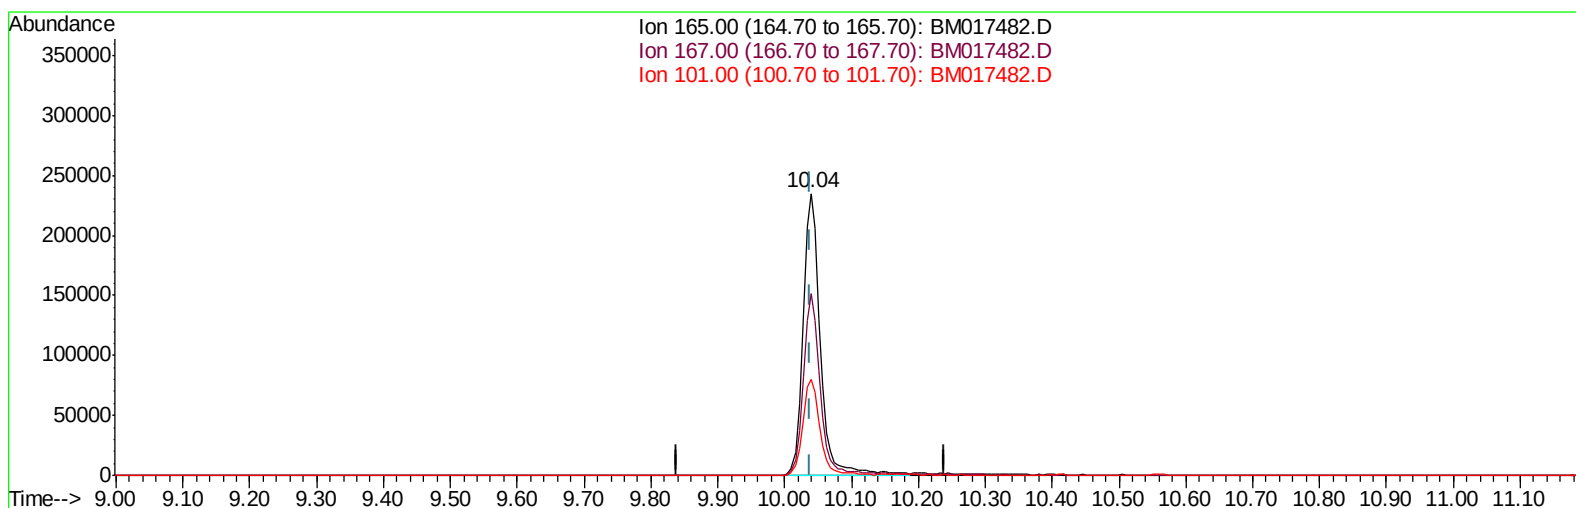

TIC: BM017482.D

(26) 2,4-Dichlorophenol-d3 (S)
10.039min (+0.000) 21.70ng/ul m
response 428169

Ion	Exp%	Act%
165.00	100	100
167.00	63.60	64.53
101.00	34.30	34.19
0.00	0.00	0.00