
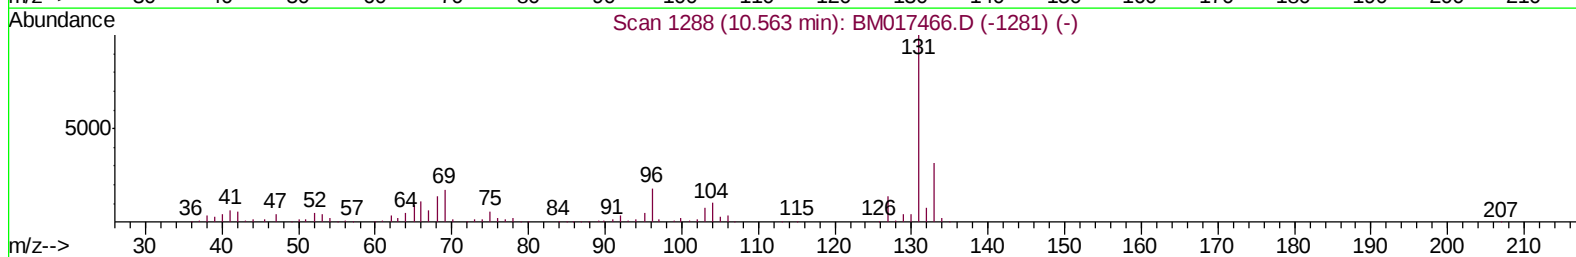
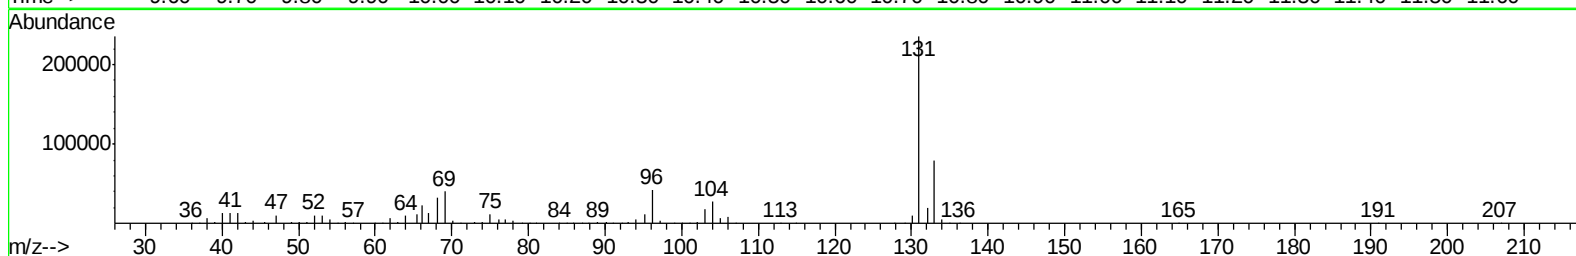


Data File : BM017482.D
Acq On : 02 Nov 2018 01:14
Operator : MJ/SJ
Sample : J5657-17MS
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Nov 02 04:23:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 02 02:41:22 2018
Response via : Initial Calibration

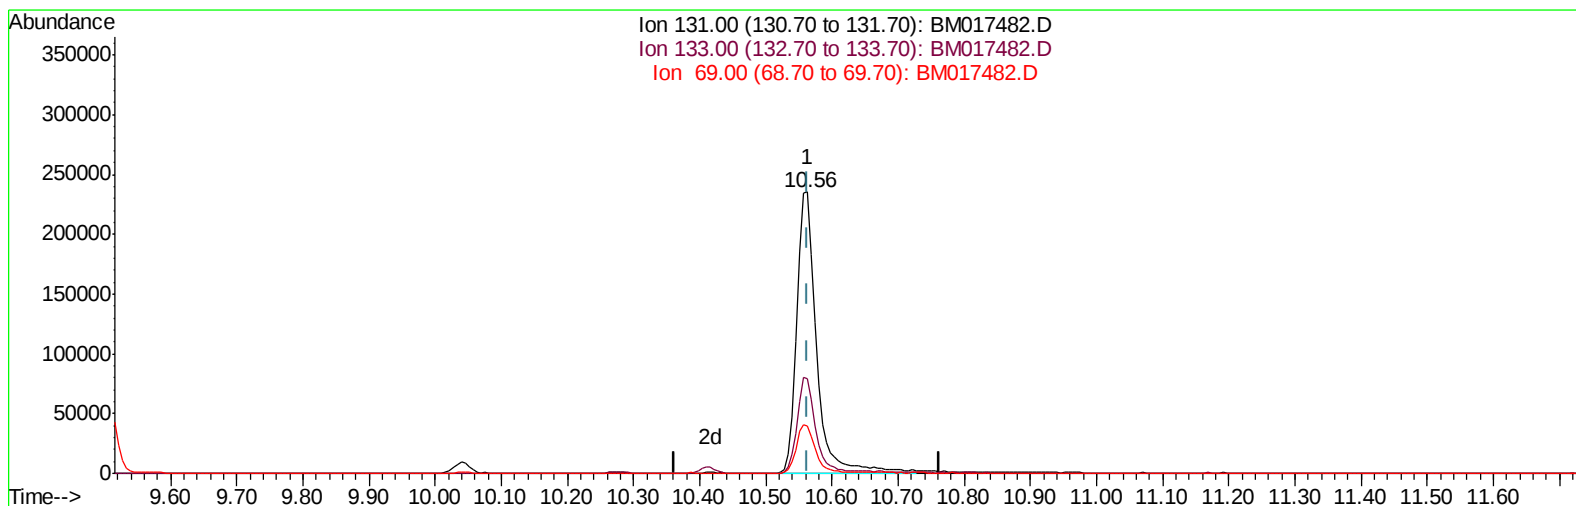

TIC: BM017482.D

(29) 4-Chloroaniline-d4 (S)

10.563min (0.000) 31.04ng/ul m

response 500037

Ion	Exp%	Act%
131.00	100	100
133.00	33.60	33.69
69.00	17.60	17.06
0.00	0.00	0.00