
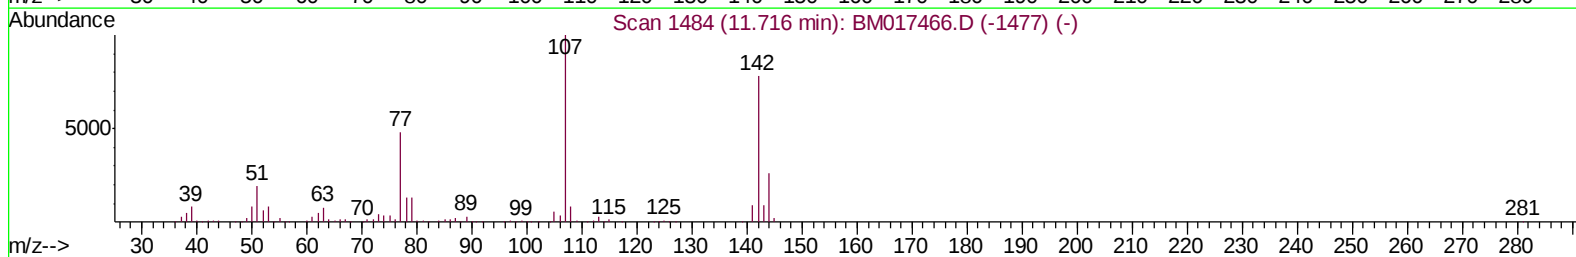
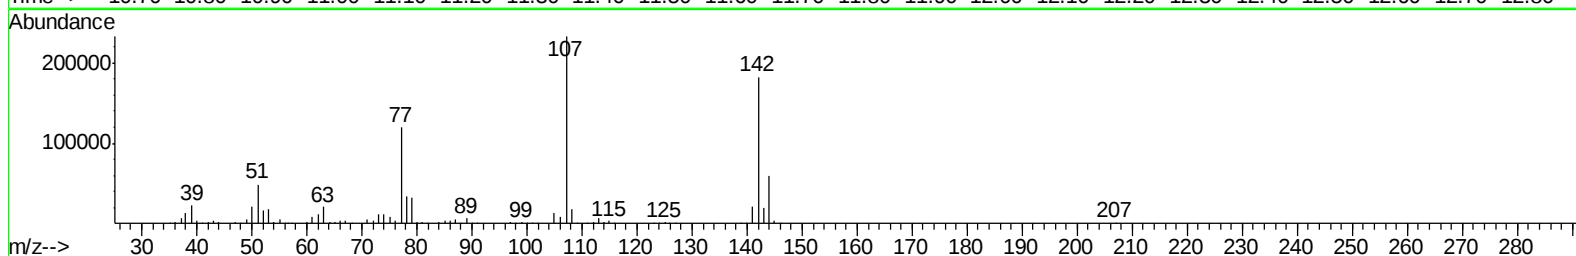


Data File : BM017482.D
Acq On : 02 Nov 2018 01:14
Operator : MJ/SJ
Sample : J5657-17MS
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Nov 02 04:23:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 02 02:41:22 2018
Response via : Initial Calibration

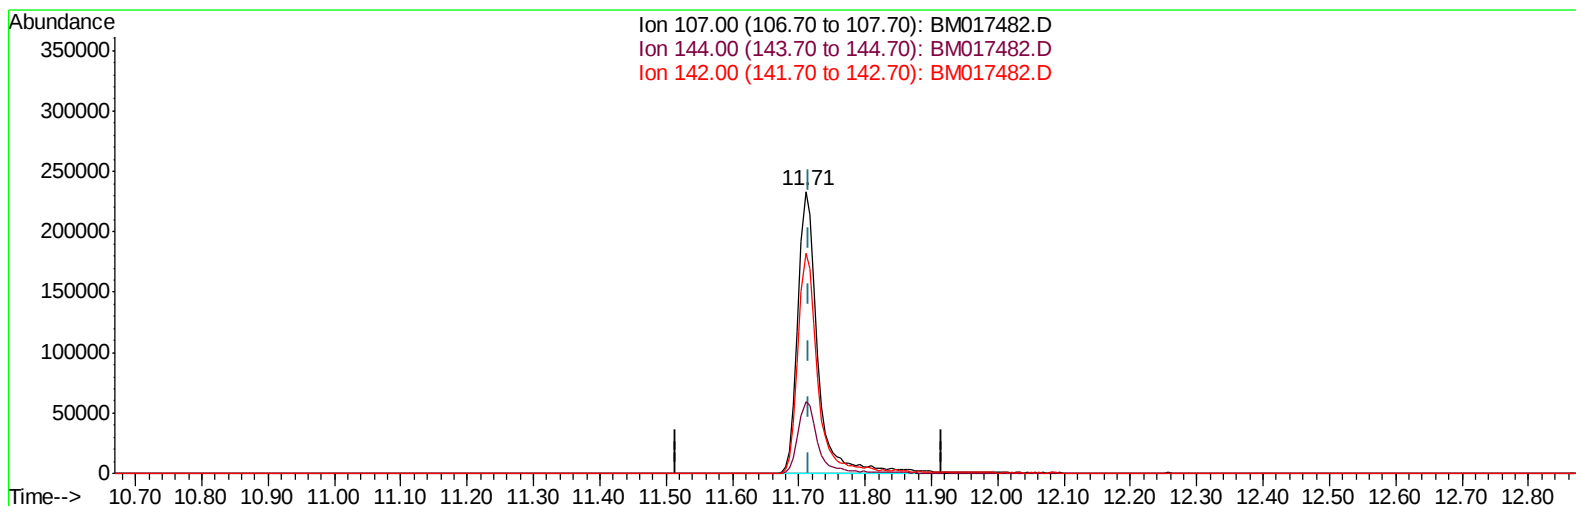

TIC: BM017482.D

(33) 4-Chloro-3-methylphenol (C)

11.710min (-0.006) 22.69ng/ul m

response 471688

Ion	Exp%	Act%
107.00	100	100
144.00	27.20	25.26
142.00	81.20	78.34
0.00	0.00	0.00