

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110118\
 Data File : BM017461.D
 Acq On : 01 Nov 2018 12:30
 Operator : MJ/SJ
 Sample : J5701-21MS
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A40K4MS

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	36	39	44	rBV	22726	31038	0.62%	0.044%
2	3.493	84	86	94	rBV	13659	25700	0.51%	0.036%
3	3.658	110	114	117	rBV6	4638	6325	0.13%	0.009%
4	3.823	136	142	149	rBV2	19597	36836	0.73%	0.052%
5	3.917	153	158	162	rBV4	6184	8974	0.18%	0.013%
6	4.134	191	195	198	rVB6	5449	7260	0.14%	0.010%
7	4.817	305	311	320	rBV2	106788	170671	3.38%	0.241%
8	6.828	645	653	654	rBV	513975	789330	15.64%	1.116%
9	6.846	654	656	669	rVV	673920	1031015	20.43%	1.458%
10	6.987	673	680	690	rVV	423569	653205	12.94%	0.924%
11	7.175	705	712	715	rBV	512505	858684	17.01%	1.214%
12	7.211	715	718	725	rVV	527321	809669	16.04%	1.145%
13	7.258	725	726	735	rVB6	12744	18138	0.36%	0.026%
14	7.640	785	791	794	rBV	758431	1209222	23.96%	1.710%
15	7.675	794	797	810	rVB	648136	999029	19.80%	1.413%
16	7.852	822	827	832	rBV4	3810	7349	0.15%	0.010%
17	7.905	832	836	842	rVB5	3320	7697	0.15%	0.011%
18	8.352	906	912	921	rBV	514107	879164	17.42%	1.243%
19	8.446	921	928	939	rVV	580094	918346	18.20%	1.299%
20	8.563	946	948	952	rVB5	4345	6864	0.14%	0.010%
21	8.793	981	987	999	rBV	547240	923053	18.29%	1.305%
22	8.916	1004	1008	1013	rVB7	5525	8163	0.16%	0.012%
23	9.193	1050	1055	1062	rVB2	14572	22132	0.44%	0.031%
24	9.510	1102	1109	1120	rBV	441667	759538	15.05%	1.074%
25	10.046	1193	1200	1218	rBV	550978	1104876	21.89%	1.562%
26	10.281	1231	1240	1248	rBV	781109	1280415	25.37%	1.811%
27	10.416	1254	1263	1274	rBV	1181178	1958106	38.80%	2.769%
28	10.563	1279	1288	1313	rBV	495639	1050926	20.82%	1.486%
29	11.193	1389	1395	1400	rBV5	7624	15076	0.30%	0.021%
30	11.257	1400	1406	1409	rVB5	4694	8191	0.16%	0.012%
31	11.716	1476	1484	1501	rBV	559096	1243179	24.63%	1.758%
32	11.963	1519	1526	1531	rBV5	10690	21171	0.42%	0.030%
33	12.010	1531	1534	1541	rVB2	13085	21126	0.42%	0.030%
34	12.628	1635	1639	1644	rBV4	3726	7990	0.16%	0.011%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110118\
 Data File : BM017461.D
 Acq On : 01 Nov 2018 12:30
 Operator : MJ/SJ
 Sample : J5701-21MS
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A40K4MS

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
 Title : SVOA CALIBRATION

35	12.887	1680	1683	1688	rBV4	4280	7135	0.14%	0.010%
36	12.963	1691	1696	1700	rBV3	8527	12901	0.26%	0.018%
37	13.110	1714	1721	1727	rVB5	3531	7672	0.15%	0.011%
38	13.469	1777	1782	1784	rBV5	4200	6621	0.13%	0.009%
39	13.704	1815	1822	1826	rBV	1258642	1883691	37.32%	2.664%
40	13.751	1826	1830	1842	rVB	514713	771520	15.29%	1.091%
41	13.975	1860	1868	1881	rBV	1416973	2223387	44.06%	3.144%
42	14.287	1914	1921	1926	rBV2	1826655	2823027	55.94%	3.992%
43	14.345	1926	1931	1950	rVB	1681453	2618101	51.88%	3.702%
44	14.516	1953	1960	1979	rBV3	536496	1559650	30.90%	2.205%
45	14.669	1980	1986	1994	rBV	764821	1190499	23.59%	1.683%
46	15.122	2060	2063	2066	rBV	23351	28337	0.56%	0.040%
47	15.281	2083	2090	2106	rBV	1997024	3006850	59.58%	4.252%
48	15.410	2106	2112	2126	rVV	535441	859494	17.03%	1.215%
49	15.522	2128	2131	2136	rVV2	27363	41045	0.81%	0.058%
50	15.845	2181	2186	2187	rBV2	5450	7521	0.15%	0.011%
51	15.863	2187	2189	2196	rVB6	4348	7666	0.15%	0.011%
52	16.010	2209	2214	2220	rVV5	10830	20012	0.40%	0.028%
53	16.198	2241	2246	2248	rBV3	4706	7086	0.14%	0.010%
54	16.239	2250	2253	2256	rBV5	5861	7934	0.16%	0.011%
55	16.322	2263	2267	2270	rBV3	3449	6830	0.14%	0.010%
56	16.457	2287	2290	2293	rBV4	9316	11833	0.23%	0.017%
57	16.686	2323	2329	2340	rBV	849508	1263632	25.04%	1.787%
58	16.769	2340	2343	2347	rVV4	31454	44196	0.88%	0.062%
59	16.810	2347	2350	2357	rVB7	10455	24424	0.48%	0.035%
60	16.939	2368	2372	2374	rBV3	6283	7547	0.15%	0.011%
61	17.039	2381	2389	2399	rBV	2686292	3976956	78.80%	5.624%
62	17.133	2399	2405	2415	rVV2	2276958	3366568	66.71%	4.761%
63	17.222	2418	2420	2426	rVB6	10731	16161	0.32%	0.023%
64	17.333	2435	2439	2445	rVB6	5904	9173	0.18%	0.013%
65	17.428	2453	2455	2459	rBV5	9298	11839	0.23%	0.017%
66	17.545	2471	2475	2478	rBV5	8734	11383	0.23%	0.016%
67	17.657	2488	2494	2500	rVB	158906	202588	4.01%	0.286%
68	17.816	2516	2521	2527	rBV9	21811	40899	0.81%	0.058%
69	17.886	2529	2533	2535	rBV5	7792	10030	0.20%	0.014%
70	17.945	2537	2543	2552	rVV	356973	539442	10.69%	0.763%
71	18.010	2552	2554	2558	rVB2	16658	24371	0.48%	0.034%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110118\
 Data File : BM017461.D
 Acq On : 01 Nov 2018 12:30
 Operator : MJ/SJ
 Sample : J5701-21MS
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A40K4MS

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
 Title : SVOA CALIBRATION

72	18.110	2569	2571	2574	rVB4	11444	12022	0.24%	0.017%
73	18.239	2588	2593	2598	rVB8	14651	22187	0.44%	0.031%
74	18.375	2613	2616	2619	rBV5	10447	12959	0.26%	0.018%
75	18.422	2622	2624	2626	rBV3	5366	6384	0.13%	0.009%
76	18.475	2631	2633	2635	rBV3	6030	6522	0.13%	0.009%
77	18.498	2635	2637	2641	rVB5	7641	9630	0.19%	0.014%
78	18.604	2653	2655	2658	rBV4	5016	6960	0.14%	0.010%
79	18.698	2668	2671	2672	rBV3	7563	8683	0.17%	0.012%
80	18.810	2687	2690	2691	rBV3	7103	6517	0.13%	0.009%
81	18.875	2698	2701	2707	rVB8	18672	27736	0.55%	0.039%
82	19.104	2727	2740	2749	rBV2	158492	357919	7.09%	0.506%
83	19.227	2757	2761	2771	rBV3	126529	206344	4.09%	0.292%
84	19.351	2774	2782	2786	rVB2	32916	74697	1.48%	0.106%
85	19.439	2791	2797	2799	rVV2	2698771	4070320	80.65%	5.756%
86	19.463	2799	2801	2813	rVB	3048456	3924855	77.77%	5.550%
87	19.963	2882	2886	2890	rBV5	52174	83206	1.65%	0.118%
88	20.492	2974	2976	2980	rVB3	43399	43917	0.87%	0.062%
89	20.951	3051	3054	3062	rBV	389606	514930	10.20%	0.728%
90	21.157	3086	3089	3093	rBV	157390	170011	3.37%	0.240%
91	21.233	3096	3102	3112	rBV	3734596	5046766	100.00%	7.137%
92	21.392	3126	3129	3133	rVB	126449	144955	2.87%	0.205%
93	21.827	3199	3203	3213	rBV4	261051	523992	10.38%	0.741%
94	22.280	3276	3280	3286	rVB	286589	356200	7.06%	0.504%
95	22.404	3298	3301	3305	rVB	183058	236300	4.68%	0.334%
96	22.774	3360	3364	3369	rBV2	620511	897815	17.79%	1.270%
97	23.298	3447	3453	3467	rVB	1924118	4377889	86.75%	6.191%
98	23.439	3470	3477	3490	rVB	2239513	4337423	85.94%	6.133%
99	23.957	3560	3565	3571	rVB	516208	938029	18.59%	1.326%
100	24.686	3684	3689	3697	rVB2	344194	735719	14.58%	1.040%


Sum of corrected areas: 70717366

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110118\
Data File : BM017461.D
Acq On : 01 Nov 2018 12:30
Operator : MJ/SJ
Sample : J5701-21MS
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40K4MS

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

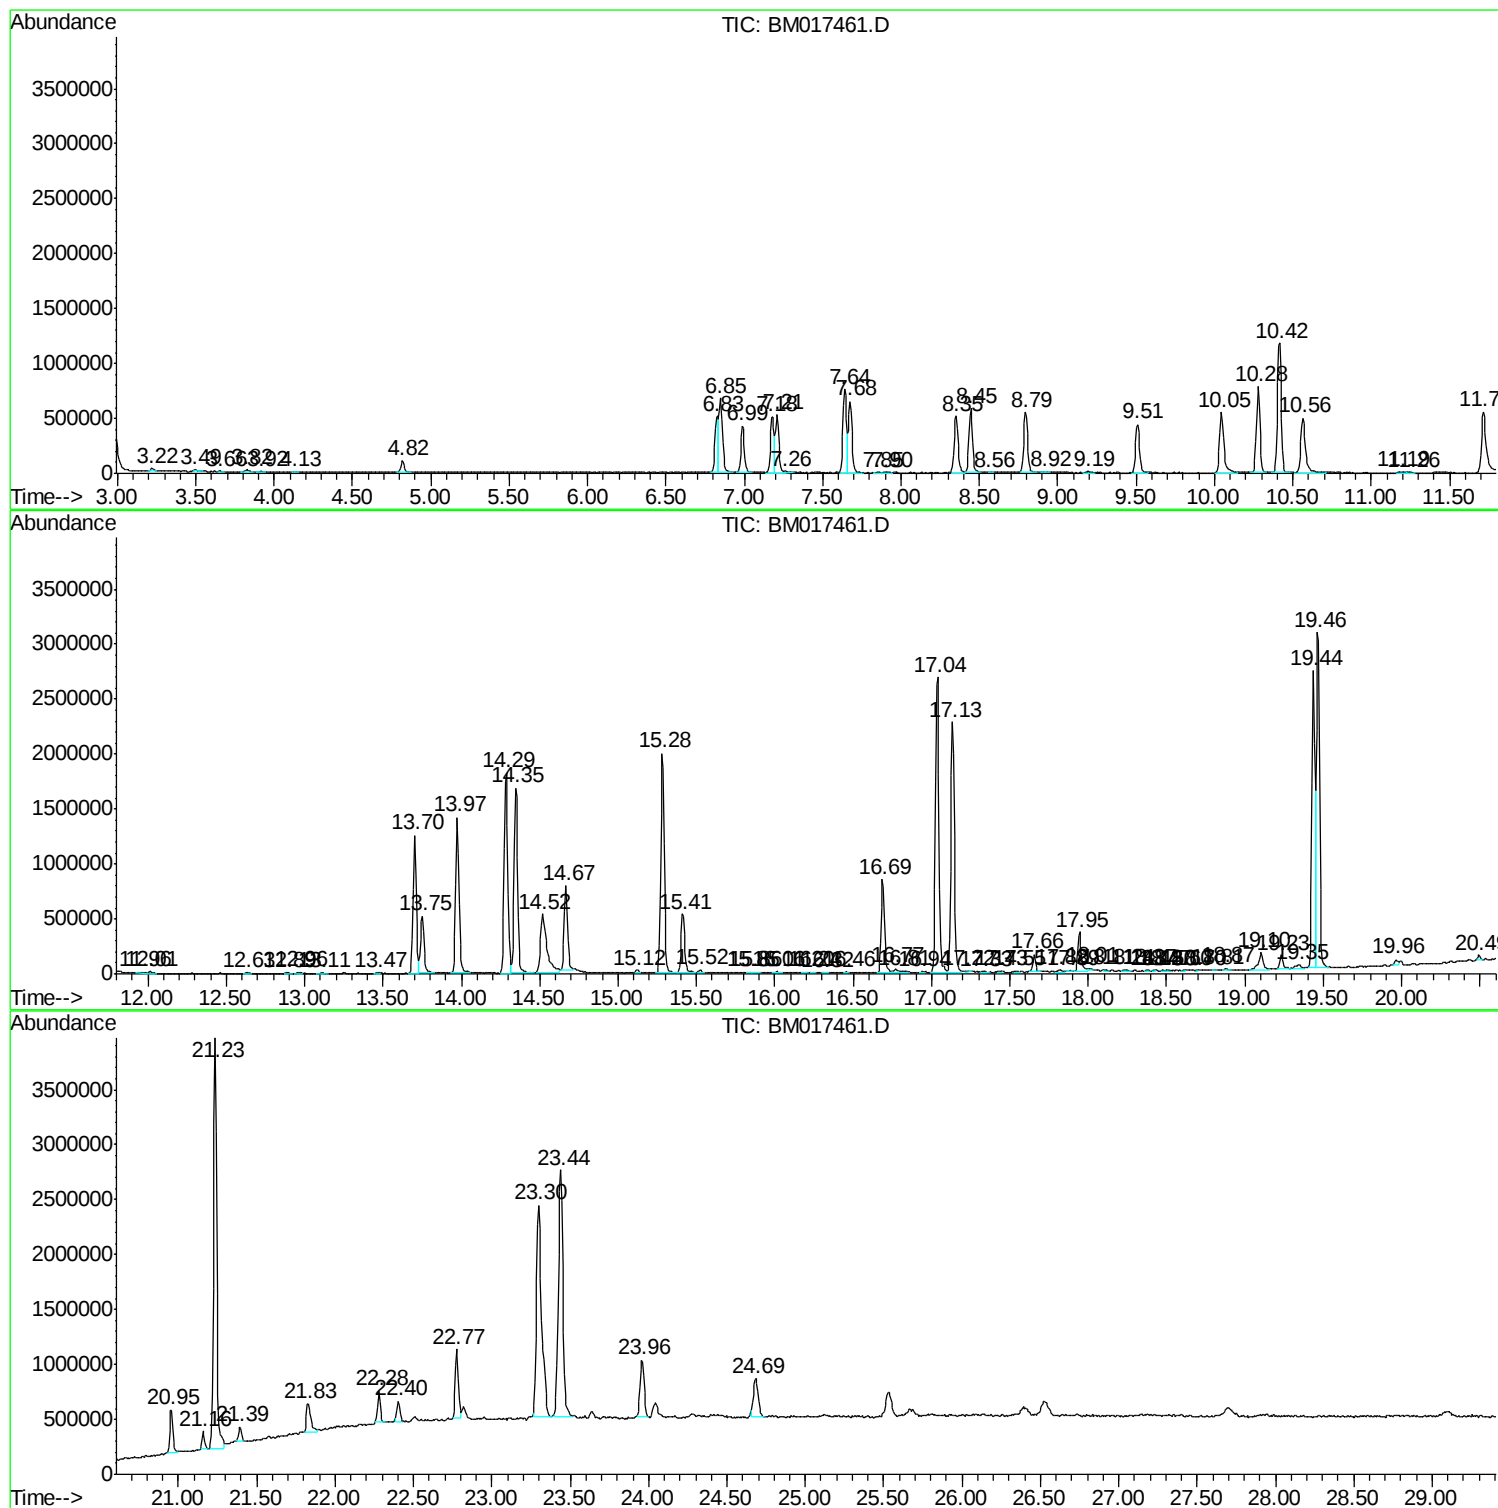

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110118\
Data_File : BM017461.D
Acq_On : 01_Nov_2018_12:300
Operator : MJ/SJJ
Sample : J5701-21MSS
Misc :
ALS_Vial : 6 Sample_Multiplier: 11

Instrument :
BNA_M
ClientSampleId :
A40K4MS

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.MM
Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
