


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110123\
Data File : BM042532.D
Acq On : 01 Nov 2023 10:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 31 02:55:18 2023

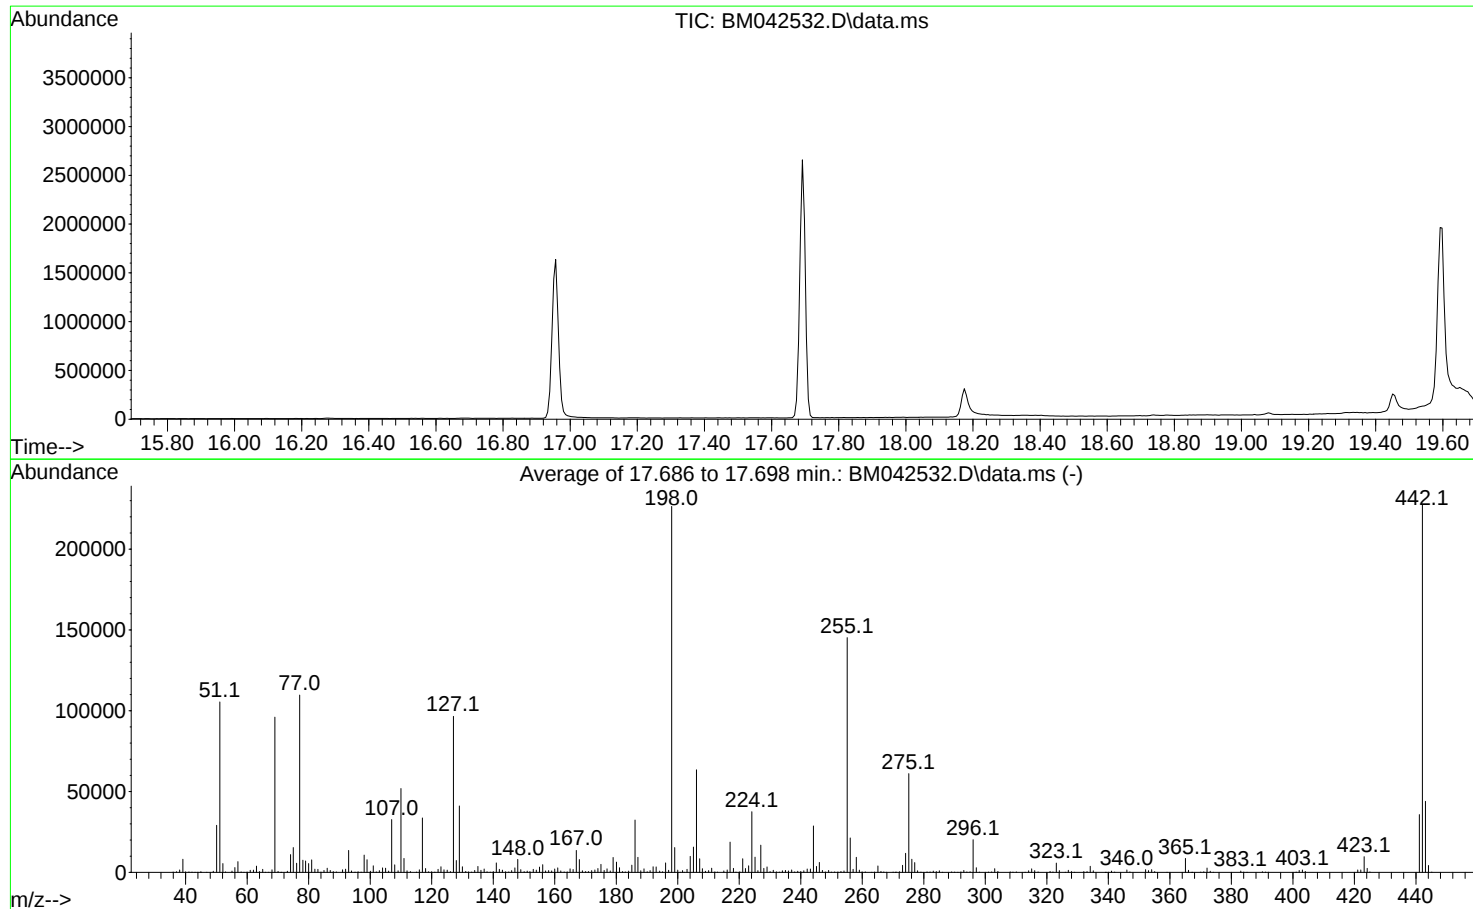




AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.6	105504	PASS
68	69	0.00	2	1.6	1566	PASS
69	198	0.00	100	42.4	96085	PASS
70	69	0.00	2	0.6	570	PASS
127	198	10	80	42.6	96560	PASS
197	198	0.00	2	0.6	1297	PASS
198	198	100	100	100.0	226453	PASS
199	198	5	9	6.8	15396	PASS
275	198	10	60	27.0	61072	PASS
365	198	1	100	3.8	8584	PASS
441	198	0.01	100	15.8	35760	PASS
442	442	50	100	100.0	227648	PASS
443	442	15	24	19.3	43939	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110123\
Data File : BM042532.D
Acq On : 01 Nov 2023 10:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 02 00:57:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 31 02:55:18 2023
Response via : Initial Calibration

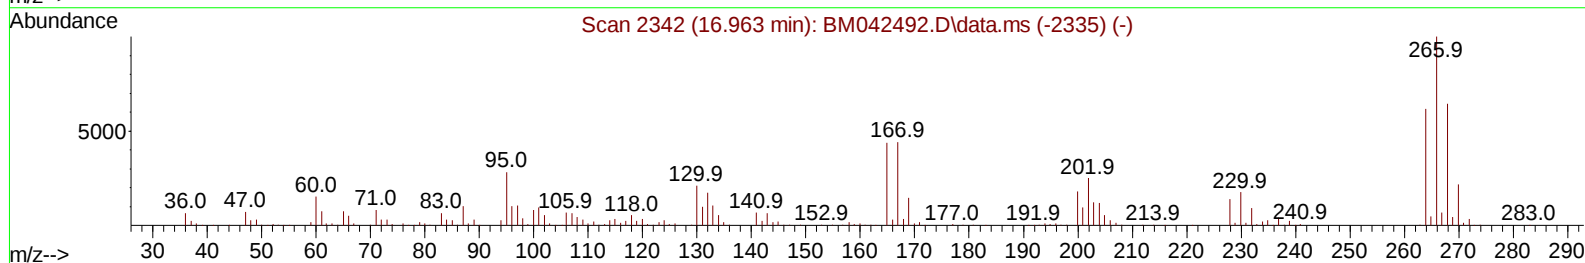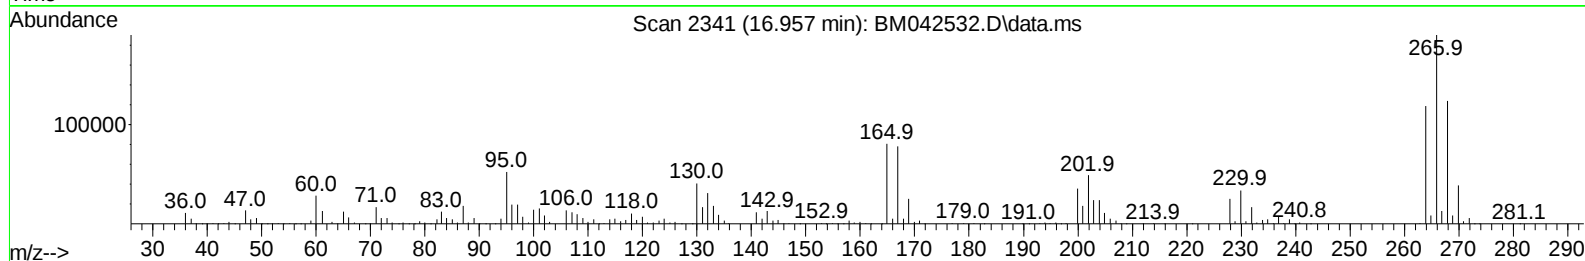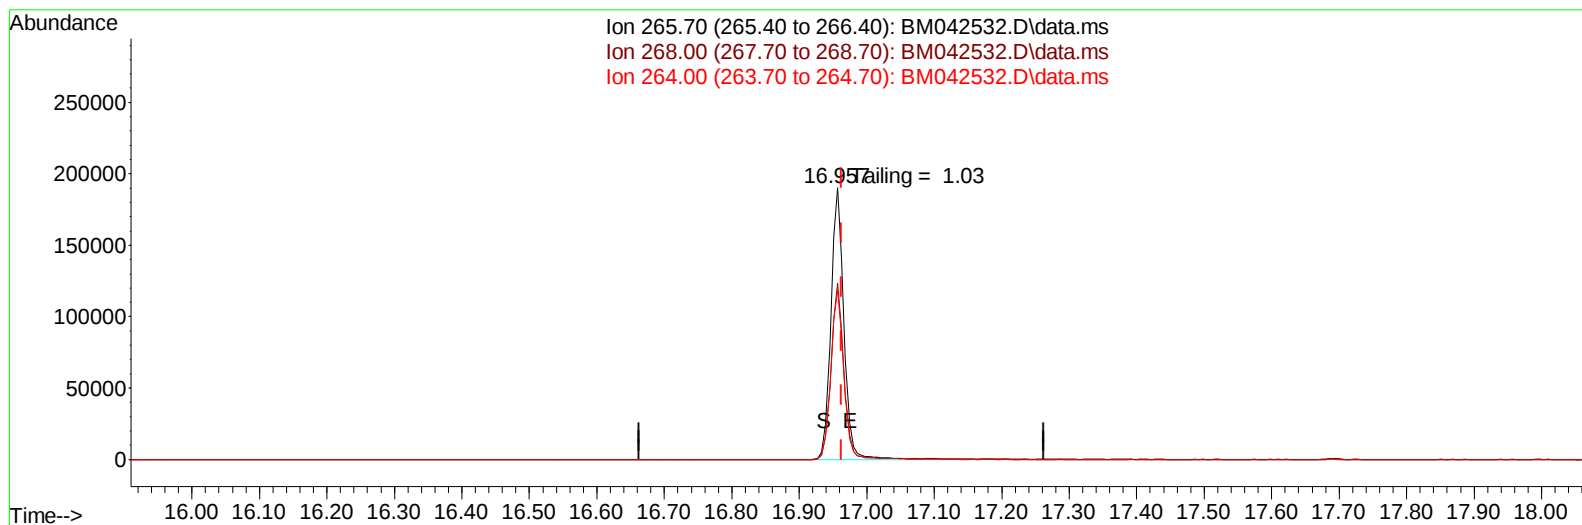

TIC: BM042532.D\data.ms

(70) Pentachlorophenol (C)

16.957min (-0.006) 0.00 ng




response 255258

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	64.96
264.00	61.80	62.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110123\
Data File : BM042532.D
Acq On : 01 Nov 2023 10:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 02 00:57:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 31 02:55:18 2023
Response via : Initial Calibration

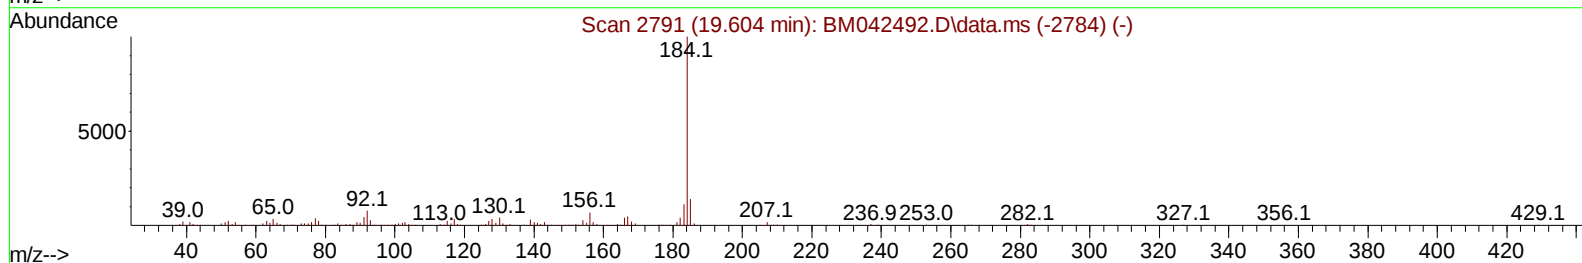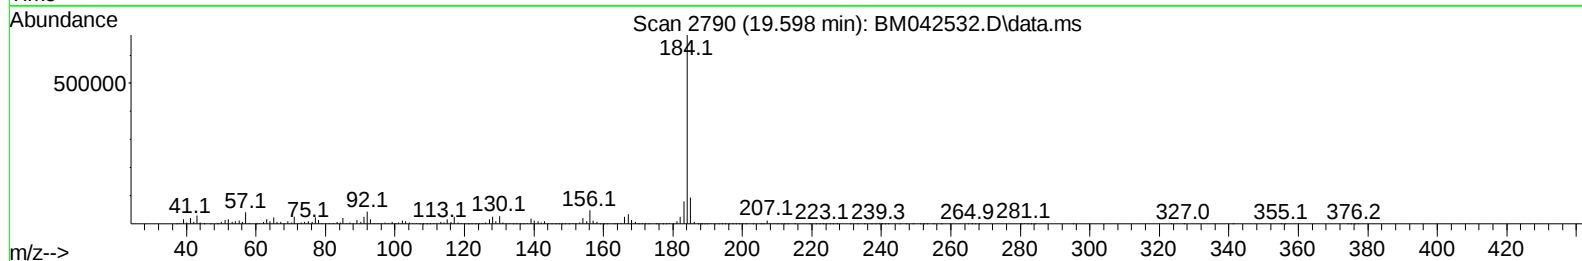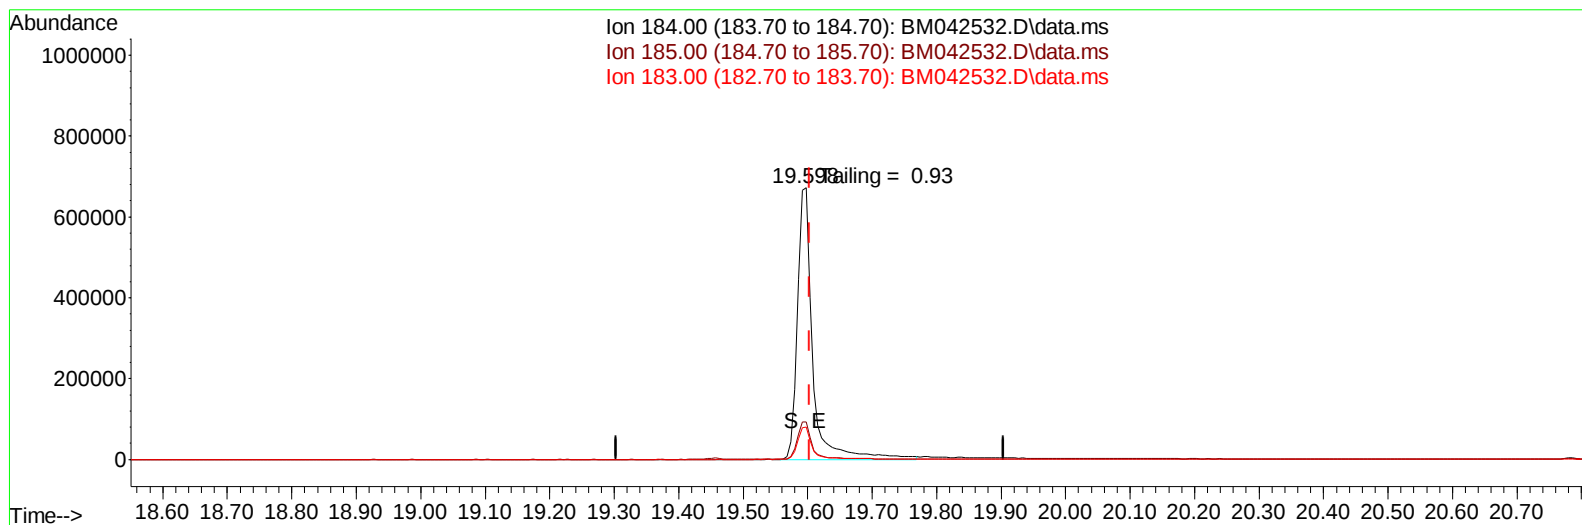

TIC: BM042532.D\data.ms

(77) Benzidine

19.598min (-0.006) 177644.94 ng

response 1111021

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.83
183.00	11.20	11.95
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/1/2023	BNA_M	<u>BM042532.D</u>
Compound Name	Response	Retention Time
DDT	756165	20.78
DDD	11282	20.392
DDE	501	19.833
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11783	767948	1.53

Instrument :
BNA_M
ClientSampleId :
DFTPP