
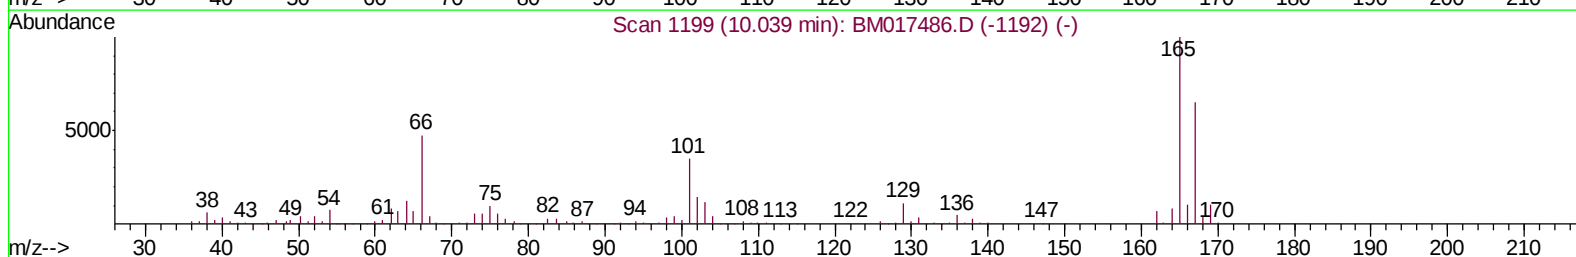
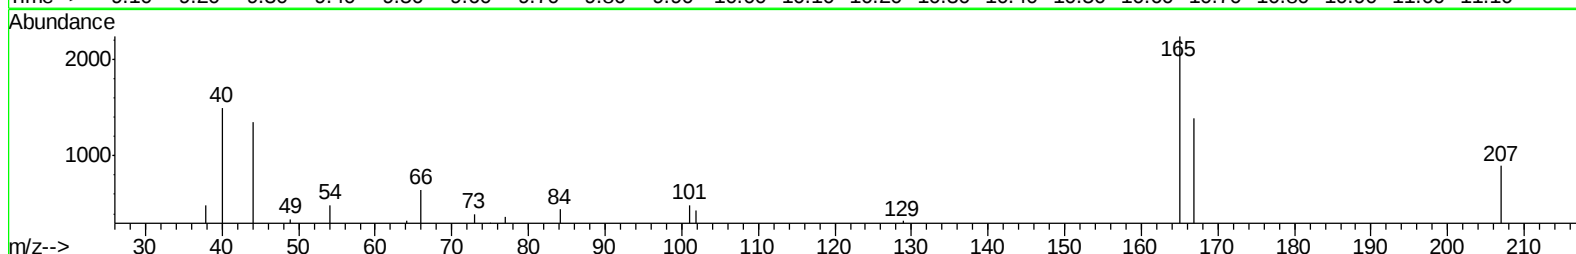


Data File : BM017490.D
Acq On : 02 Nov 2018 10:52
Operator : MJ/SJ
Sample : J5701-13MEDL 30X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Nov 03 02:33:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 02:25:47 2018
Response via : Initial Calibration

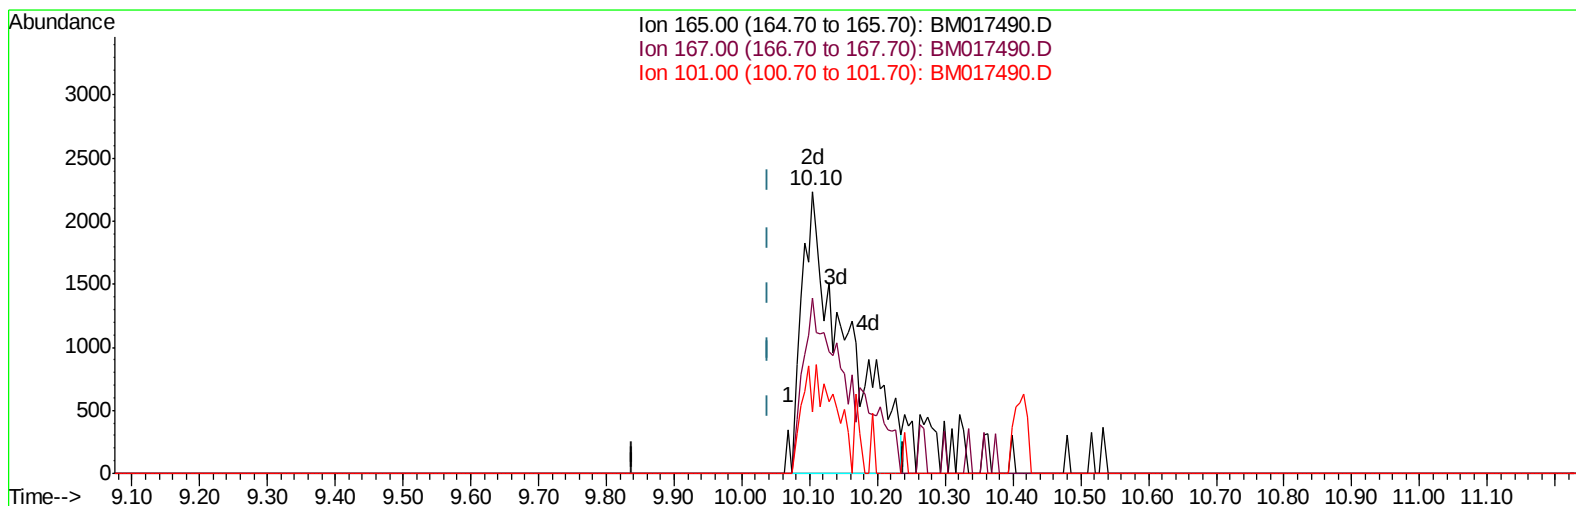

TIC: BM017490.D

(26) 2,4-Dichlorophenol-d3 (S)

10.104min (+0.065) 0.65ng/ul m

response 10191

Ion	Exp%	Act%
165.00	100	100
167.00	63.60	62.07
101.00	34.30	21.99#
0.00	0.00	0.00