
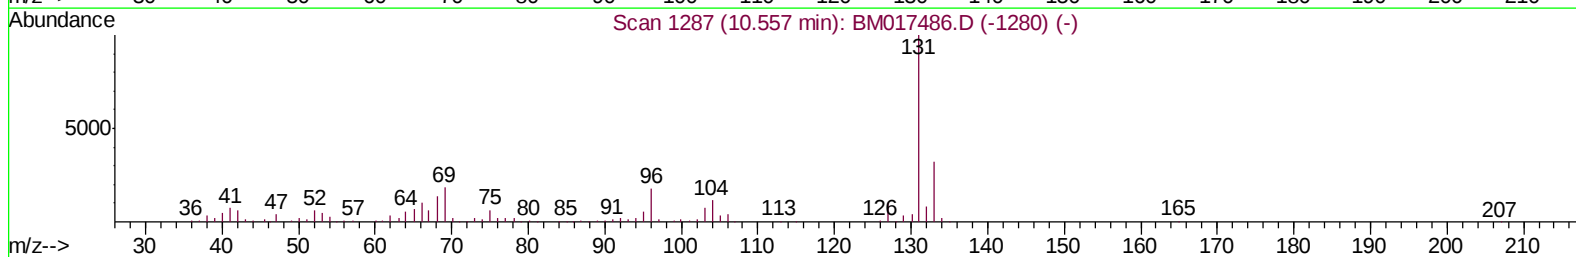
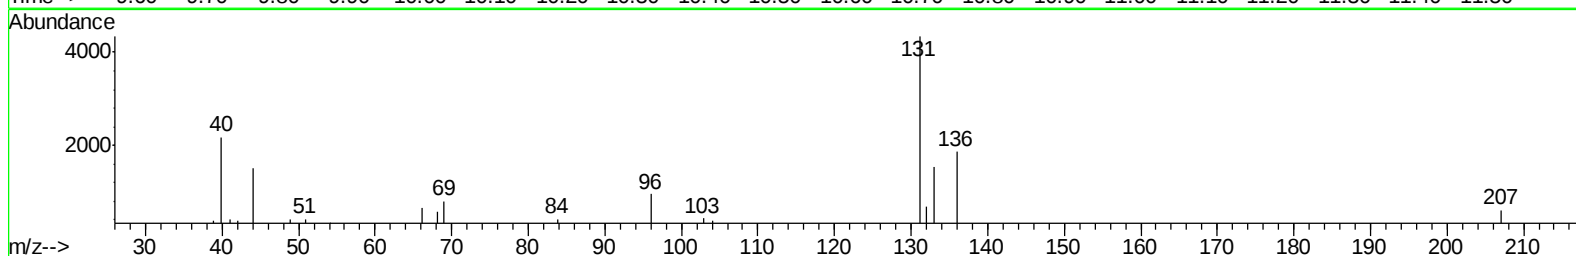


Data File : BM017490.D
Acq On : 02 Nov 2018 10:52
Operator : MJ/SJ
Sample : J5701-13MEDL 30X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Nov 03 02:33:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 02:25:47 2018
Response via : Initial Calibration

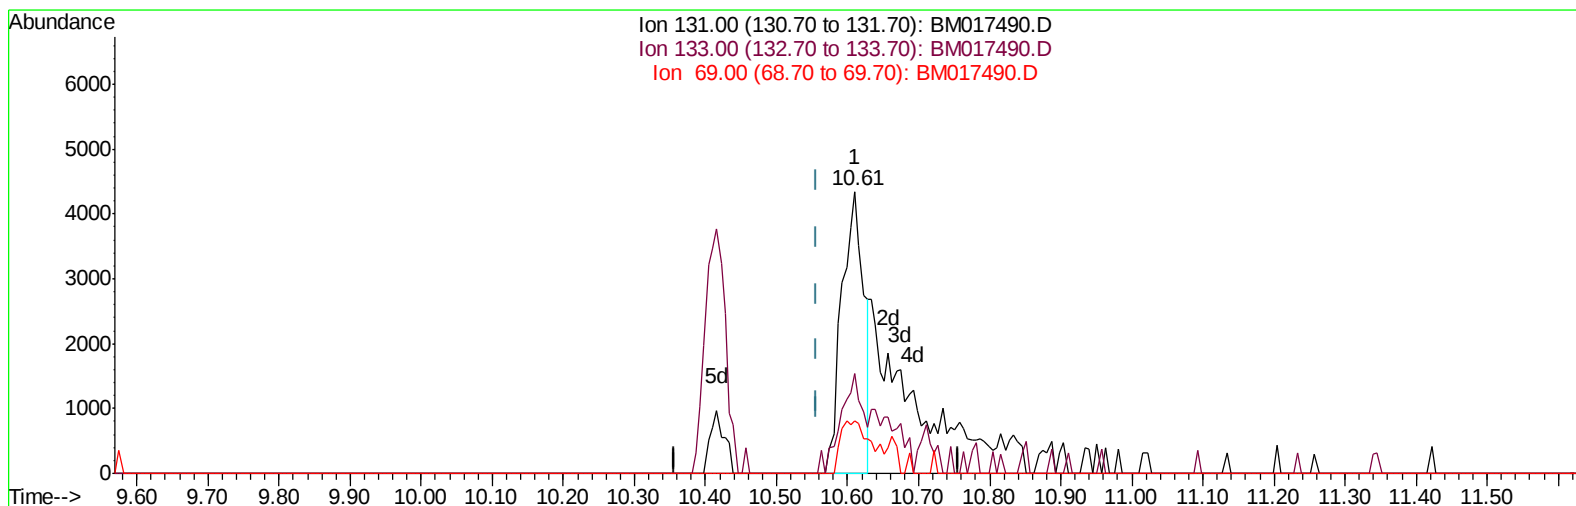

TIC: BM017490.D

(29) 4-Chloroaniline-d4 (S)
10.610min (+0.053) 0.73ng/ul
response 9354

Ion	Exp%	Act%
131.00	100	100
133.00	33.60	35.47
69.00	17.60	18.56
0.00	0.00	0.00