
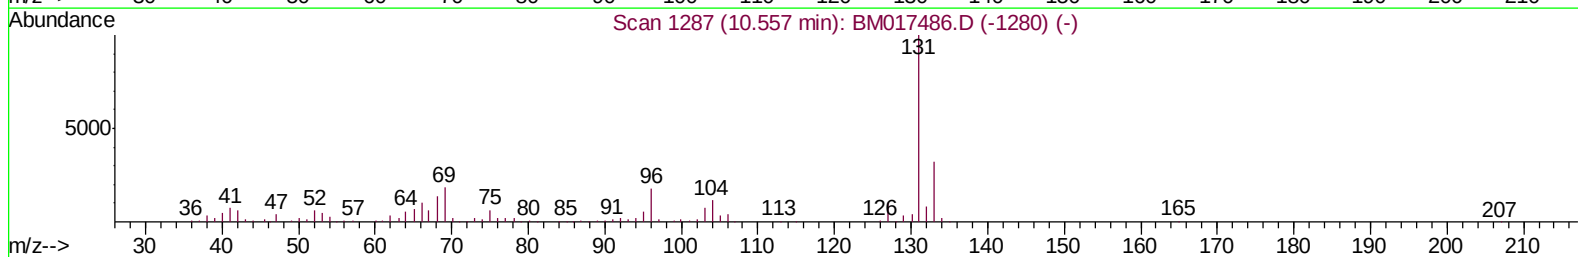
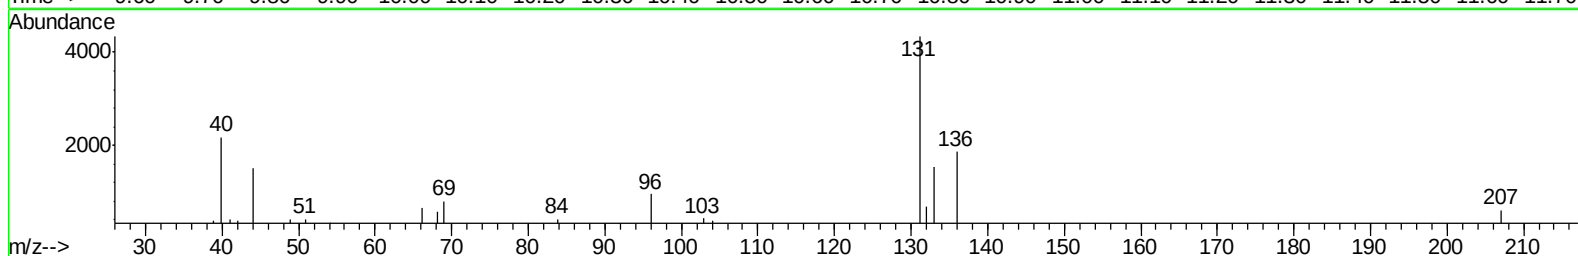


Data File : BM017490.D  
Acq On : 02 Nov 2018 10:52  
Operator : MJ/SJ  
Sample : J5701-13MEDL 30X  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Nov 03 02:33:35 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM102418MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Sat Nov 03 02:25:47 2018  
Response via : Initial Calibration

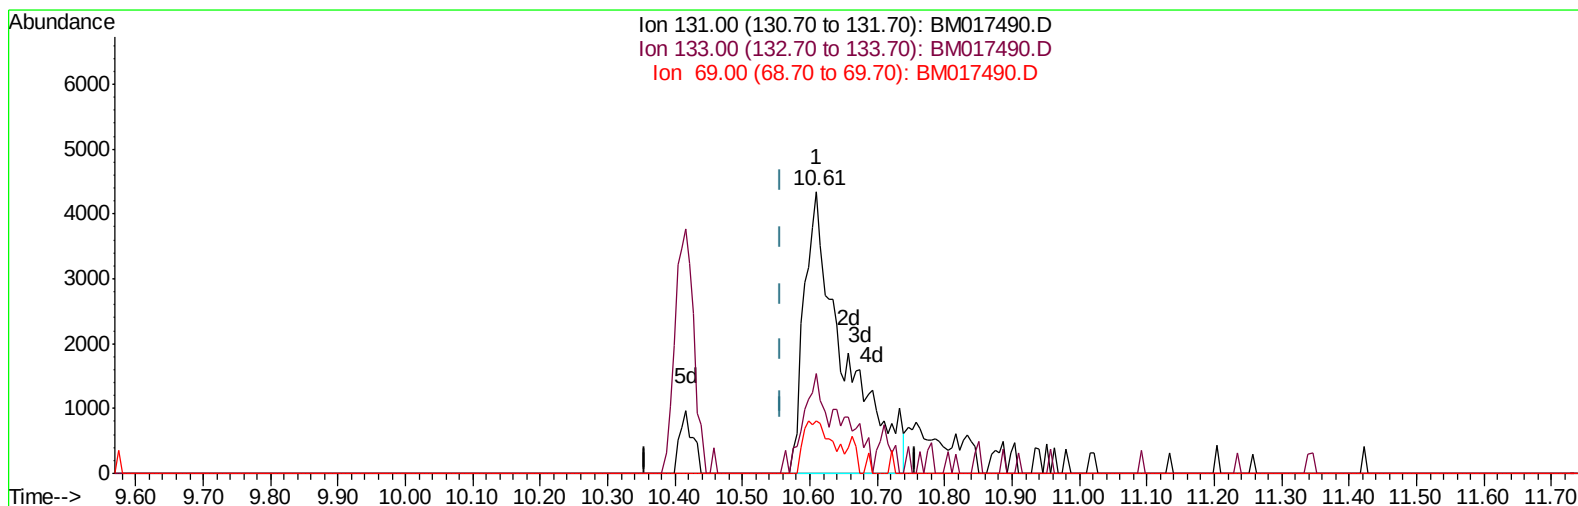

TIC: BM017490.D

(29) 4-Chloroaniline-d4 (S)

10.610min (+0.053) 1.40ng/ul m

response 17851

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 131.00 | 100   | 100   |
| 133.00 | 33.60 | 35.47 |
| 69.00  | 17.60 | 18.56 |
| 0.00   | 0.00  | 0.00  |