
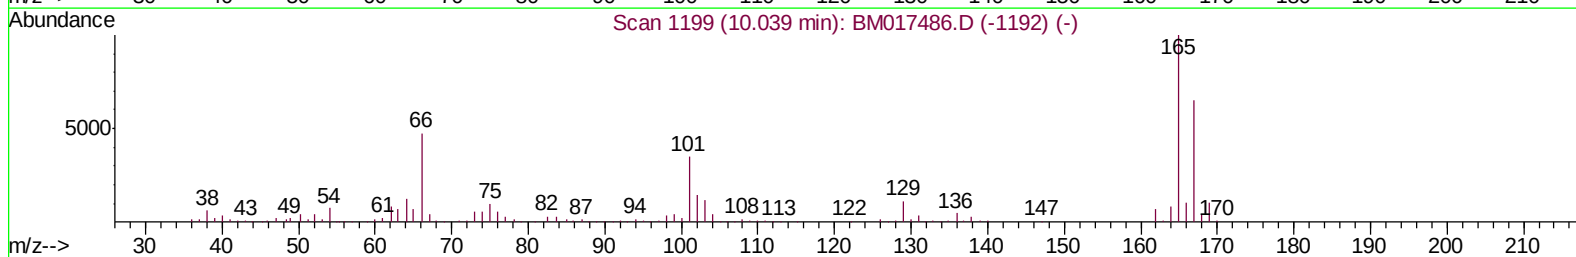
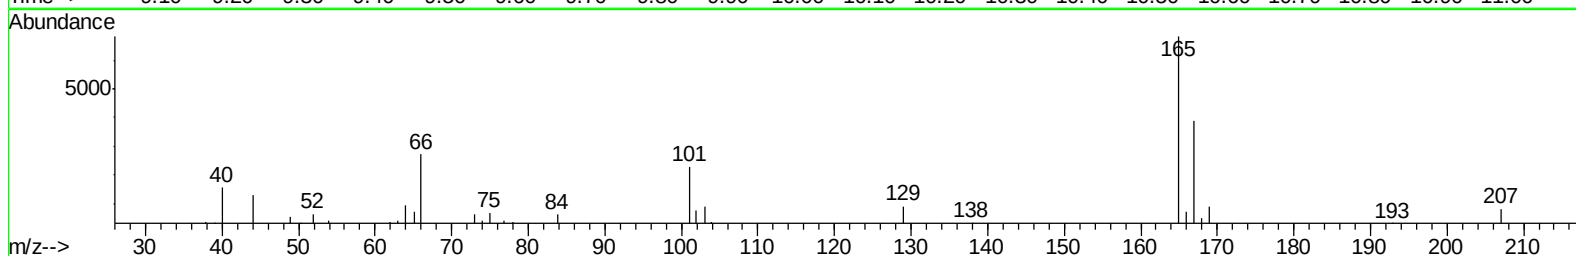


Data File : BM017491.D  
Acq On : 02 Nov 2018 11:29  
Operator : MJ/SJ  
Sample : J5701-16MEDL 10X  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Nov 03 02:33:44 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM102418MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Sat Nov 03 02:25:47 2018  
Response via : Initial Calibration

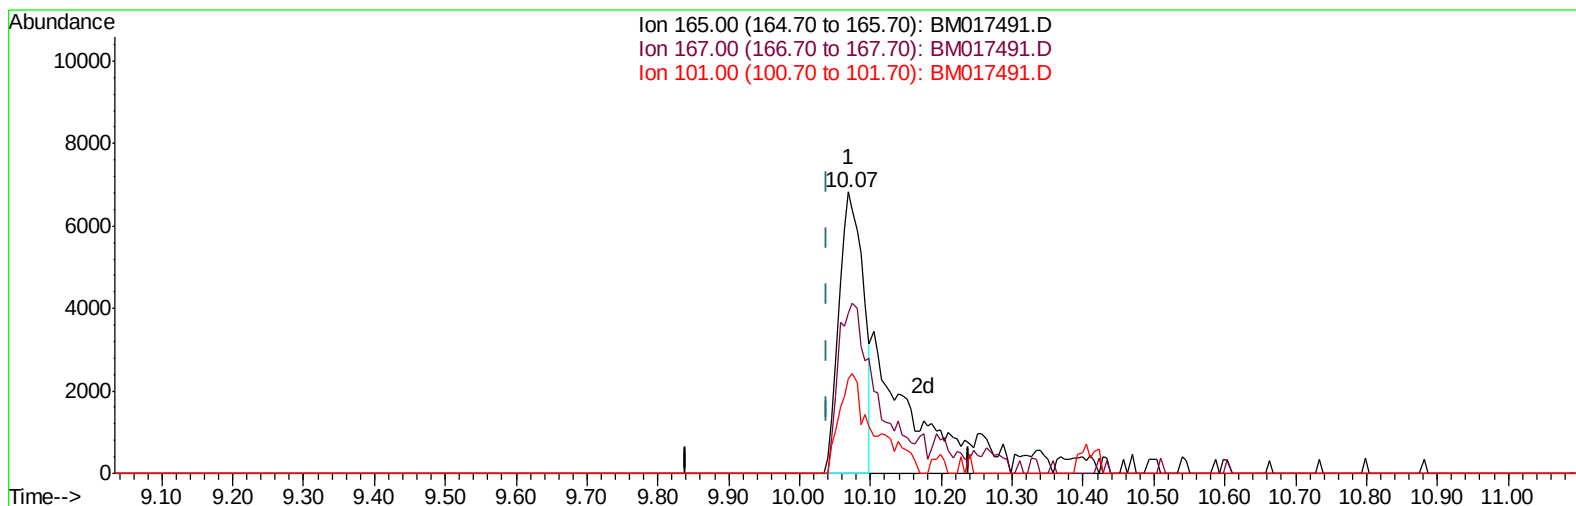

TIC: BM017491.D

(26) 2,4-Dichlorophenol-d3 (S)

10.069min (+0.030) 1.04ng/ul

response 16481

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 165.00 | 100   | 100   |
| 167.00 | 63.60 | 57.01 |
| 101.00 | 34.30 | 33.59 |
| 0.00   | 0.00  | 0.00  |