
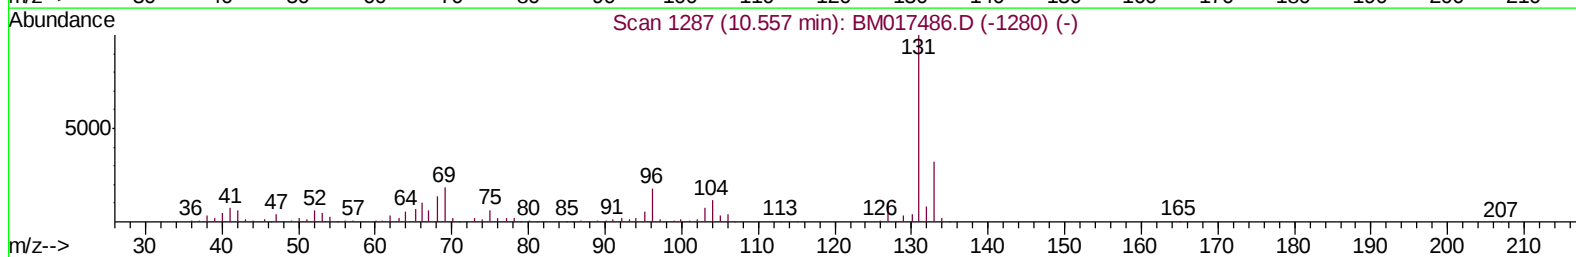
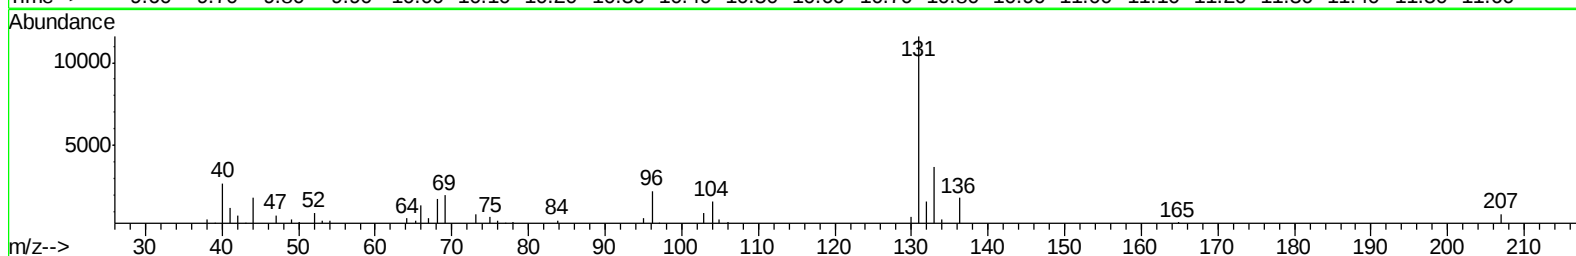


Data File : BM017491.D
Acq On : 02 Nov 2018 11:29
Operator : MJ/SJ
Sample : J5701-16MEDL 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Nov 03 02:33:44 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 02:25:47 2018
Response via : Initial Calibration

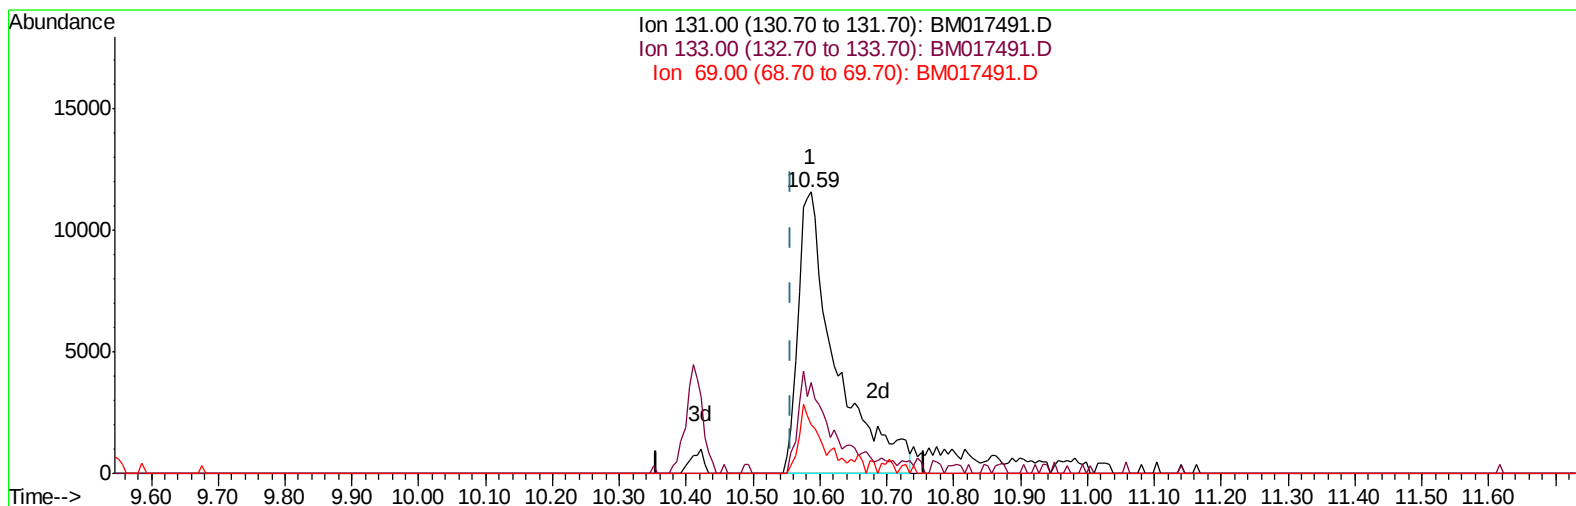

TIC: BM017491.D

(29) 4-Chloroaniline-d4 (S)

10.587min (+0.030) 3.49ng/ul m

response 45316

Ion	Exp%	Act%
131.00	100	100
133.00	33.60	32.13
69.00	17.60	17.24
0.00	0.00	0.00