

Data File : BM017493.D

Acq On : 02 Nov 2018 12:59

Operator : MJ/SJ

Sample : J5701-16MEDL 100X

Misc :

ALS Vial : 9 Sample Multiplier: 1




Quant Time: Nov 03 02:33:59 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Sat Nov 03 02:25:47 2018

Response via : Initial Calibration

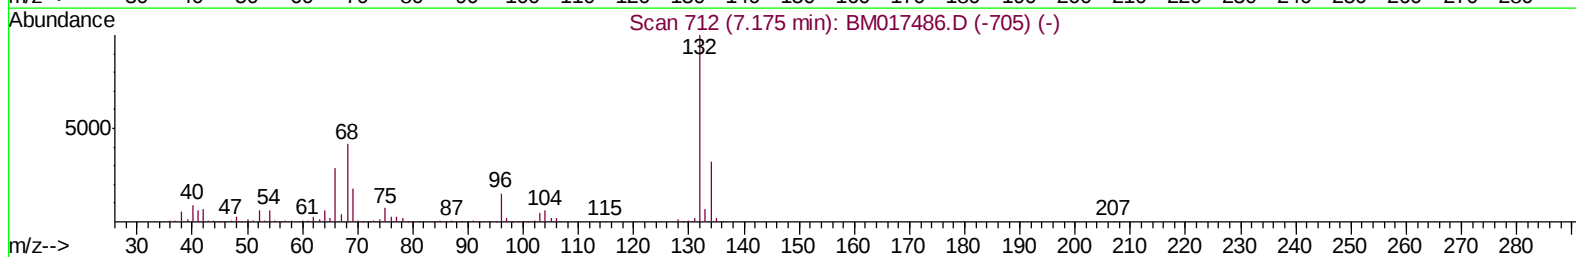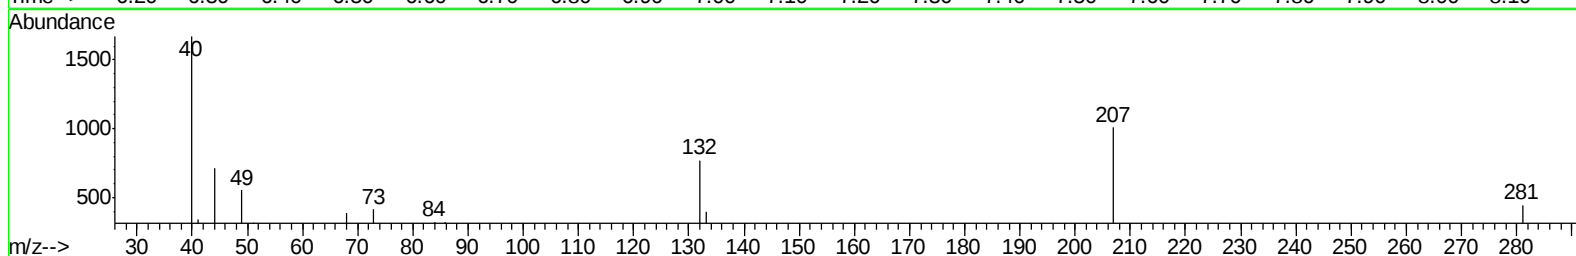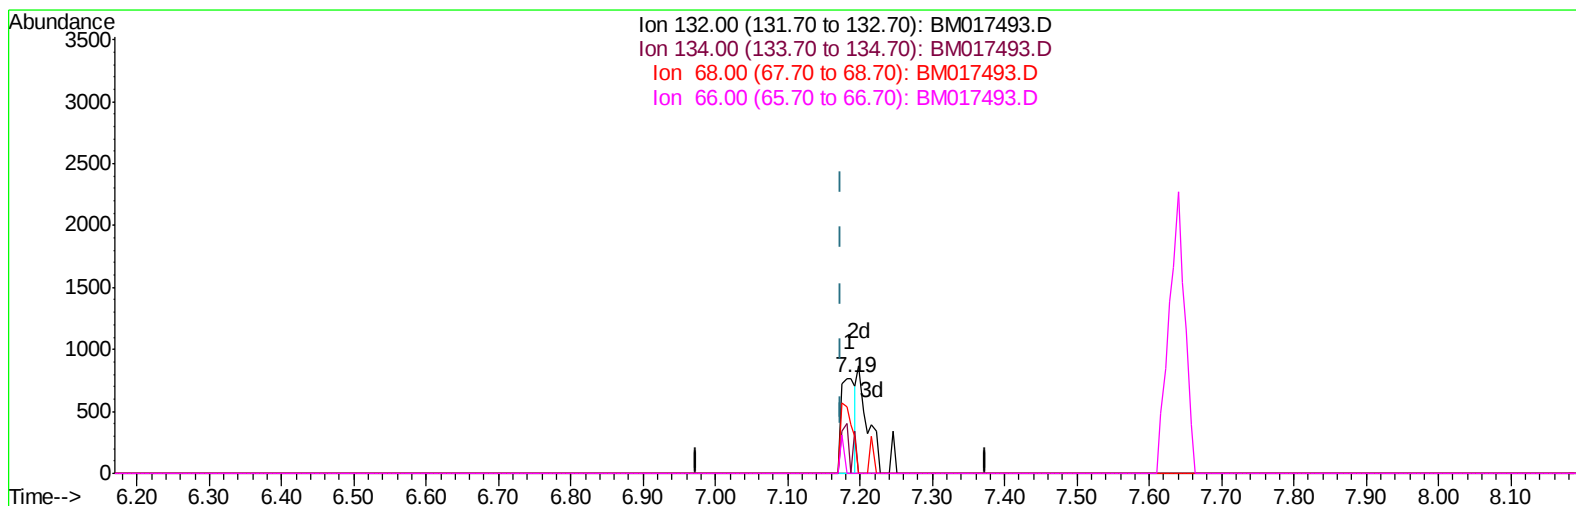

TIC: BM017493.D

(9) 2-Chlorophenol-d4 (S)

7.187min (+0.012) 0.08ng/ul

response 1043

Ion	Exp%	Act%
132.00	100	100
134.00	32.10	0.00#
68.00	39.20	50.85#
66.00	26.90	0.00#