
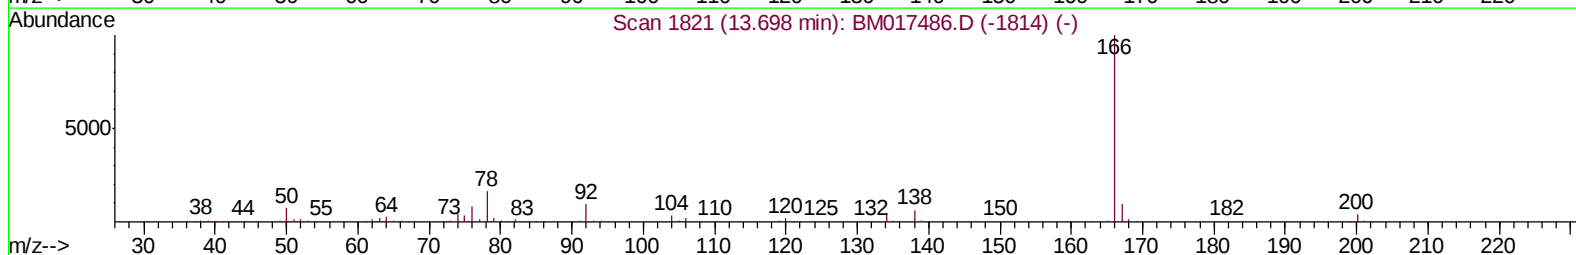
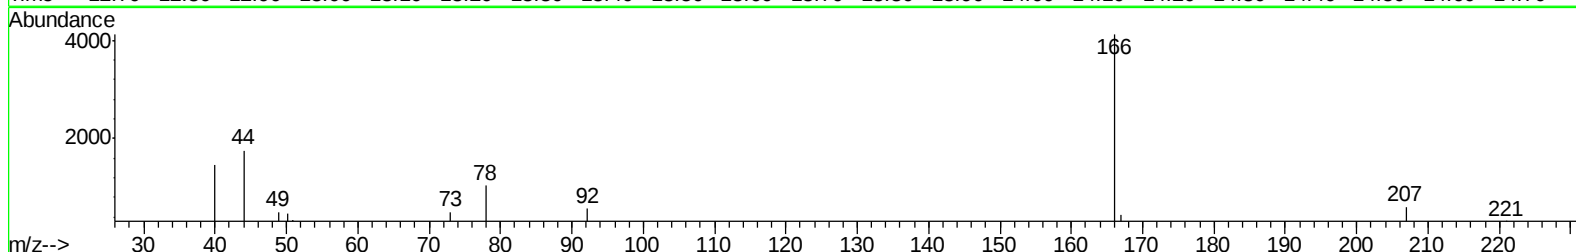


Data File : BM017493.D
Acq On : 02 Nov 2018 12:59
Operator : MJ/SJ
Sample : J5701-16MEDL 100X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Nov 03 02:33:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 02:25:47 2018
Response via : Initial Calibration

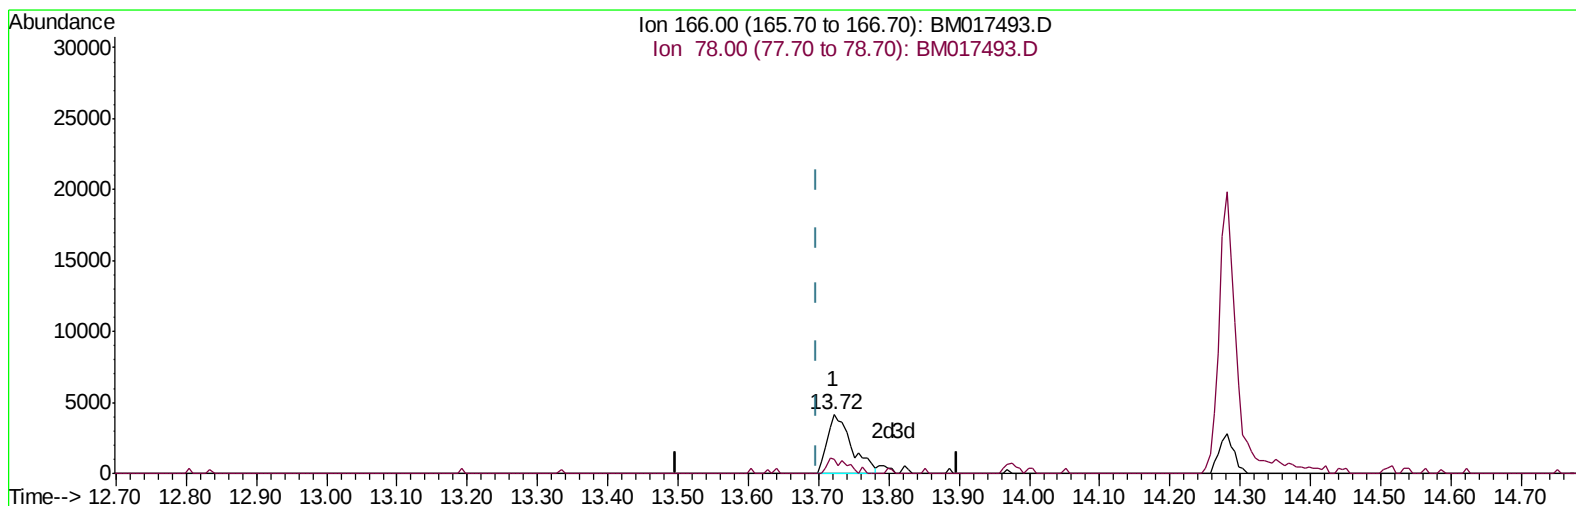

TIC: BM017493.D

(44) Dimethylphthalate-d6 (S)

13.722min (+0.024) 0.21ng/ul m

response 9793

Ion	Exp%	Act%
166.00	100	100
78.00	16.40	25.12#
0.00	0.00	0.00
0.00	0.00	0.00