
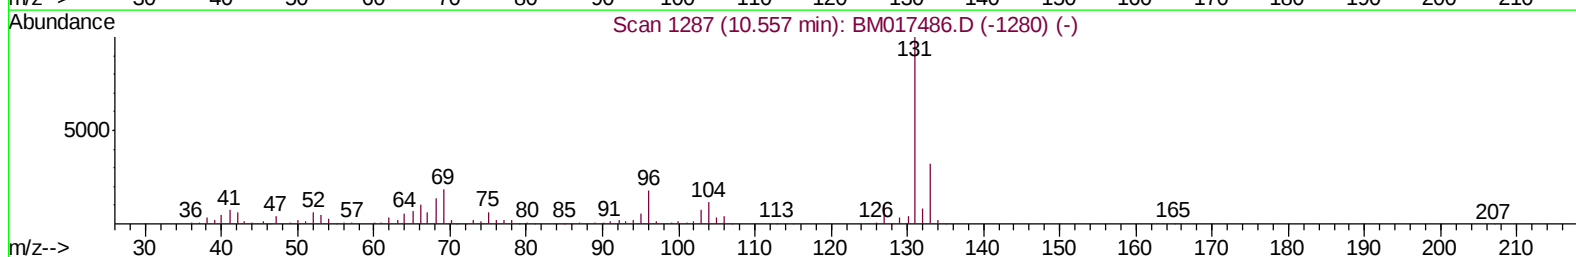
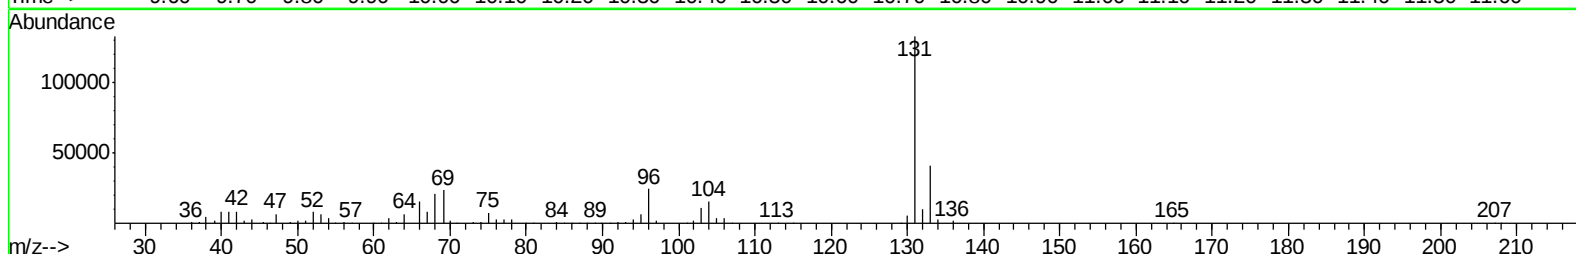


Data File : BM017494.D
Acq On : 02 Nov 2018 13:35
Operator : MJ/SJ
Sample : J5701-17
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Nov 03 02:34:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 02:25:47 2018
Response via : Initial Calibration

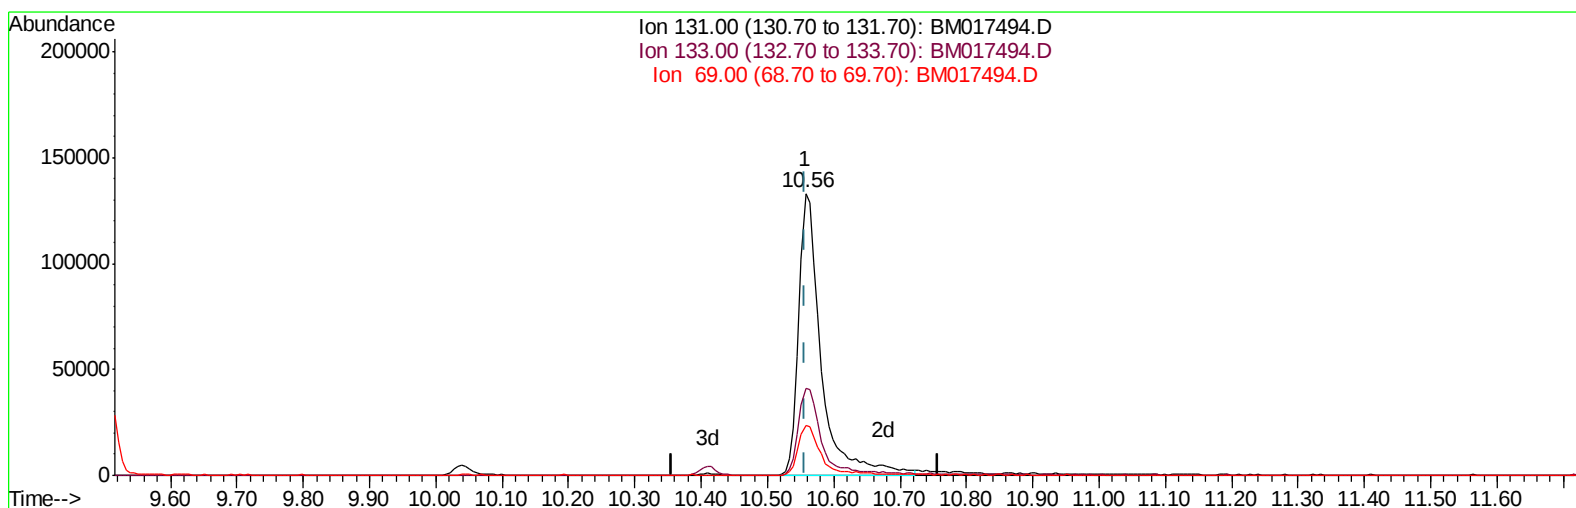

TIC: BM017494.D

(29) 4-Chloroaniline-d4 (S)
10.557min (+0.000) 22.50ng/ul m
response 306597

Ion	Exp%	Act%
131.00	100	100
133.00	33.60	30.90
69.00	17.60	17.90
0.00	0.00	0.00