
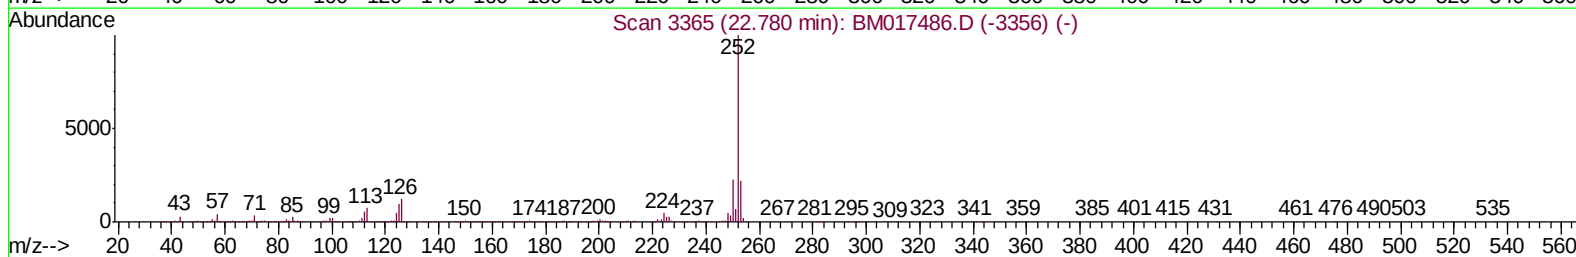
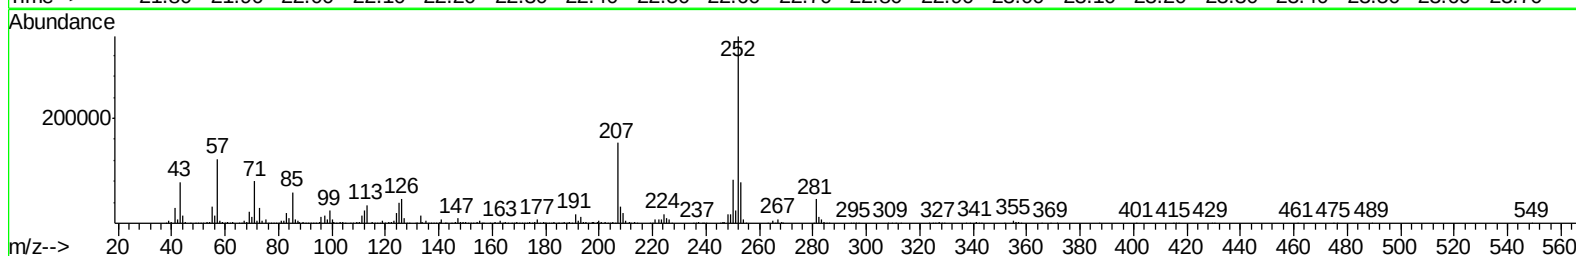


Data File : BM017496.D
Acq On : 02 Nov 2018 18:49
Operator : MJ/SJ
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Nov 03 02:34:27 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 02:25:47 2018
Response via : Initial Calibration

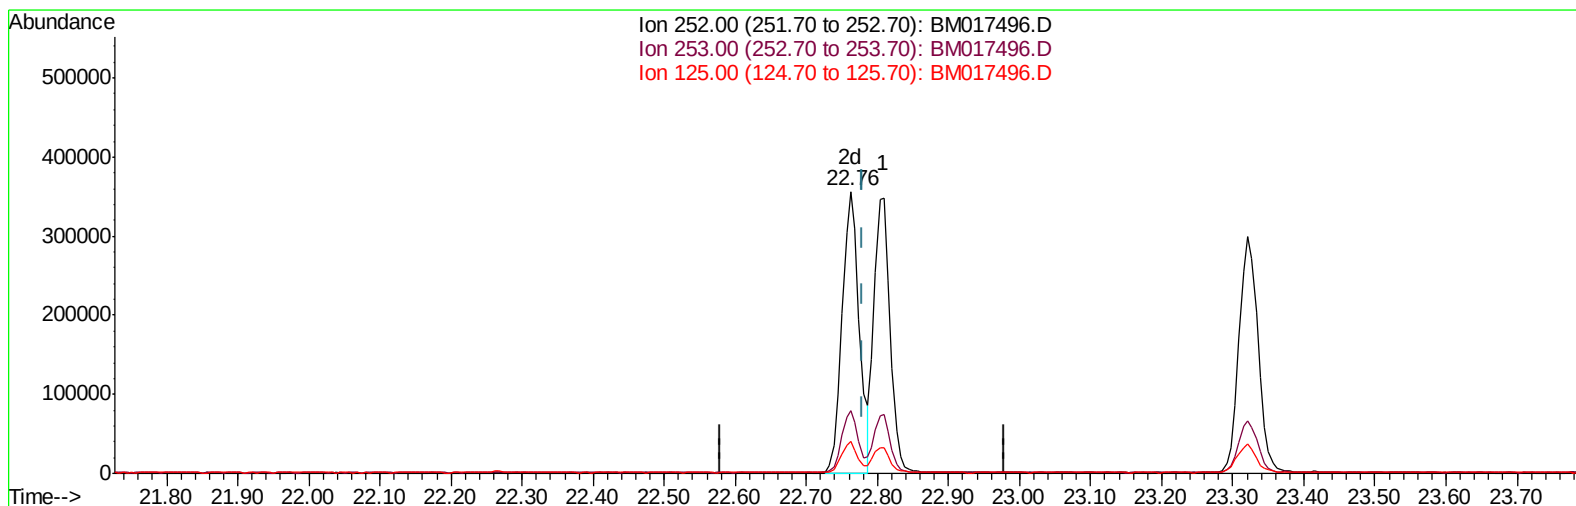

TIC: BM017496.D

(88) Benzo(b)fluoranthene

22.762min (-0.018) 21.53ng/ul m

response 599071

Ion	Exp%	Act%
252.00	100	100
253.00	22.00	22.28
125.00	9.00	11.37#
0.00	0.00	0.00