
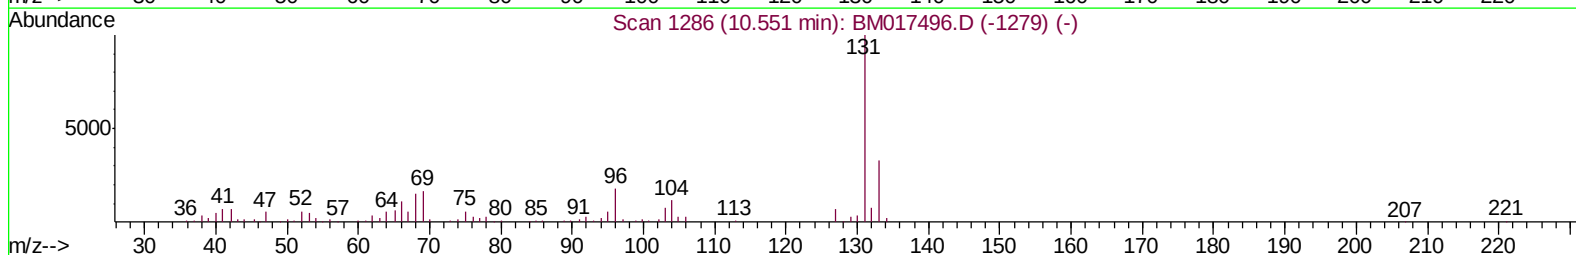
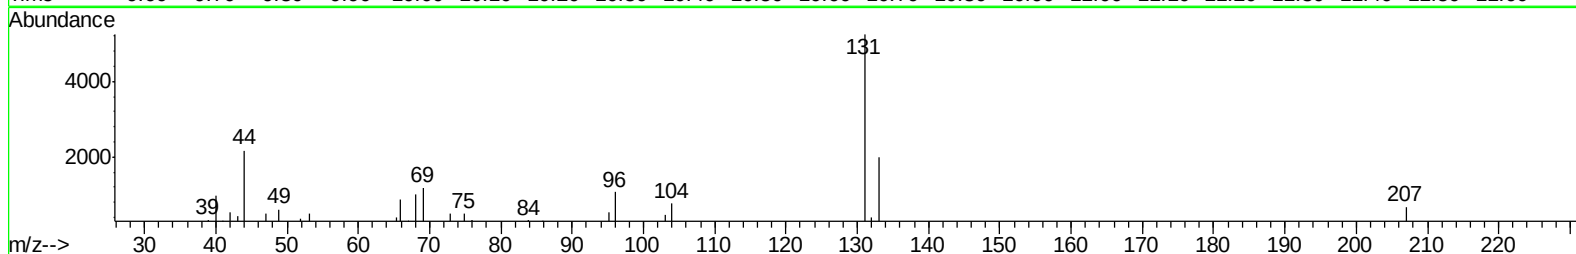


Data File : BM017499.D
Acq On : 02 Nov 2018 20:37
Operator : MJ/SJ
Sample : J5802-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Nov 03 04:02:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 03:58:03 2018
Response via : Initial Calibration

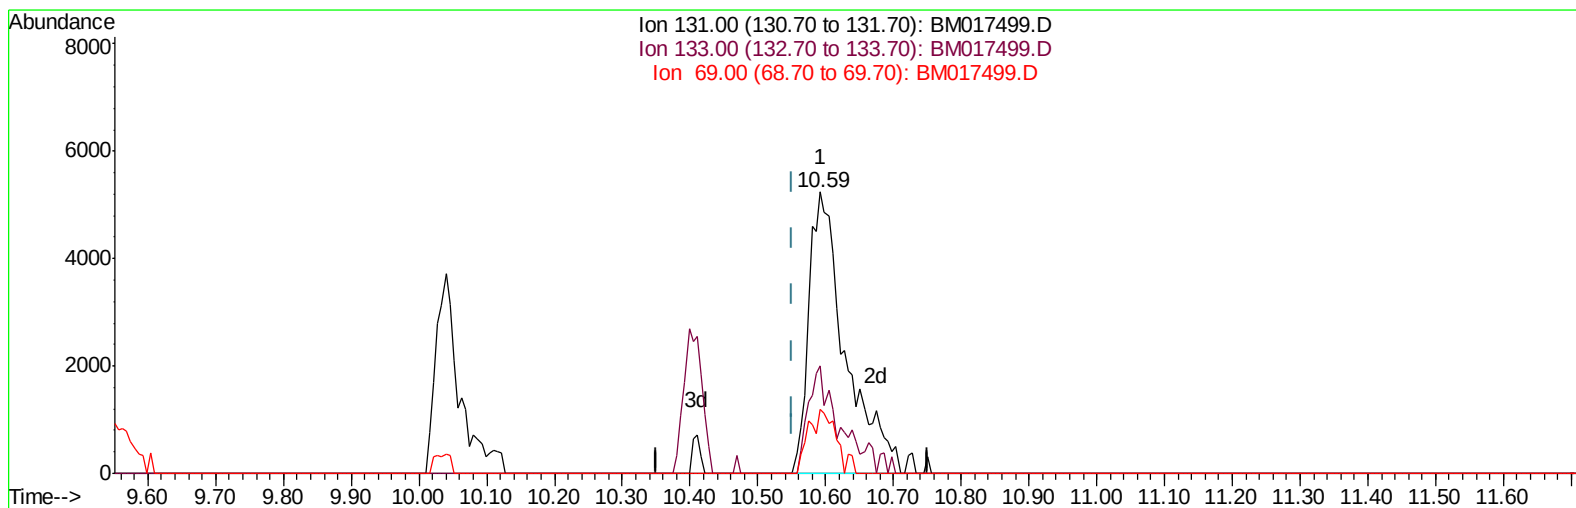

TIC: BM017499.D

(29) 4-Chloroaniline-d4 (S)

10.592min (+0.041) 2.16ng/ul m

response 19527

Ion	Exp%	Act%
131.00	100	100
133.00	33.60	38.09
69.00	17.60	22.76#
0.00	0.00	0.00