
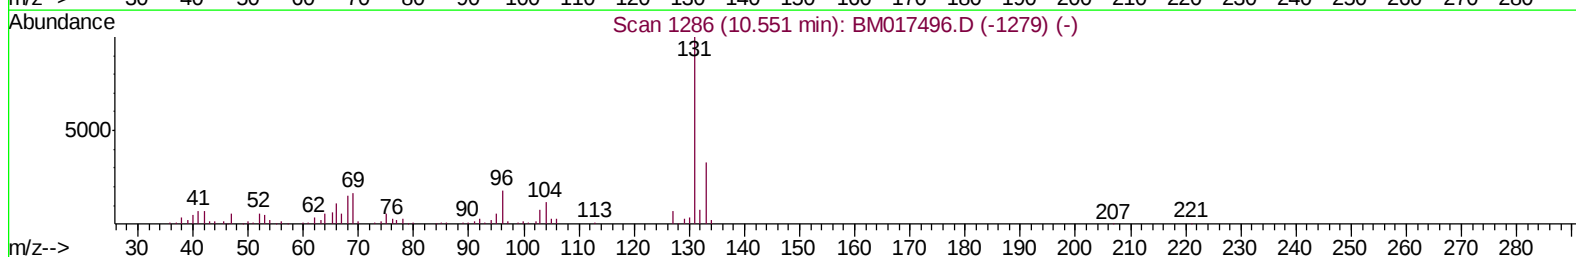
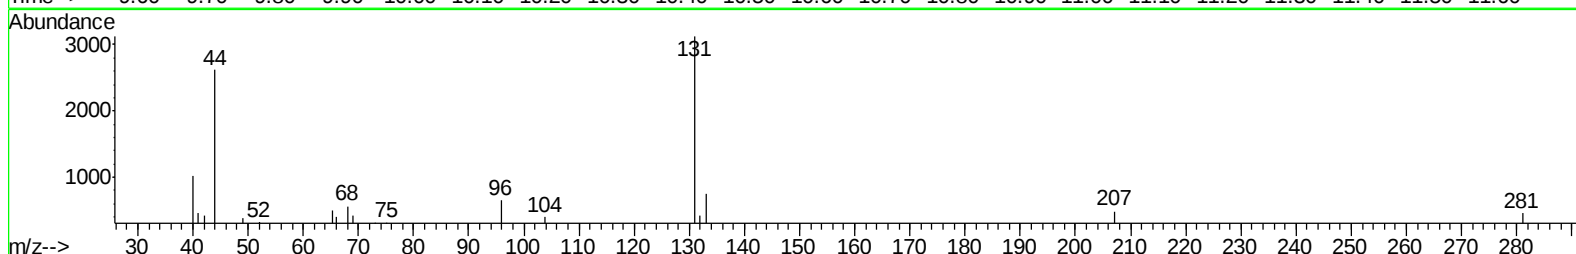


Data File : BM017501.D
Acq On : 02 Nov 2018 21:50
Operator : MJ/SJ
Sample : J5802-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Nov 03 04:02:34 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 03:58:03 2018
Response via : Initial Calibration

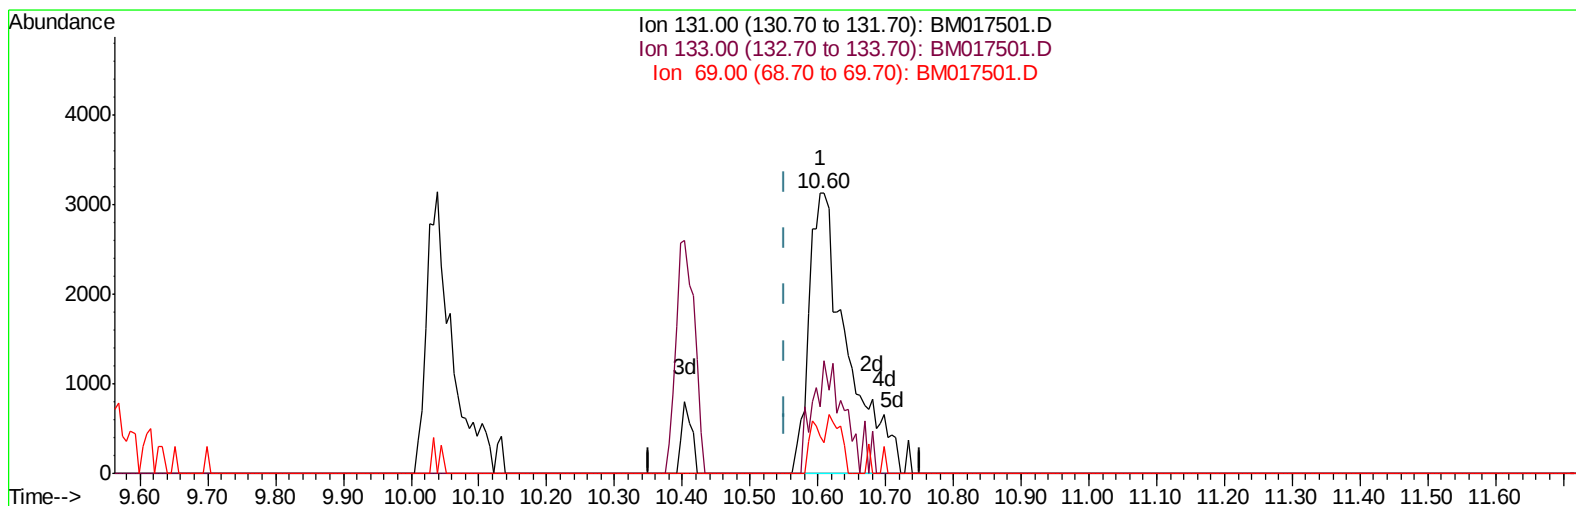

TIC: BM017501.D

(29) 4-Chloroaniline-d4 (S)

10.604min (+0.053) 1.41ng/ul m

response 12211

Ion	Exp%	Act%
131.00	100	100
133.00	33.60	23.87#
69.00	17.60	13.09#
0.00	0.00	0.00