
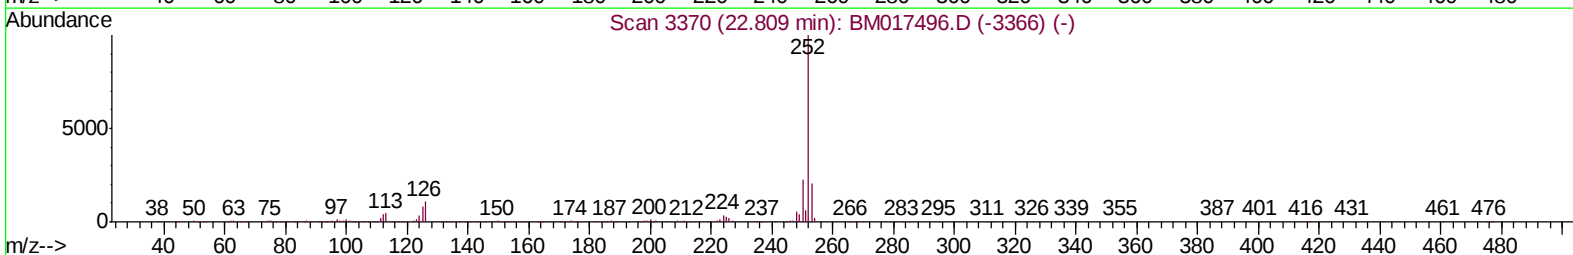
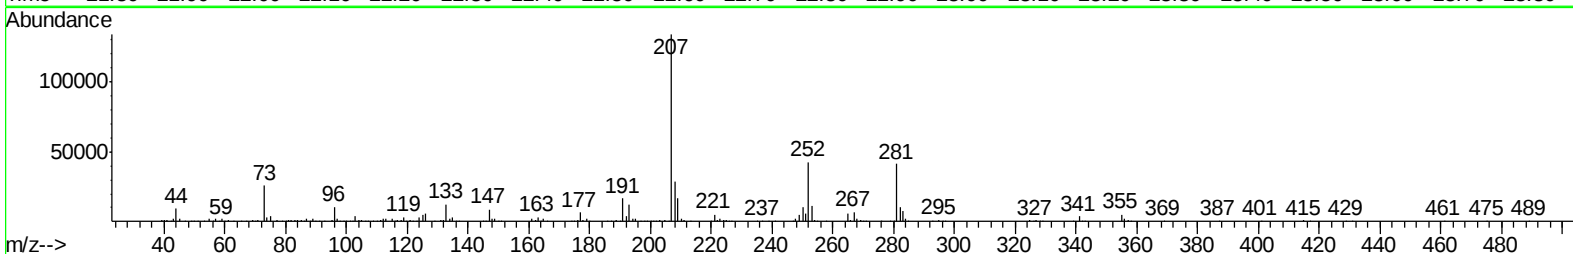


Data File : BM017503.D
Acq On : 02 Nov 2018 23:02
Operator : MJ/SJ
Sample : J5704-24
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Nov 03 04:02:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 03:58:03 2018
Response via : Initial Calibration

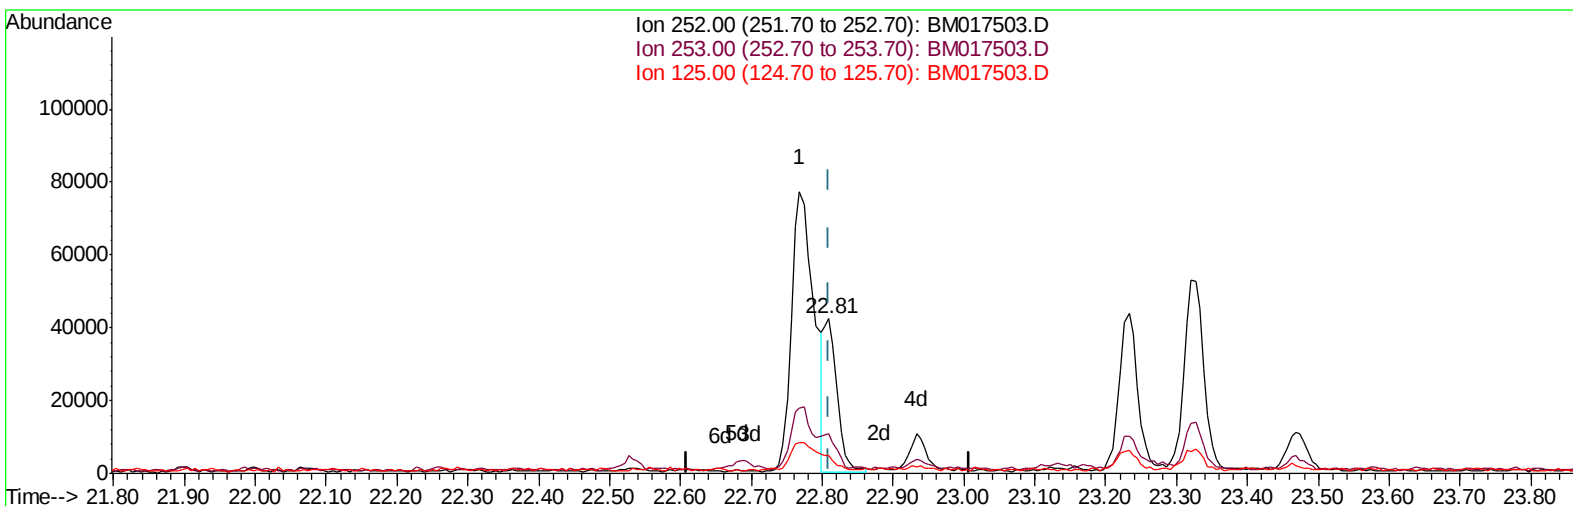

TIC: BM017503.D

(89) Benzo(k)fluoranthene

22.809min (+0.000) 2.95ng/ul m

response 56632

Ion	Exp%	Act%
252.00	100	100
253.00	22.10	26.04
125.00	9.70	11.37
0.00	0.00	0.00