
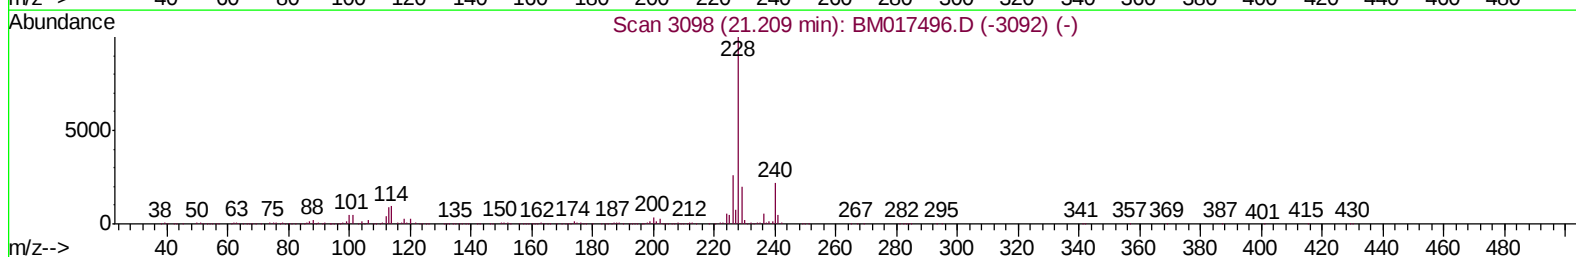
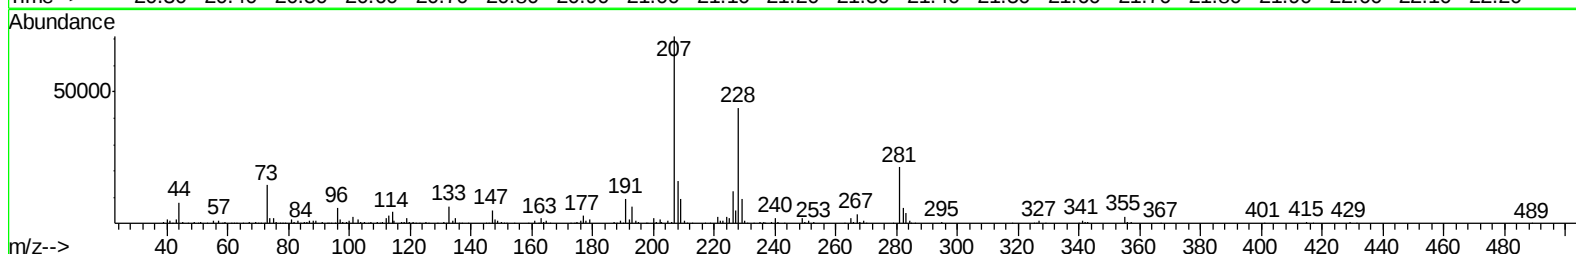


Data File : BM017505.D  
Acq On : 03 Nov 2018 00:14  
Operator : MJ/SJ  
Sample : J5704-26MSD  
Misc :  
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Nov 03 04:03:31 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM102418MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Sat Nov 03 03:58:03 2018  
Response via : Initial Calibration

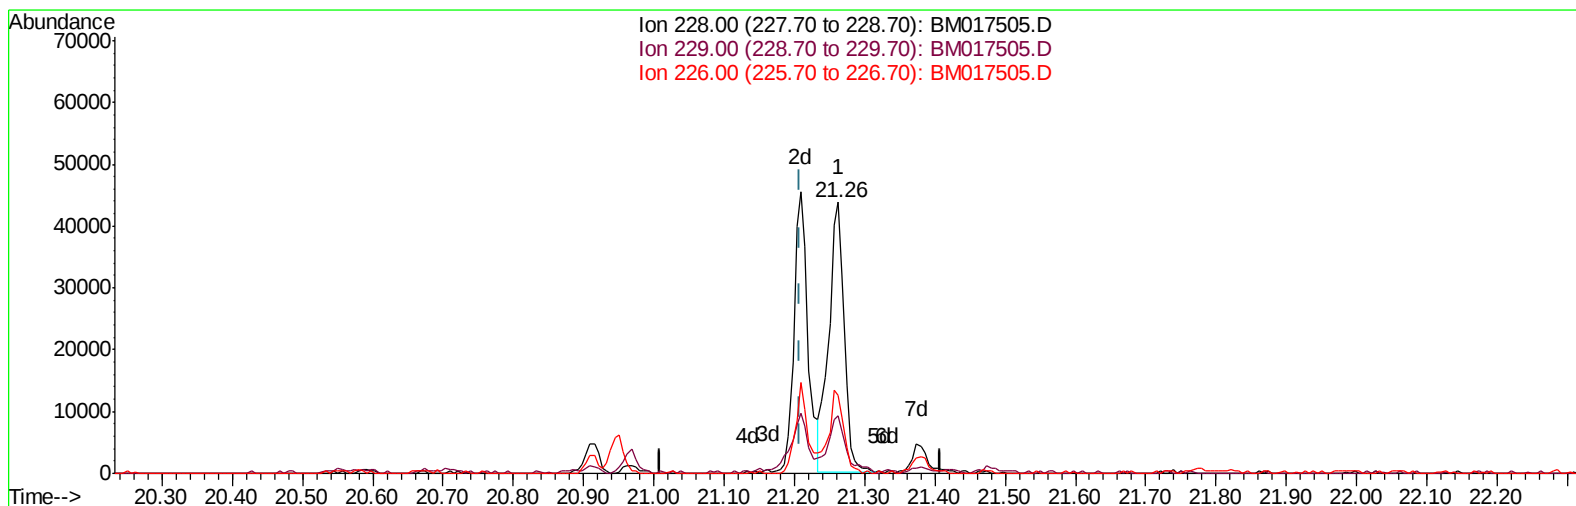

TIC: BM017505.D

(83) Benzo(a)anthracene  
21.262min (+0.053) 2.36ng/ul  
response 66085

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 228.00 | 100   | 100   |
| 229.00 | 19.50 | 21.13 |
| 226.00 | 26.00 | 28.68 |
| 0.00   | 0.00  | 0.00  |