
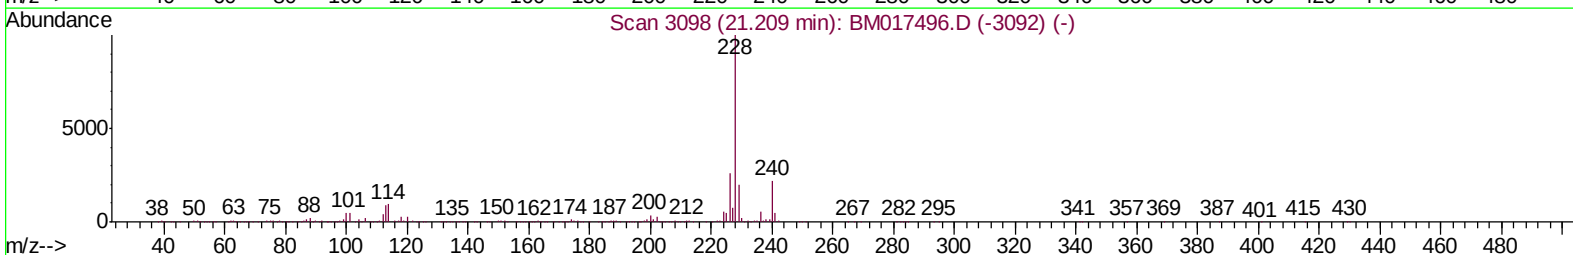
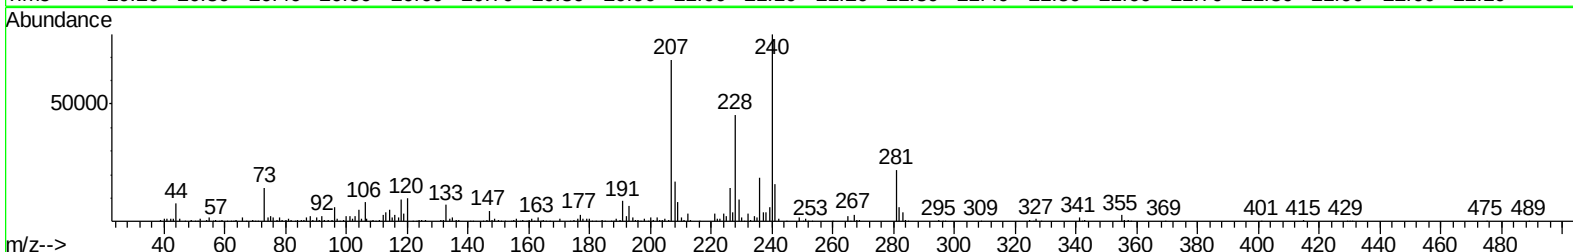


Data File : BM017505.D
Acq On : 03 Nov 2018 00:14
Operator : MJ/SJ
Sample : J5704-26MSD
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Nov 03 04:03:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 03:58:03 2018
Response via : Initial Calibration

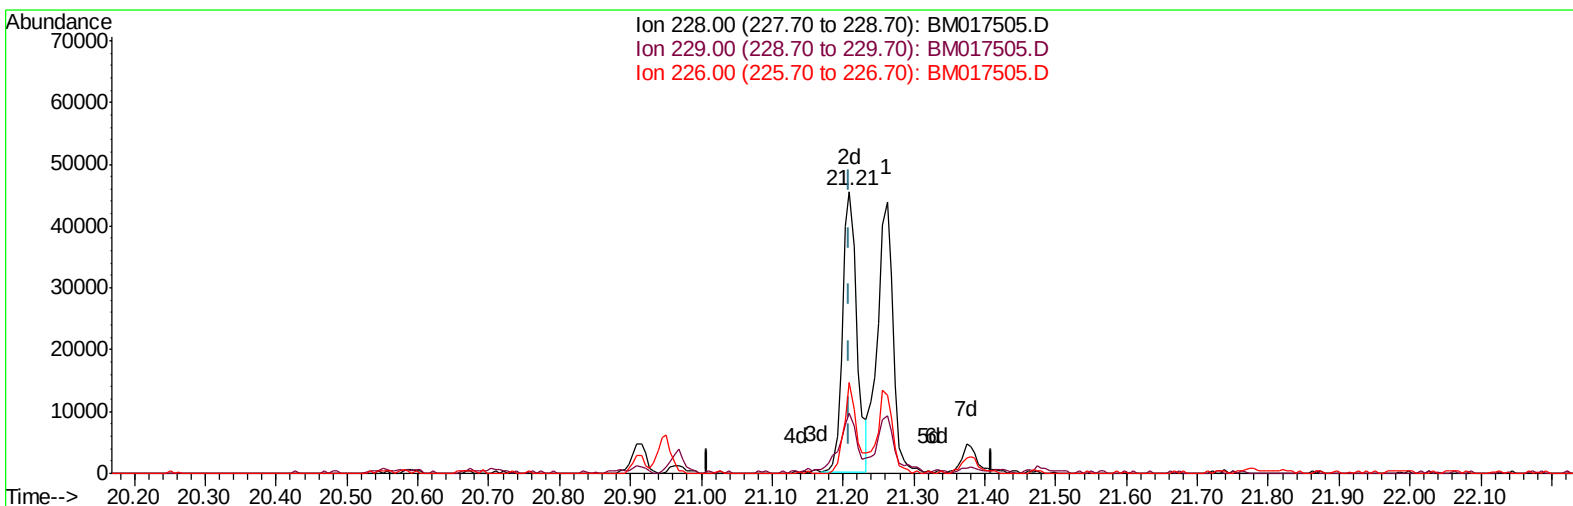

TIC: BM017505.D

(83) Benzo(a)anthracene
21.209min (-0.000) 2.28ng/ul m
response 63899

Ion	Exp%	Act%
228.00	100	100
229.00	19.50	21.30
226.00	26.00	32.07#
0.00	0.00	0.00