
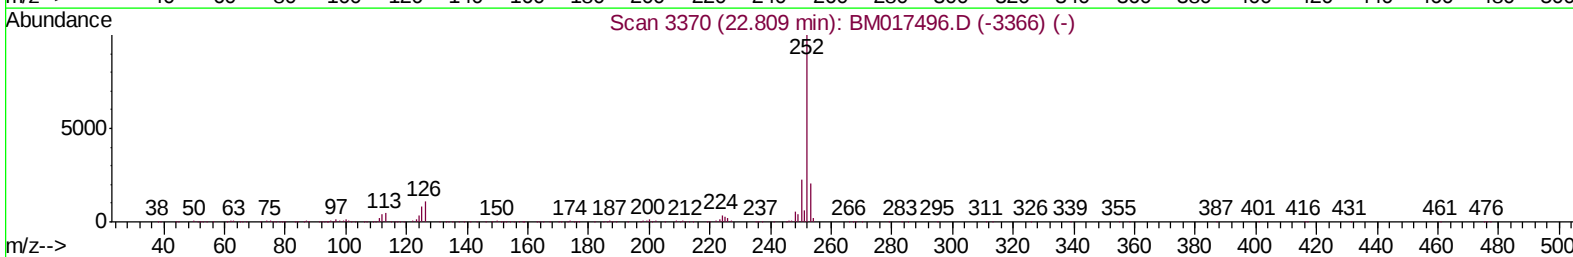
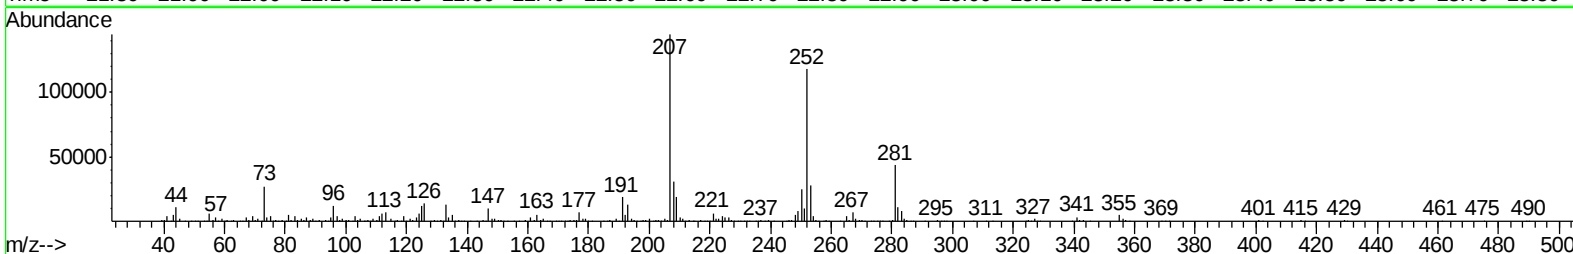


Data File : BM017506.D
Acq On : 03 Nov 2018 00:50
Operator : MJ/SJ
Sample : J5635-12
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Nov 03 04:03:49 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 03:58:03 2018
Response via : Initial Calibration

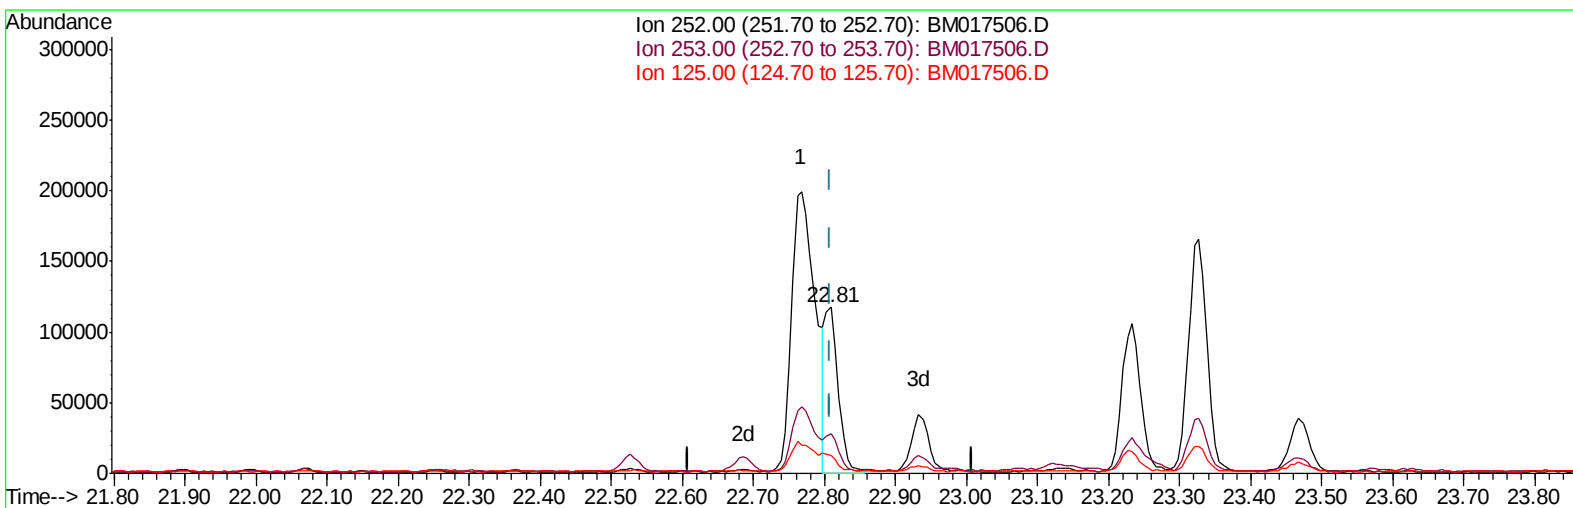

TIC: BM017506.D

(89) Benzo(k)fluoranthene

22.809min (-0.000) 7.07ng/ul m

response 147364

Ion	Exp%	Act%
252.00	100	100
253.00	22.10	23.87
125.00	9.70	10.46
0.00	0.00	0.00