

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (QT Reviewed)


Data File : BM017489.D
Acq On : 02 Nov 2018 10:14
Operator : MJ/SJ
Sample : J5701-16ME
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
Client Sample ID :
A40G0ME

Manual Integrations
APPROVED

Sohil
11/5/2018 4:05:54 PM

Quant Time: Nov 03 02:51:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 02:25:47 2018
Response via : Initial Calibration

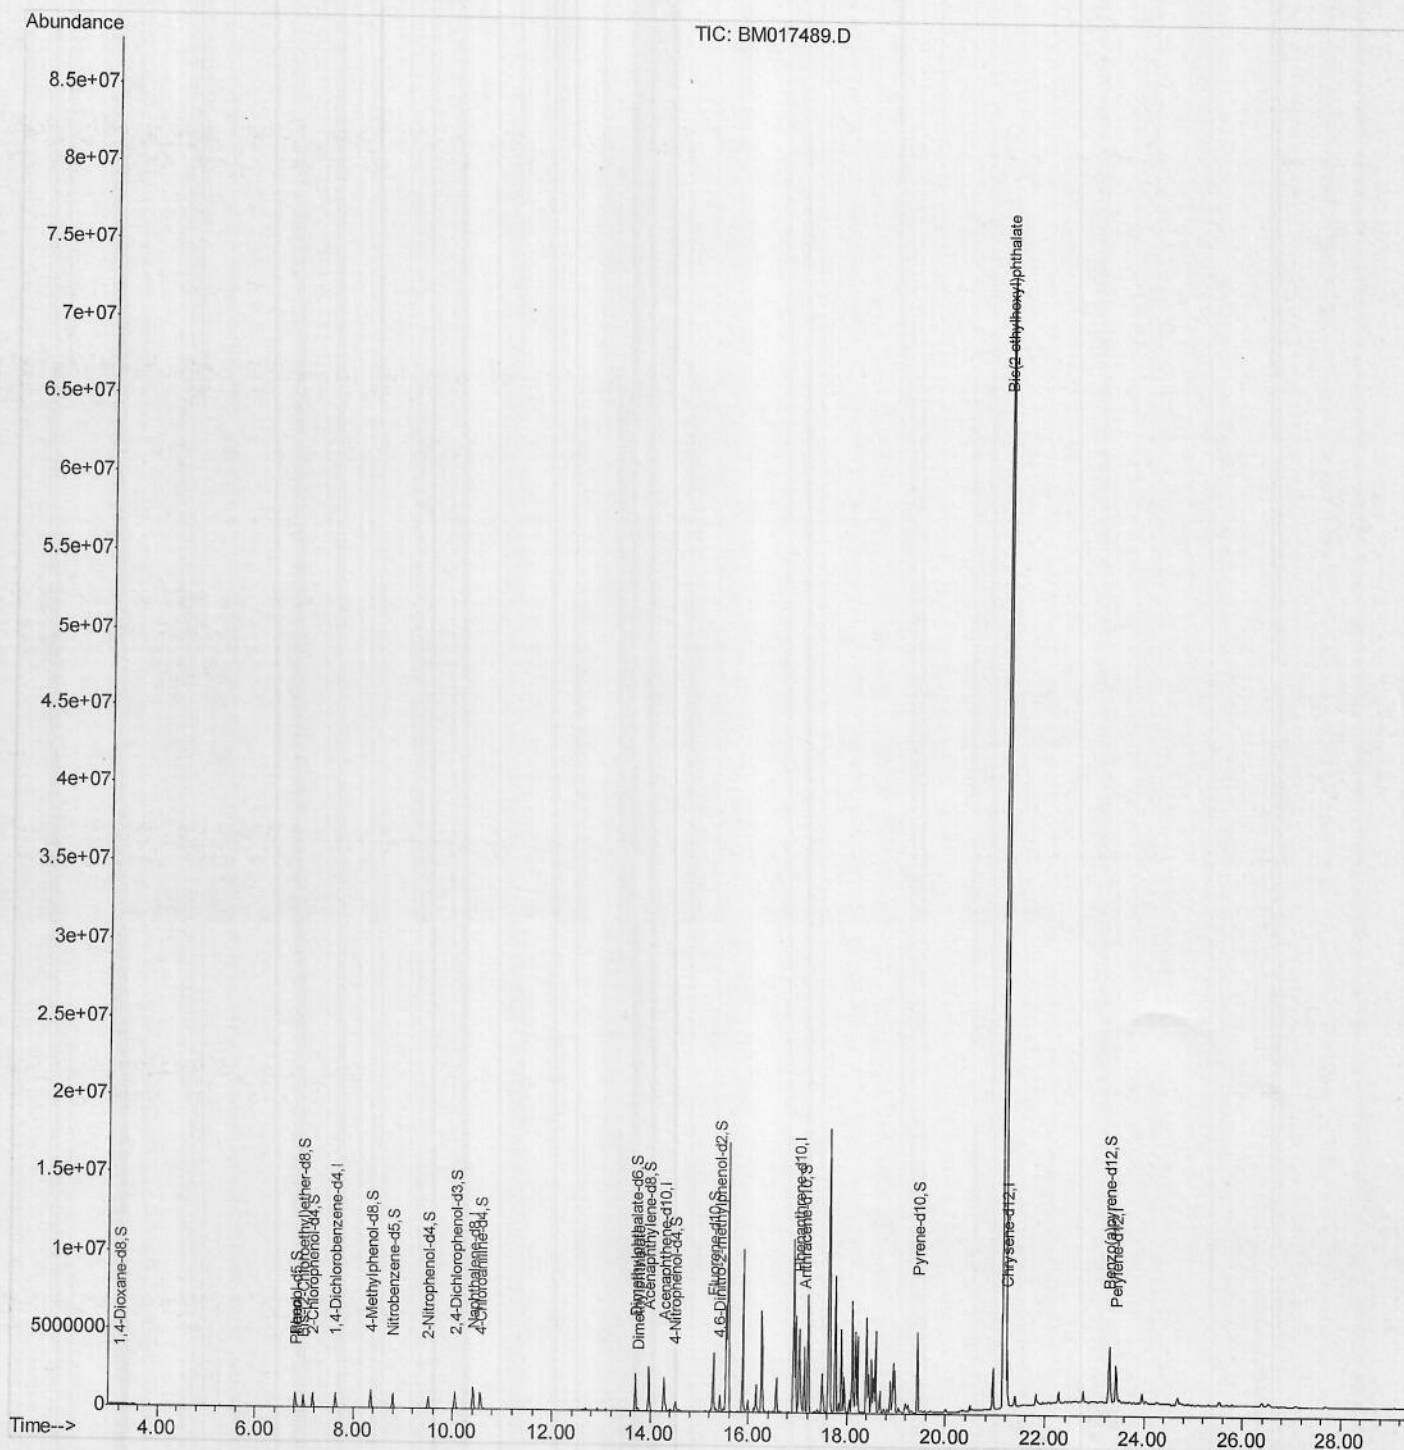

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (Qedit)




Data File : BM017489.D
Acq On : 02 Nov 2018 10:14
Operator : MJ/SJ
Sample : J5701-16ME
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40G0ME

Manual Integrations
APPROVED

Sohil
11/5/2018 4:05:54 PM

Quant Time: Nov 03 02:33:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 02:25:47 2018
Response via : Initial Calibration

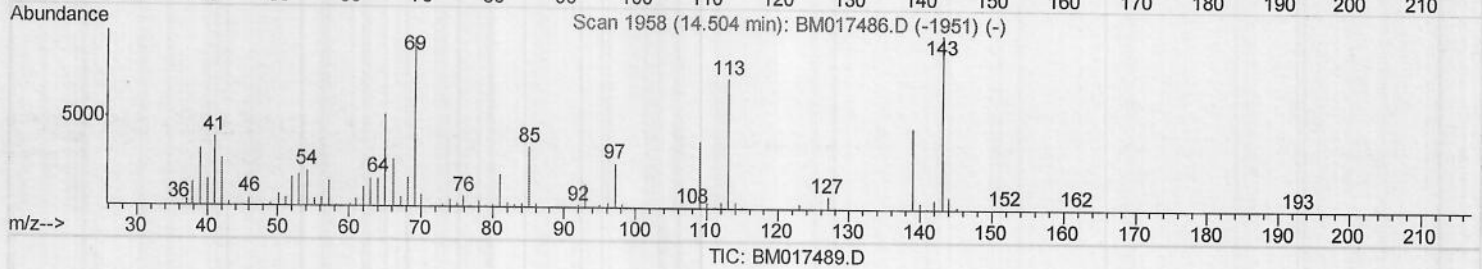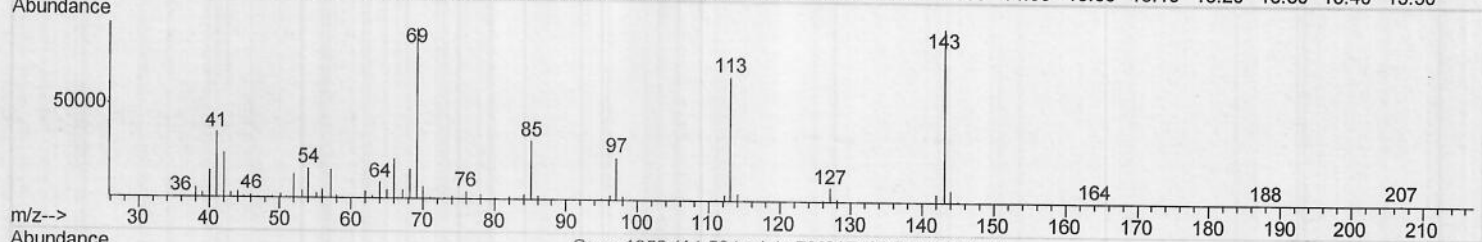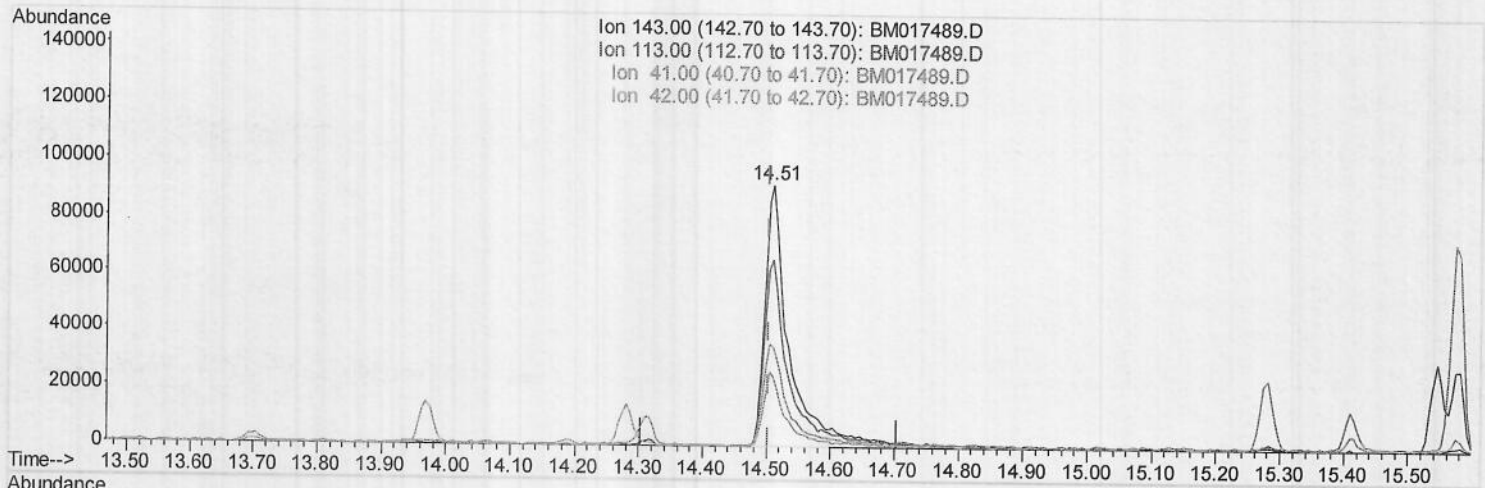

TIC: BM017489.D

(52) 4-Nitrophenol-d4 (S)

14.510min (+0.006) 20.27ng/ul

response 222995

Ion	Exp%	Act%
143.00	100	100
113.00	74.20	71.42
41.00	39.30	37.79
42.00	25.10	26.40




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
 Quantitation Report (Qedit)
 Data File : BM017489.D
 Acq On : 02 Nov 2018 10:14
 Operator : MJ/SJ
 Sample : J5701-16ME
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A40G0ME

Manual Integrations
 APPROVED

Sohil
 11/5/2018 4:05:54 PM

Quant Time: Nov 03 02:33:26 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Nov 03 02:25:47 2018
 Response via : Initial Calibration

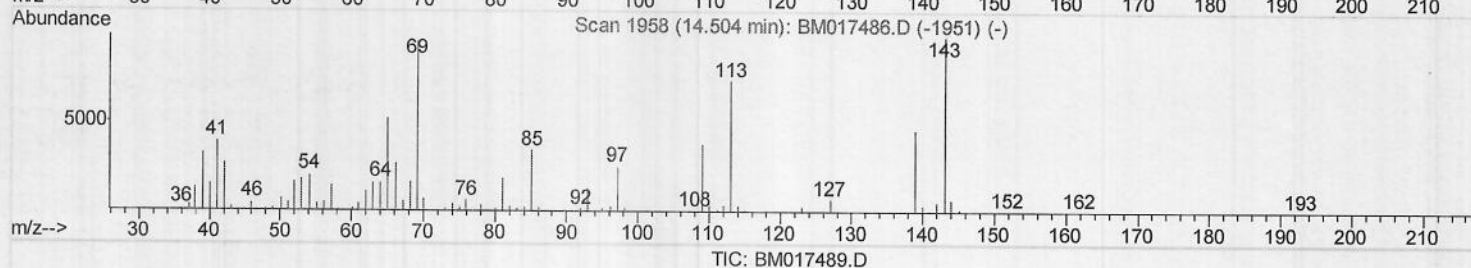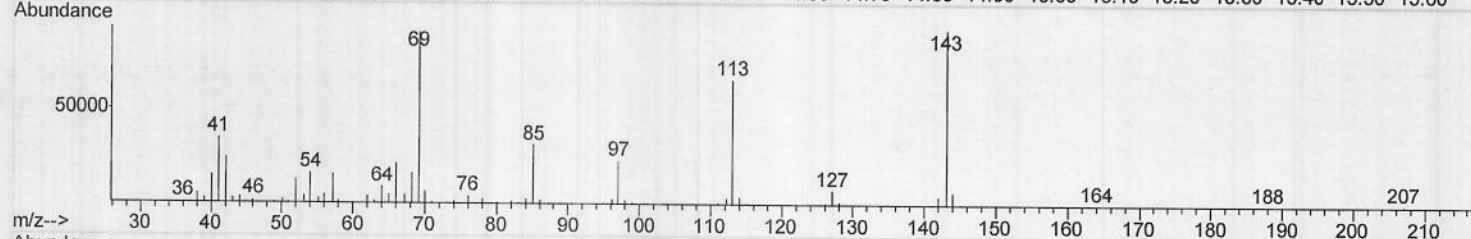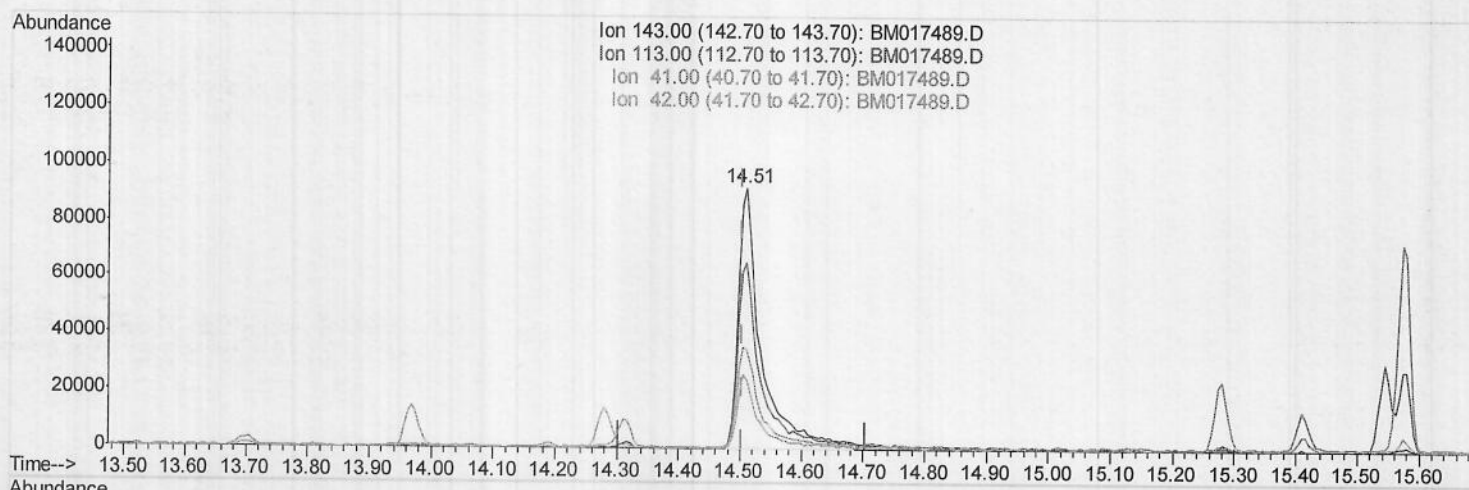

(52) 4-Nitrophenol-d4 (S)

14.510min (+0.006) 22.00ng/ul m

response 242051

Ion	Exp%	Act%
143.00	100	100
113.00	74.20	71.42
41.00	39.30	37.79
42.00	25.10	26.40

28 5/11/06/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (Qedit)




Data File : BM017489.D
Acq On : 02 Nov 2018 10:14
Operator : MJ/SJ
Sample : J5701-16ME
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40G0ME

Manual Integrations
APPROVED

Sohil
11/5/2018 4:05:54 PM

Quant Time: Nov 03 02:33:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 02:25:47 2018
Response via : Initial Calibration

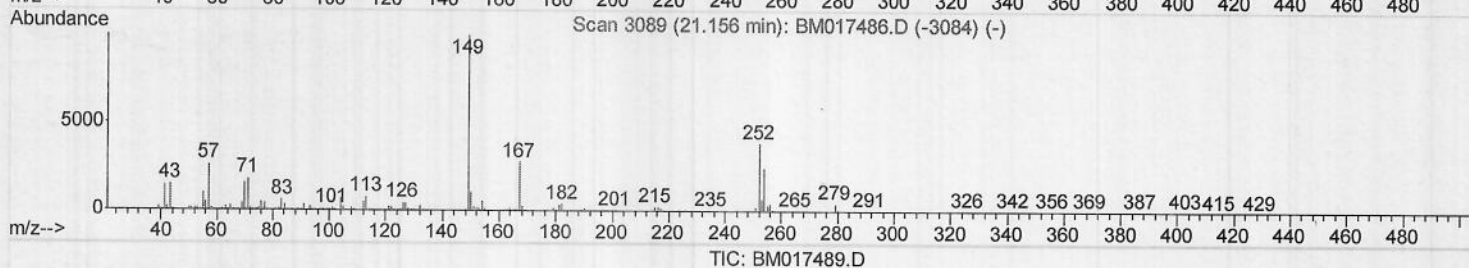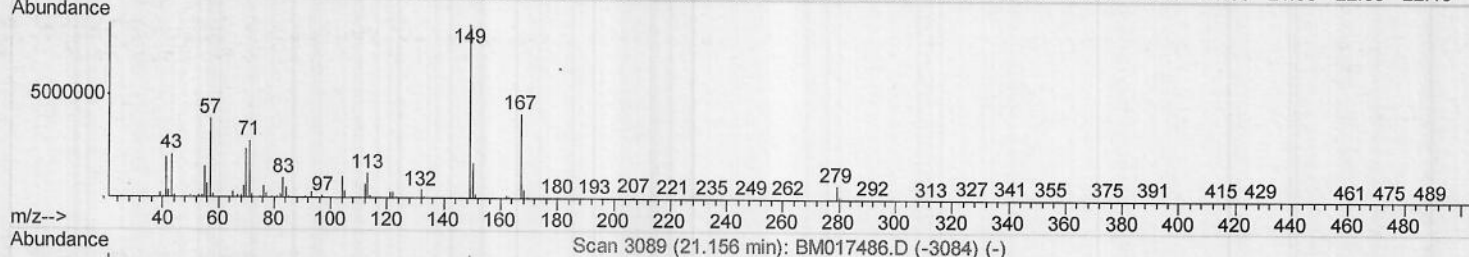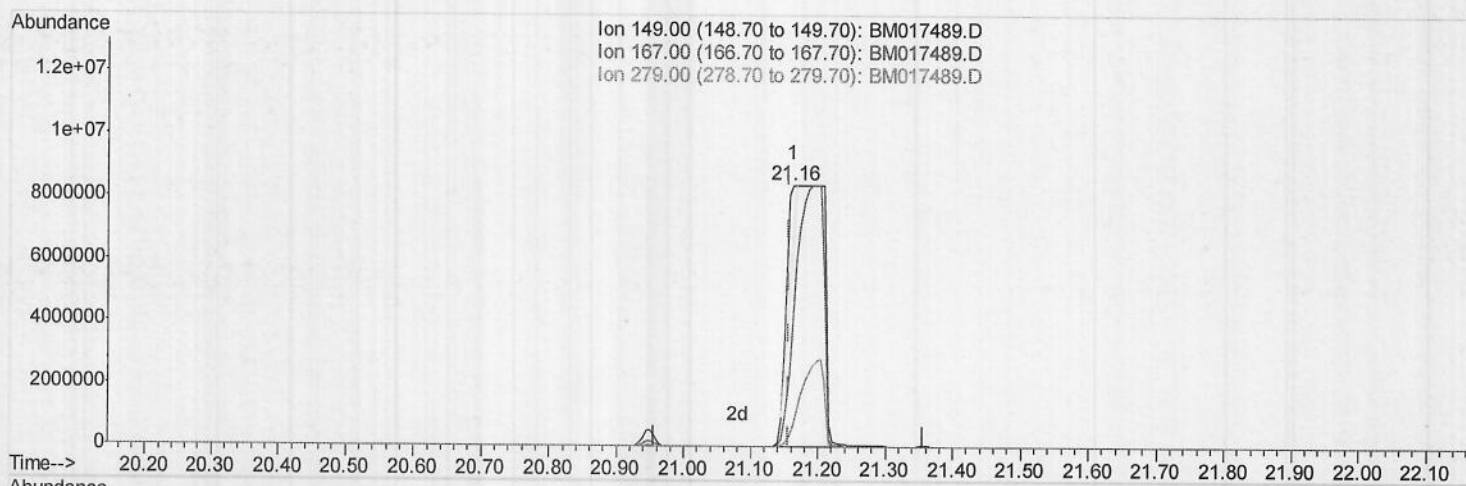

(84) Bis(2-ethylhexyl)phthalate

21.162min (+0.006) 59.78ng/ul

response 3772121

Ion	Exp%	Act%
149.00	100	100
167.00	28.80	49.00#
279.00	5.10	8.00#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
 Quantitation Report (Qedit)
 Data File : BM017489.D
 Acq On : 02 Nov 2018 10:14
 Operator : MJ/SJ
 Sample : J5701-16ME
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A40G0ME

Manual Integrations
 APPROVED

Sohil
 11/5/2018 4:05:54 PM

Quant Time: Nov 03 02:33:26 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Nov 03 02:25:47 2018
 Response via : Initial Calibration

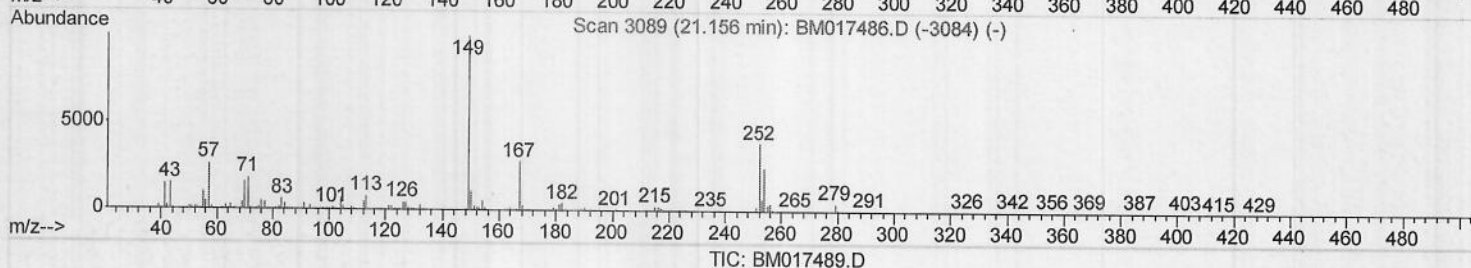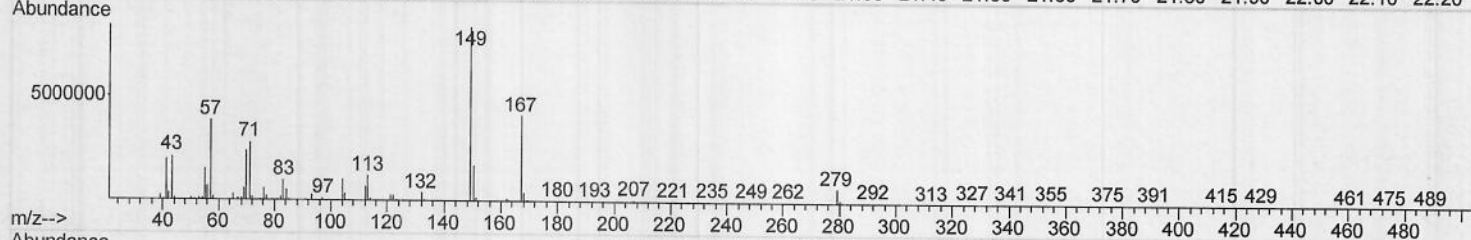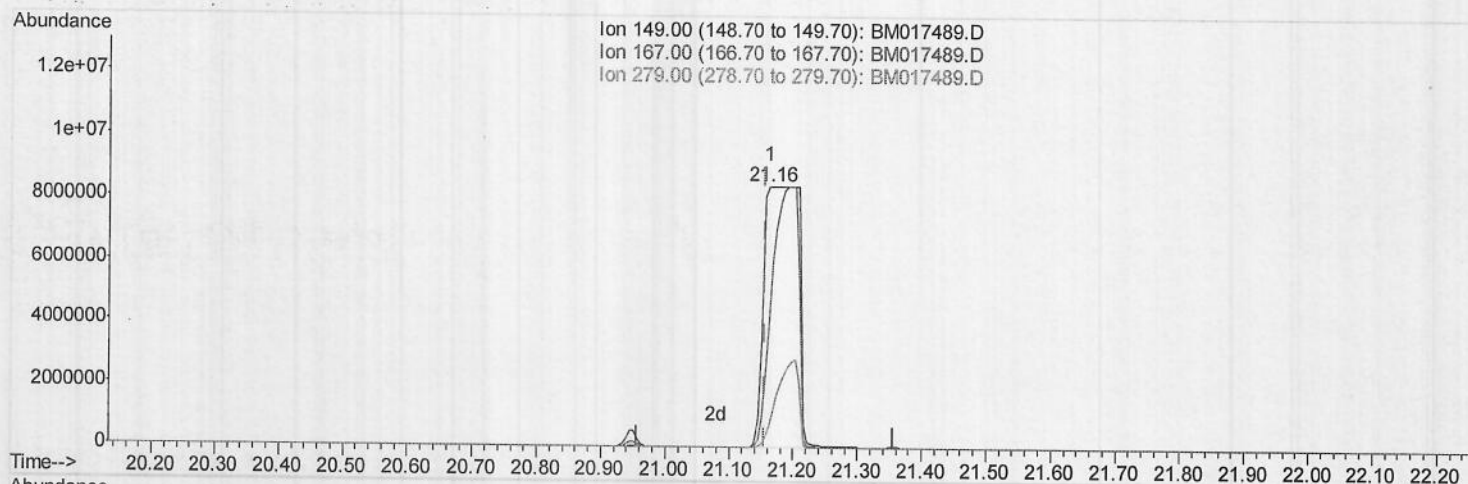

(84) Bis(2-ethylhexyl)phthalate

21.162min (+0.006) 499.84ng/ul m *J5711/06/18*

response 31540211

Ion	Exp%	Act%
149.00	100	100
167.00	28.80	49.00#
279.00	5.10	8.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\

Quantitation Report (QT Reviewed)

Data File : BM017489.D

Acq On : 02 Nov 2018 10:14

Operator : MJ/SJ

Sample : J5701-16ME

Misc :

ALS Vial : 5 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

A40G0ME

Manual Integrations

APPROVED

Sohil

11/5/2018 4:05:54 PM

Quant Time: Nov 03 02:51:37 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Sat Nov 03 02:25:47 2018

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	246335	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1135891	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.28	164	686621	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1714906	20.00	ng/ul	0.00
78) Chrysene-d12	21.23	240	1862662	20.00	ng/ul	0.00
86) Perylene-d12	23.44	264	1725935	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	20083	3.75	ng/uL	0.00
5) Phenol-d5	6.82	99	522815	23.23	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	329019	25.07	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	424183	24.31	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	438294	24.63	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	220971	24.89	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	248943	25.00	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	433048	23.42	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	629807	41.72	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	1629837	27.68	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	2028599	28.37	ng/ul	0.00
52) 4-Nitrophenol-d4	14.51	143	242051m	22.00	ng/ul	0.00
58) Fluorene-d10	15.28	176	1452501	28.40	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.42	200	229340	19.19	ng/ul	0.00
71) Anthracene-d10	17.13	188	2338386	27.55	ng/ul	0.00
79) Pyrene-d10	19.43	212	2648193	30.69	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.30	264	2700141	29.62	ng/ul	0.00

Target Compounds

					Qvalue	
6) Phenol	6.85	94	39583	1.772	ng/ul#	86
45) Dimethylphthalate	13.75	163	141560	2.481	ng/ul	99
84) Bis(2-ethylhexyl)phthalate	21.16	149	31540211m	499.843	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJ11/06/18