

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (QT Reviewed)


Data File : BM017493.D
Acq On : 02 Nov 2018 12:59
Operator : MJ/SJ
Sample : J5701-16MEDL 100X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40G0MEDL

Manual Integrations
APPROVED

Sohil
11/5/2018 4:05:57 PM

Quant Time: Nov 03 03:44:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 02:25:47 2018
Response via : Initial Calibration

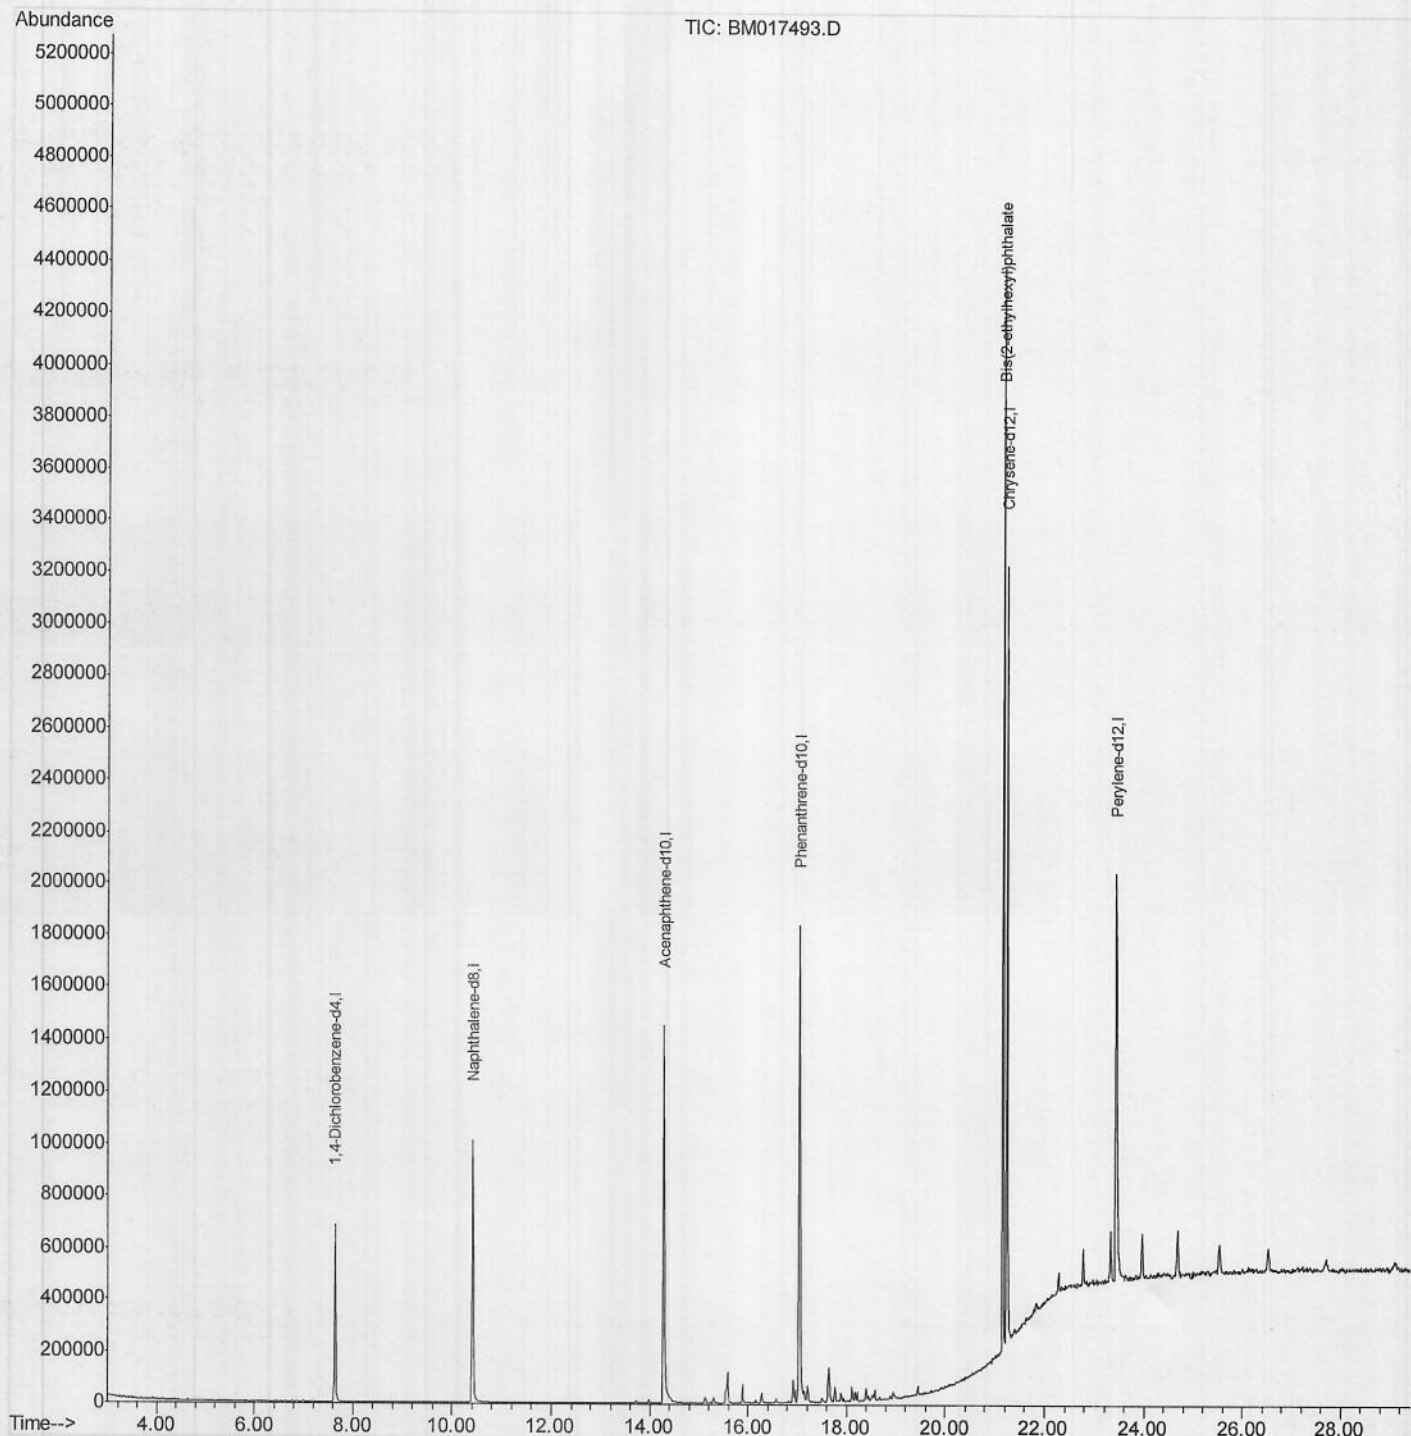

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (Qedit)




Data File : BM017493.D
Acq On : 02 Nov 2018 12:59
Operator : MJ/SJ
Sample : J5701-16MEDL 100X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40G0MEDL

Manual Integrations
APPROVED

Sohil
11/5/2018 4:05:57 PM

Quant Time: Nov 03 02:33:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 02:25:47 2018
Response via : Initial Calibration

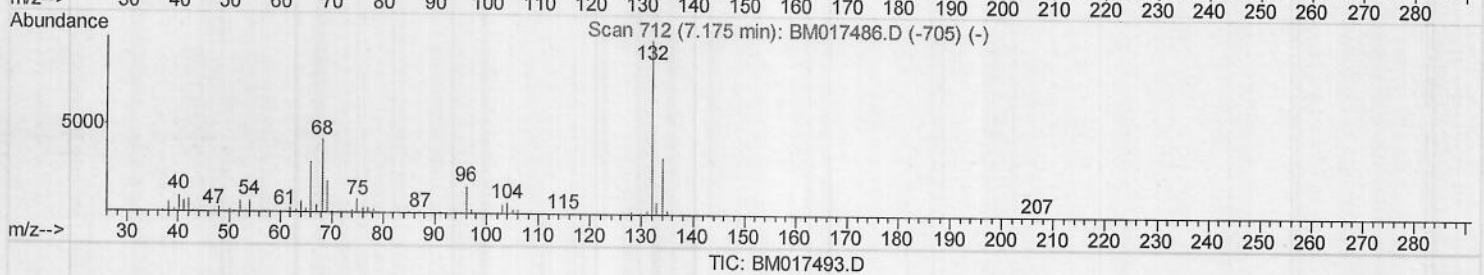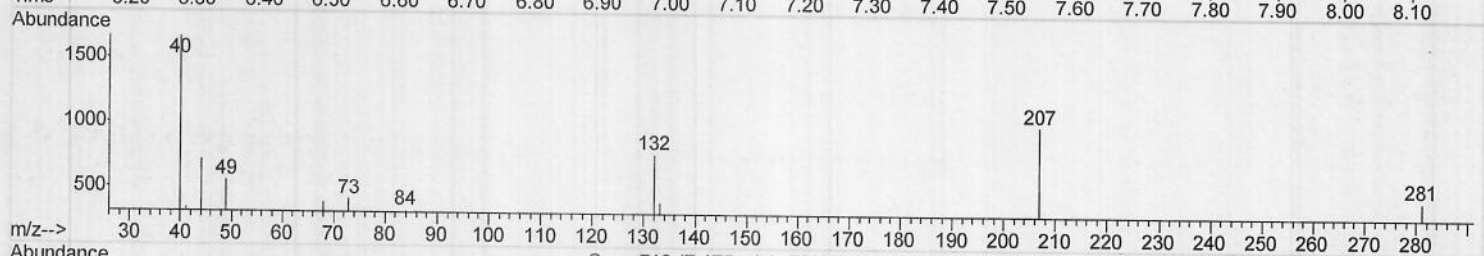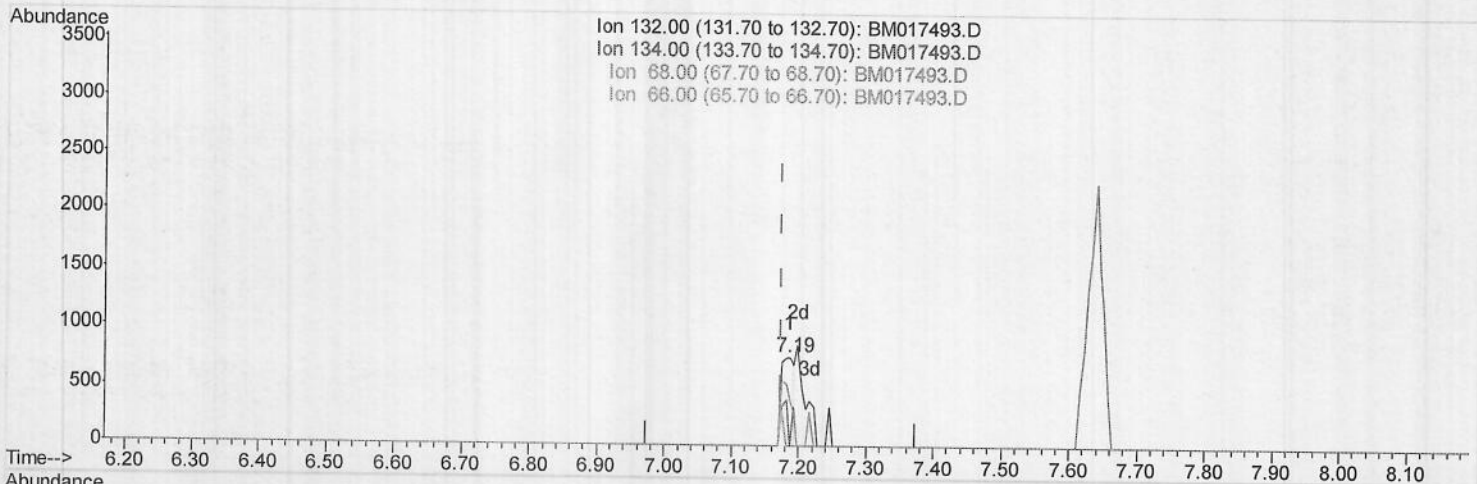

(9) 2-Chlorophenol-d4 (S)

7.187min (+0.012) 0.08ng/ul

response 1043

Ion	Exp%	Act%
132.00	100	100
134.00	32.10	0.00#
68.00	39.20	50.85#
66.00	26.90	0.00#

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (Qedit)




Data File : BM017493.D
Acq On : 02 Nov 2018 12:59
Operator : MJ/SJ
Sample : J5701-16MEDL 100X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
Client Sample Id :
A40G0MEDL

Manual Integrations
APPROVED

Sohil
11/5/2018 4:05:57 PM

Quant Time: Nov 03 02:33:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 02:25:47 2018
Response via : Initial Calibration

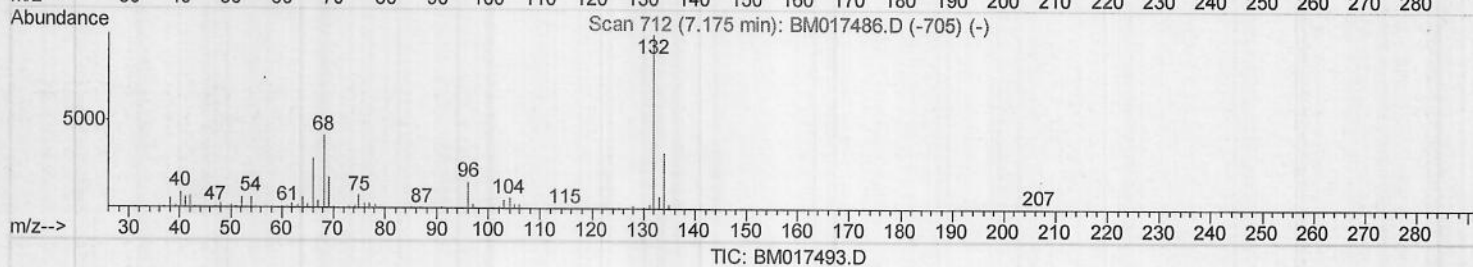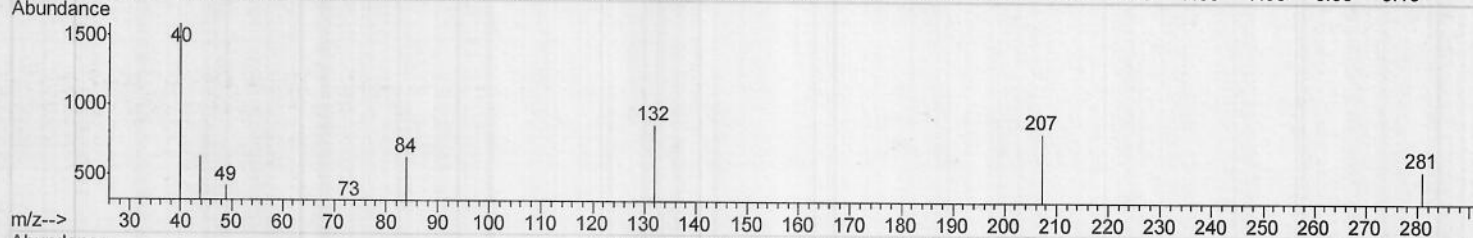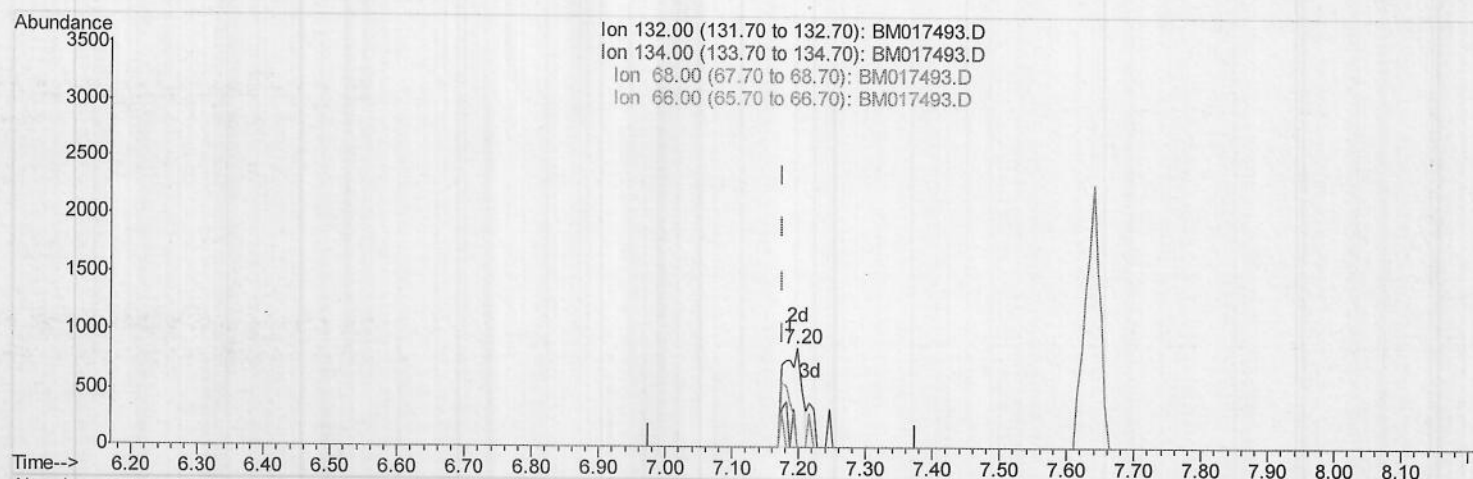

TIC: BM017493.D

(9) 2-Chlorophenol-d4 (S)

7.199min (+0.024) 0.12ng/ul m

SJH/06/18

response 1634

Ion	Exp%	Act%
132.00	100	100
134.00	32.10	0.00#
68.00	39.20	0.00#
66.00	26.90	0.00#

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (Qedit)




Data File : BM017493.D
Acq On : 02 Nov 2018 12:59
Operator : MJ/SJ
Sample : J5701-16MEDL 100X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40G0MEDL

Manual Integrations
APPROVED

Sohil
11/5/2018 4:05:57 PM

Quant Time: Nov 03 02:33:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 02:25:47 2018
Response via : Initial Calibration

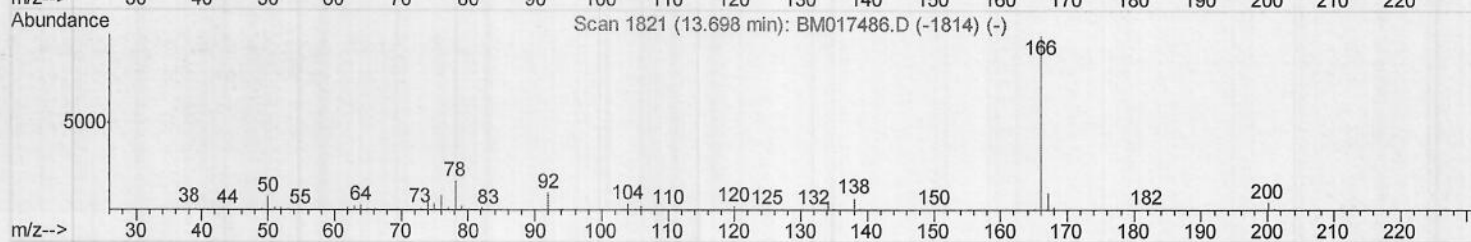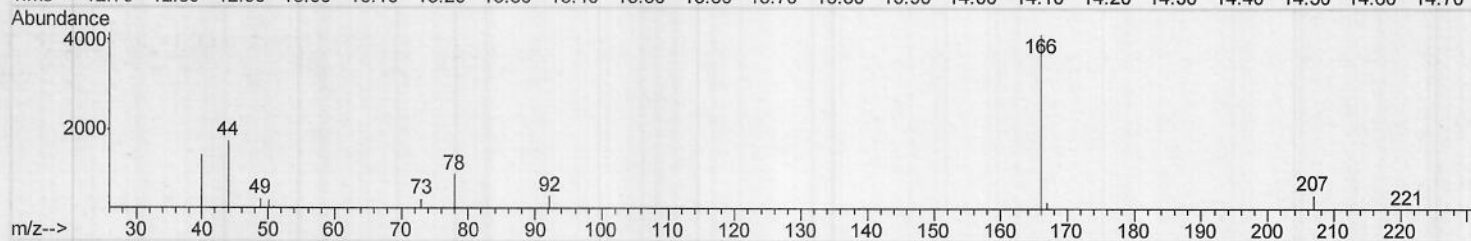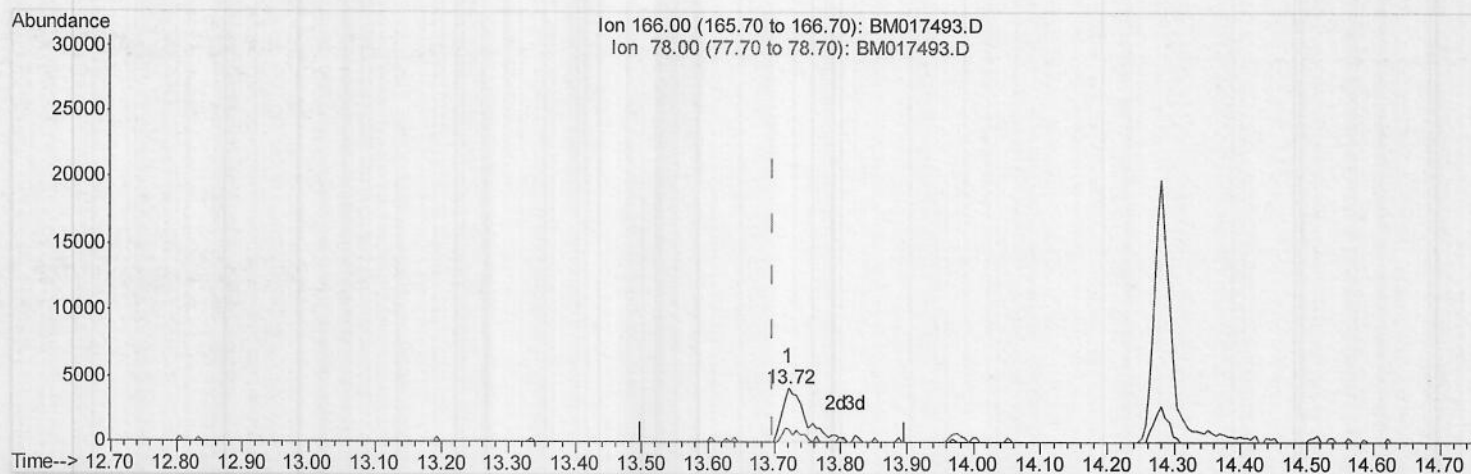

TIC: BM017493.D

(44) Dimethylphthalate-d6 (S)

13.722min (+0.024) 0.18ng/ul

response 8139

Ion	Exp%	Act%
166.00	100	100
78.00	16.40	25.12#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (Qedit)




Data File : BM017493.D
Acq On : 02 Nov 2018 12:59
Operator : MJ/SJ
Sample : J5701-16MEDL 100X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40G0MEDL

Manual Integrations
APPROVED

Sohil
11/5/2018 4:05:57 PM

Quant Time: Nov 03 02:33:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 02:25:47 2018
Response via : Initial Calibration

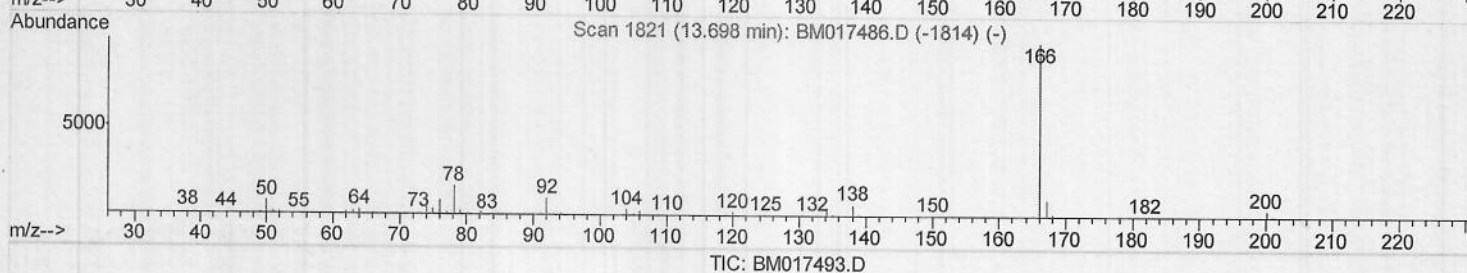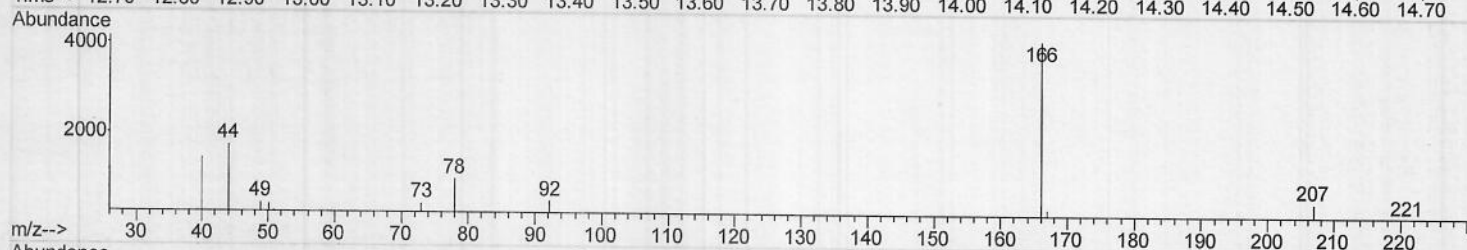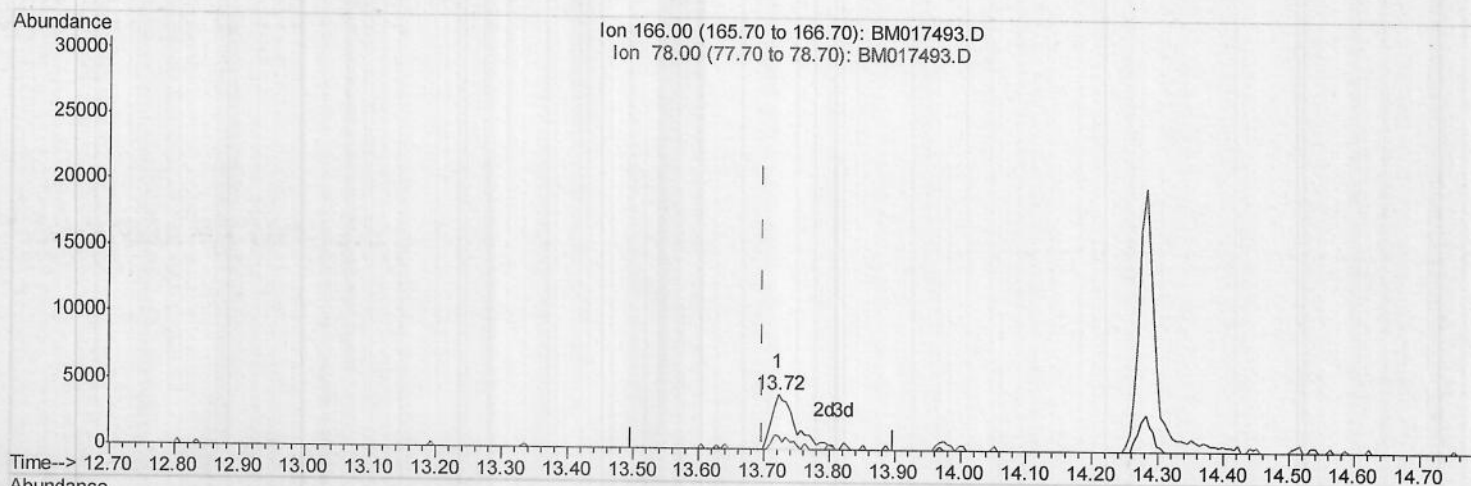

(44) Dimethylphthalate-d6 (S)

13.722min (+0.024) 0.21ng/ul m

JS11/06/18

response 9793

Ion	Exp%	Act%
166.00	100	100
78.00	16.40	25.12#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (QT Reviewed)

Data File : BM017493.D
Acq On : 02 Nov 2018 12:59
Operator : MJ/SJ
Sample : J5701-16MEDL 100X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
Client Sampled :
A40G0MEDL

Manual Integrations
APPROVED

Sohil
11/5/2018 4:05:57 PM

Quant Time: Nov 03 03:44:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 02:25:47 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	190602	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	869395	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.28	164	536613	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1359476	20.00	ng/ul	0.00
78) Chrysene-d12	21.23	240	1483038	20.00	ng/ul	0.00
86) Perylene-d12	23.44	264	1317584	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	6.85	99	200	0.01	ng/ul	0.03
7) Bis-(2-Chloroethyl)ether-d	6.99	67	1536	0.15	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	1634m)	0.12	ng/ul	0.02
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul	
19) Nitrobenzene-d5	8.82	128	412	0.06	ng/ul	0.02
22) 2-Nitrophenol-d4	9.52	143	137	0.02	ng/ul	0.02
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul	
29) 4-Chloroaniline-d4	10.68	131	365	0.03	ng/ul	0.12
44) Dimethylphthalate-d6	13.72	166	9793m)	0.21	ng/ul	0.02
47) Acenaphthylene-d8	13.97	160	11552	0.21	ng/ul	0.00
52) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
58) Fluorene-d10	15.29	176	15129	0.38	ng/ul	0.01
63) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
71) Anthracene-d10	17.13	188	25030	0.37	ng/ul	0.00
79) Pyrene-d10	19.45	212	19550	0.28	ng/ul	0.01
90) Benzo(a)pyrene-d12	23.30	264	17908	0.26	ng/ul	0.00

Target Compounds					Qvalue	
84) Bis(2-ethylhexyl)phthalate	21.16	149	1312662	26.128	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed