


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (QT Reviewed)
Data File : BM017502.D
Acq On : 02 Nov 2018 22:26
Operator : MJ/SJ
Sample : J5802-14
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COBE0

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:05 PM

Quant Time: Nov 03 04:19:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 03:58:03 2018
Response via : Initial Calibration

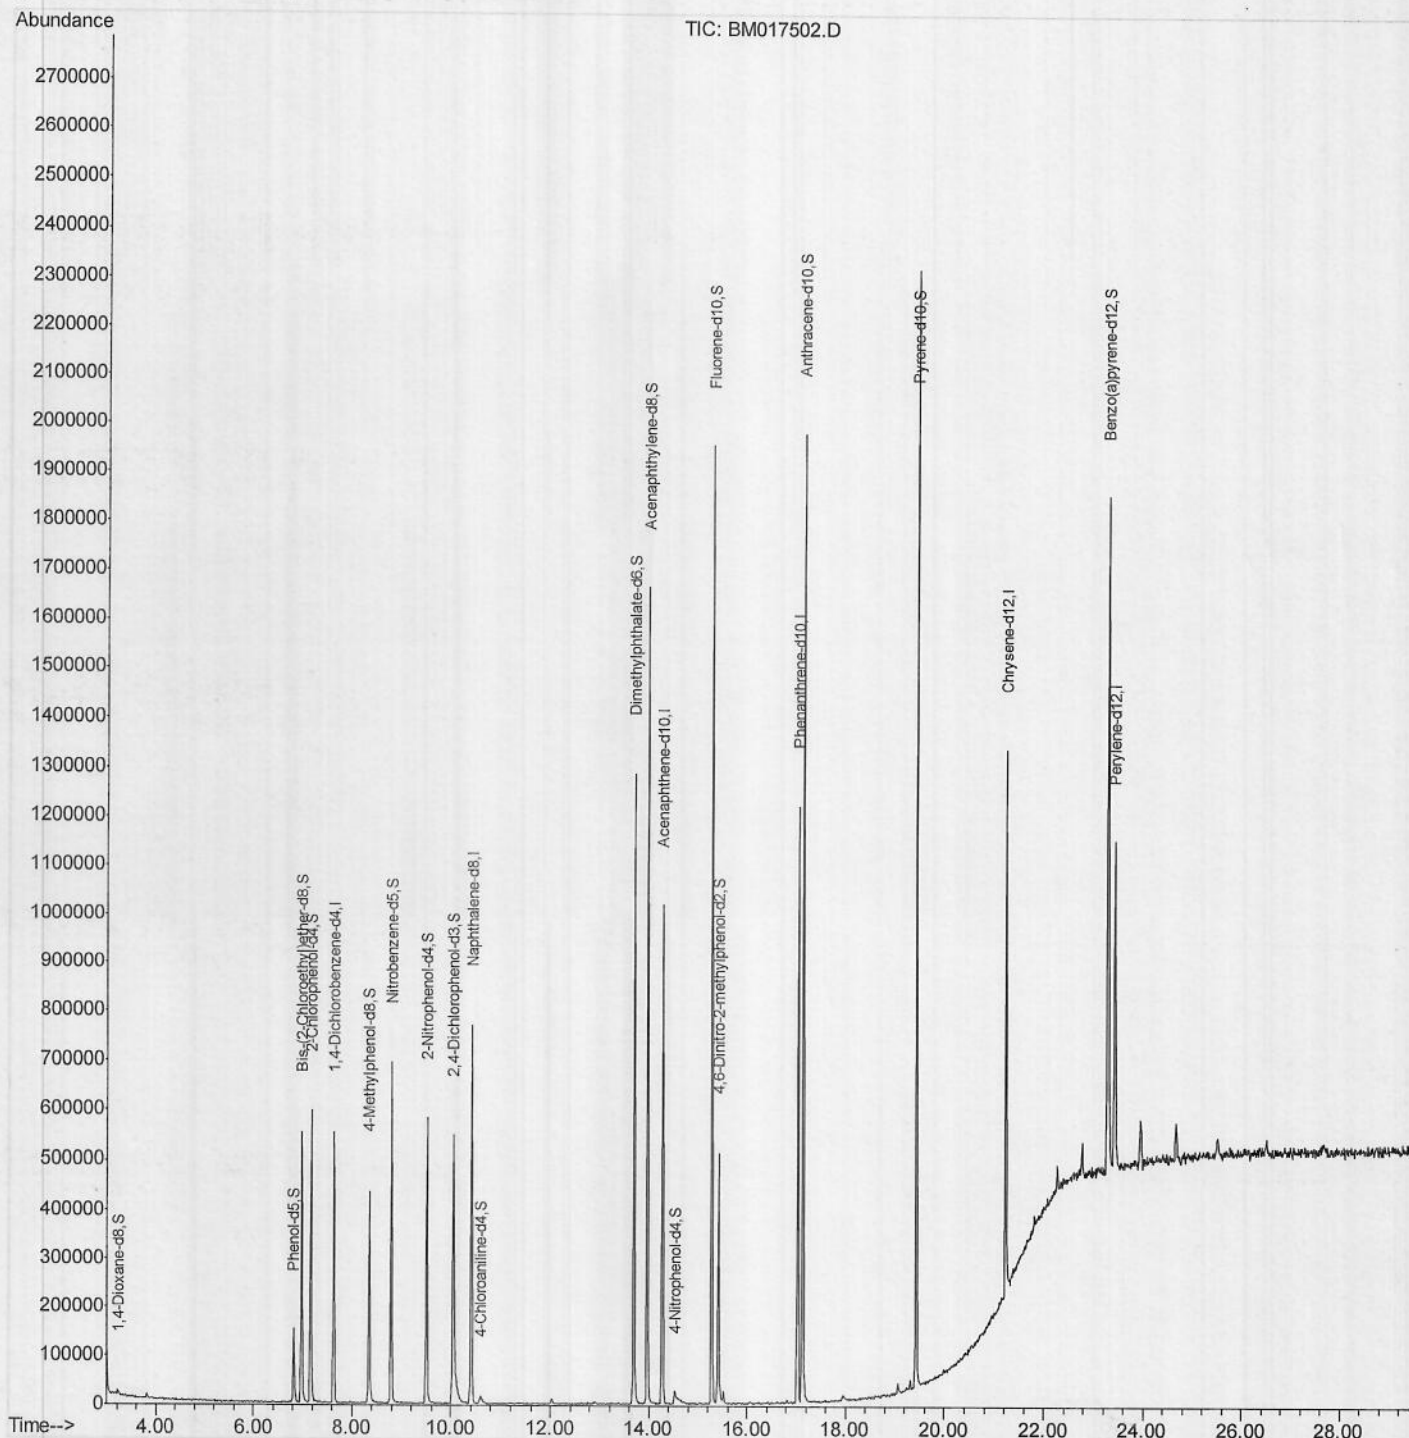

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (Qedit)




Data File : BM017502.D
Acq On : 02 Nov 2018 22:26
Operator : MJ/SJ
Sample : J5802-14
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COBE0

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:05 PM

Quant Time: Nov 03 04:02:44 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 03:58:03 2018
Response via : Initial Calibration

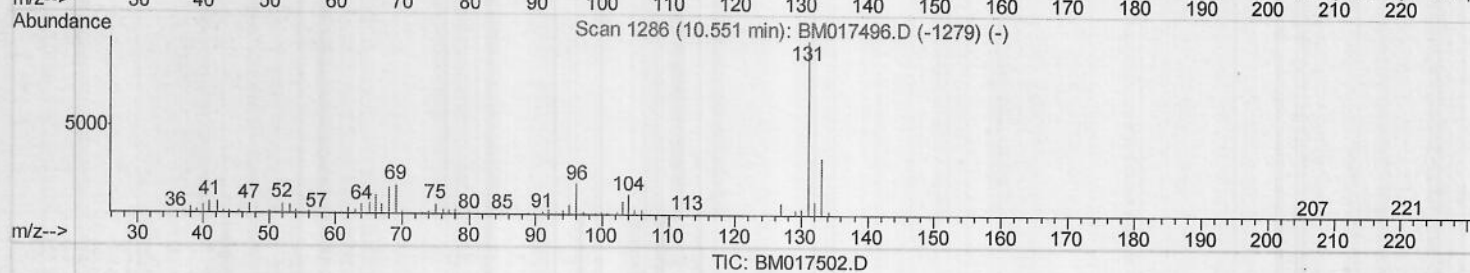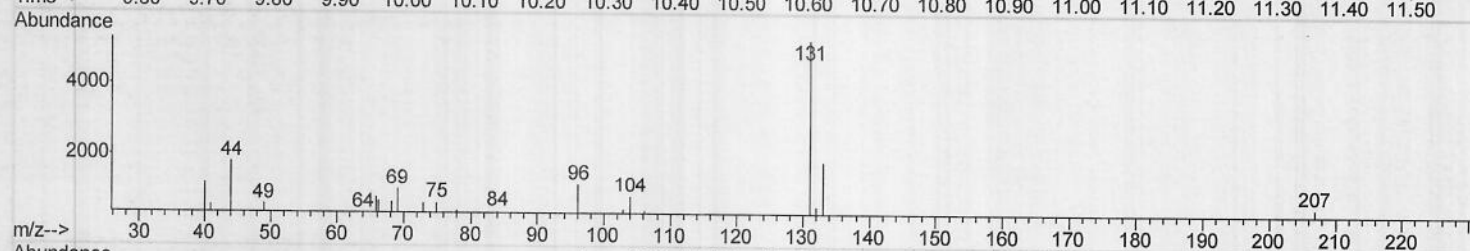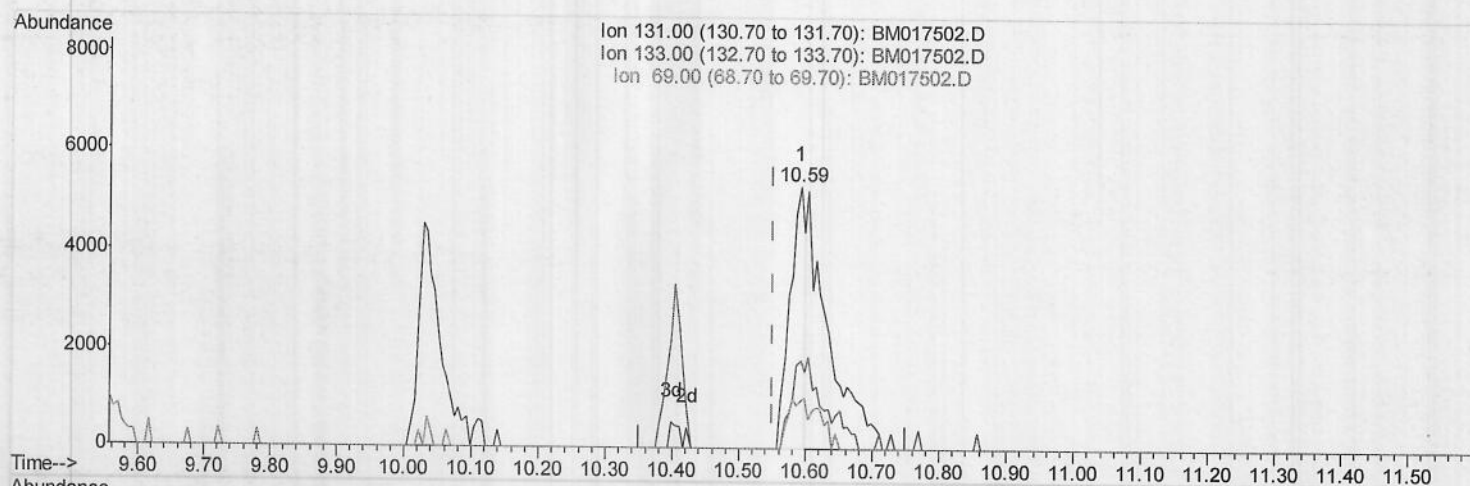

(29) 4-Chloroaniline-d4 (S)

10.592min (+0.041) 1.00ng/ul

response 8463

Ion	Exp%	Act%
131.00	100	100
133.00	33.60	34.14
69.00	17.60	18.63
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
 Quantitation Report (Qedit)
 Data File : BM017502.D
 Acq On : 02 Nov 2018 22:26
 Operator : MJ/SJ
 Sample : J5802-14
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COBE0

Manual Integrations
 APPROVED

Sohil
 11/5/2018 4:06:05 PM

Quant Time: Nov 03 04:02:44 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Nov 03 03:58:03 2018
 Response via : Initial Calibration

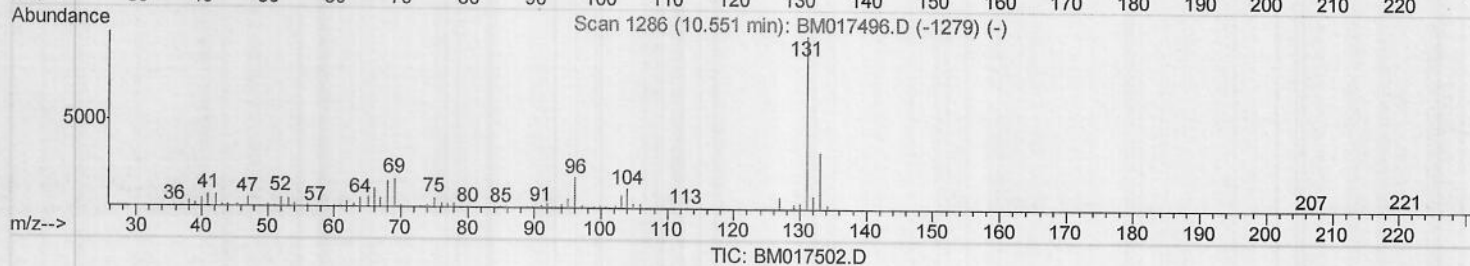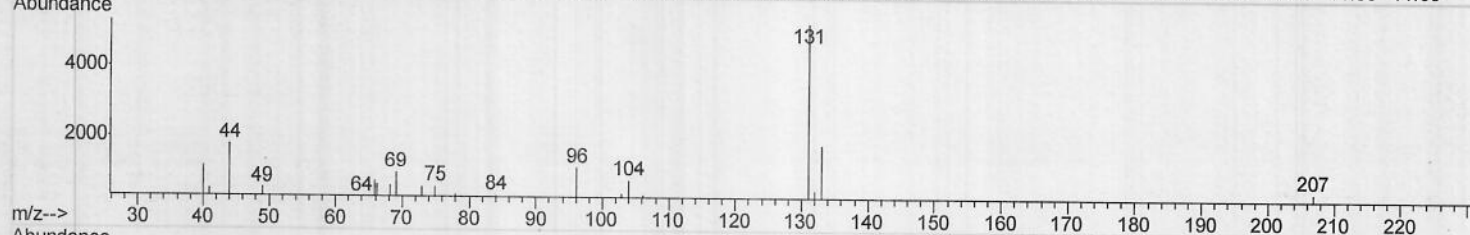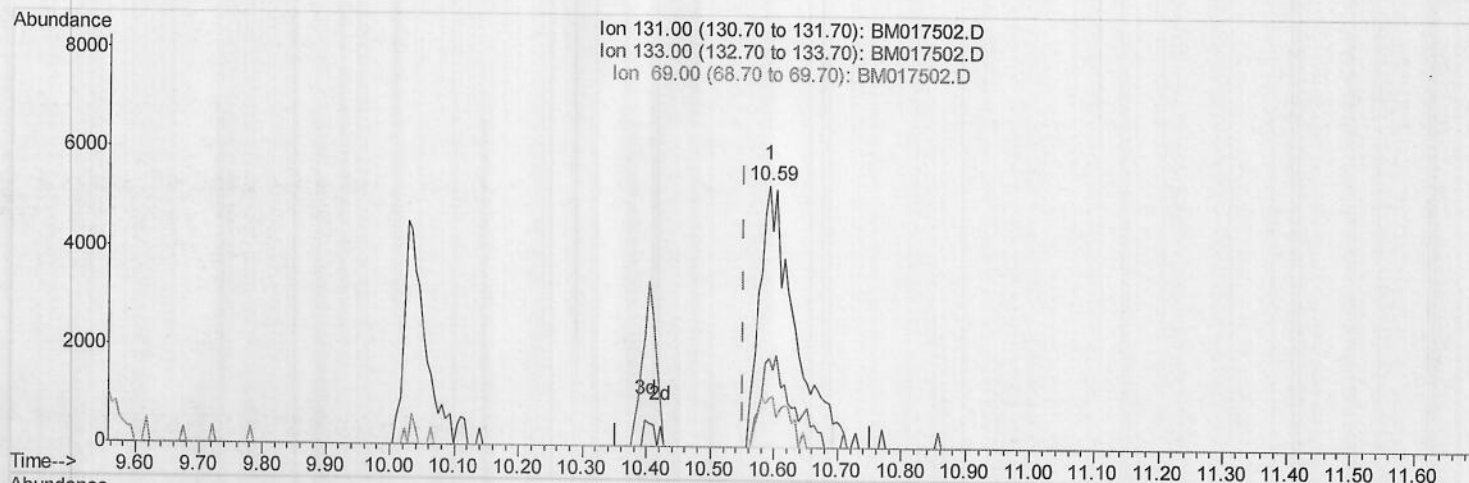

(29) 4-Chloroaniline-d4 (S)

10.592min (+0.041) 2.33ng/ul m

Signature

response 19758

Ion	Exp%	Act%
131.00	100	100
133.00	33.60	34.14
69.00	17.60	18.63
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (Qedit)




Data File : BM017502.D
Acq On : 02 Nov 2018 22:26
Operator : MJ/SJ
Sample : J5802-14
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COBE0

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:05 PM

Quant Time: Nov 03 04:02:44 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 03:58:03 2018
Response via : Initial Calibration

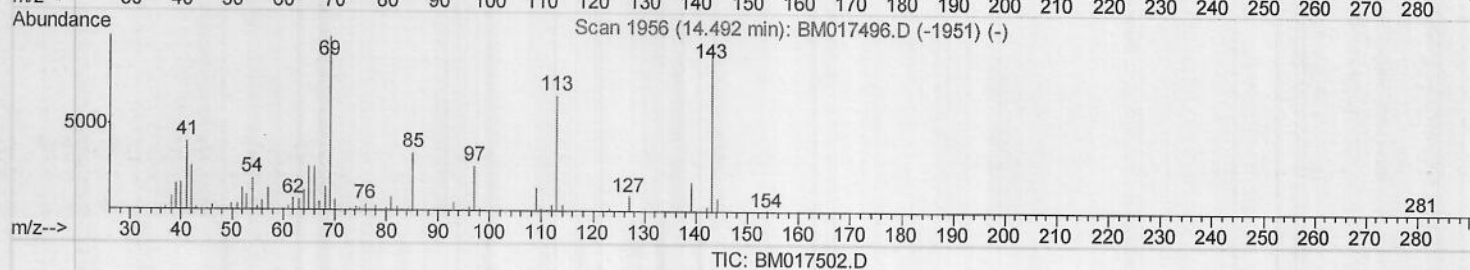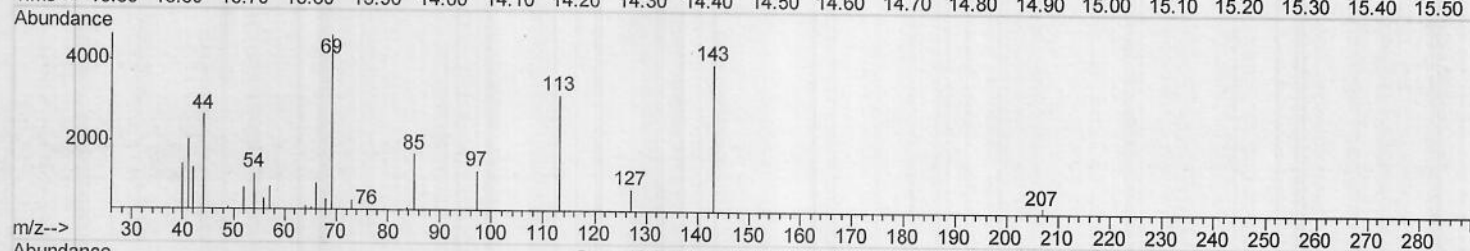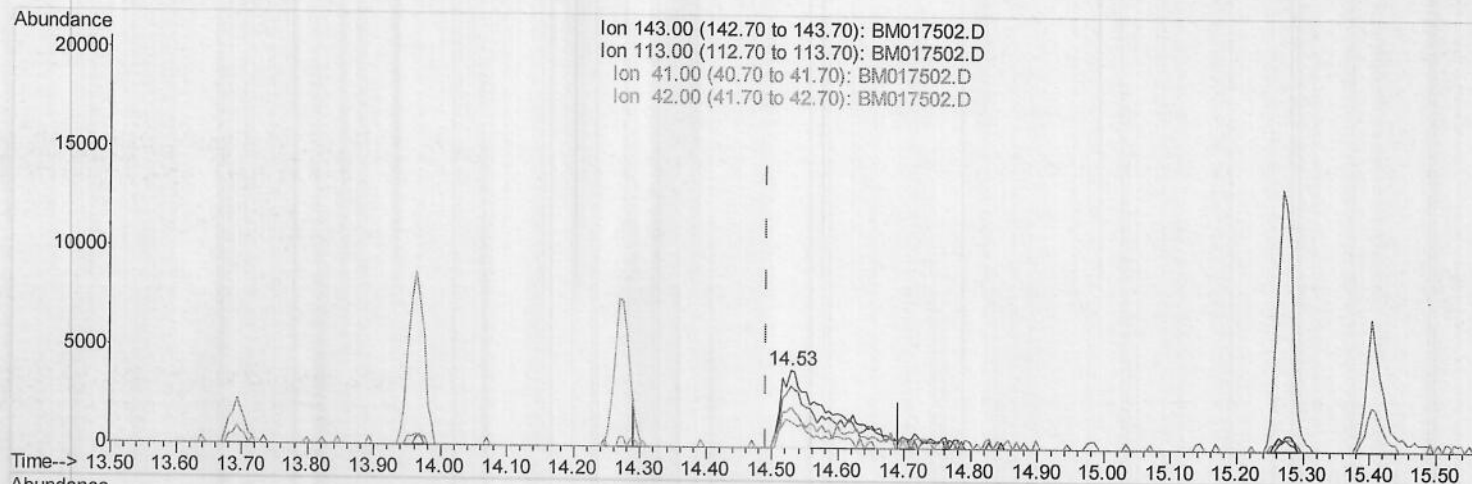

(52) 4-Nitrophenol-d4 (S)

14.527min (+0.035) 1.82ng/ul

response 9711

Ion	Exp%	Act%
143.00	100	100
113.00	74.20	79.93
41.00	39.30	51.60#
42.00	25.10	34.36#

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (Qedit)




Data File : BM017502.D
Acq On : 02 Nov 2018 22:26
Operator : MJ/SJ
Sample : J5802-14
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COBE0

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:05 PM

Quant Time: Nov 03 04:02:44 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 03:58:03 2018
Response via : Initial Calibration

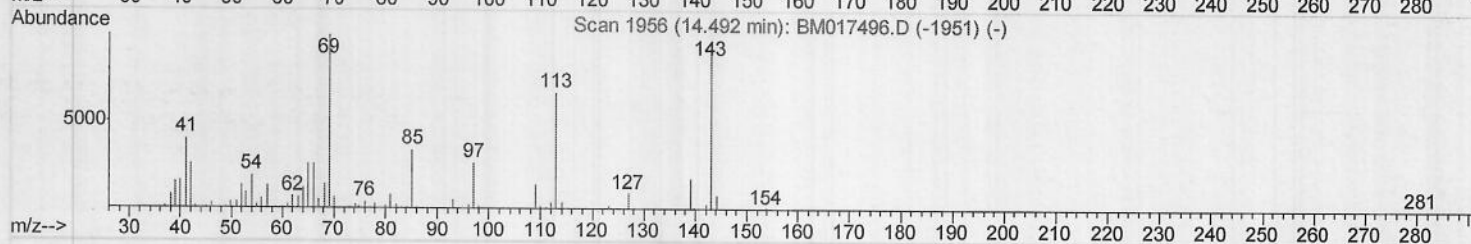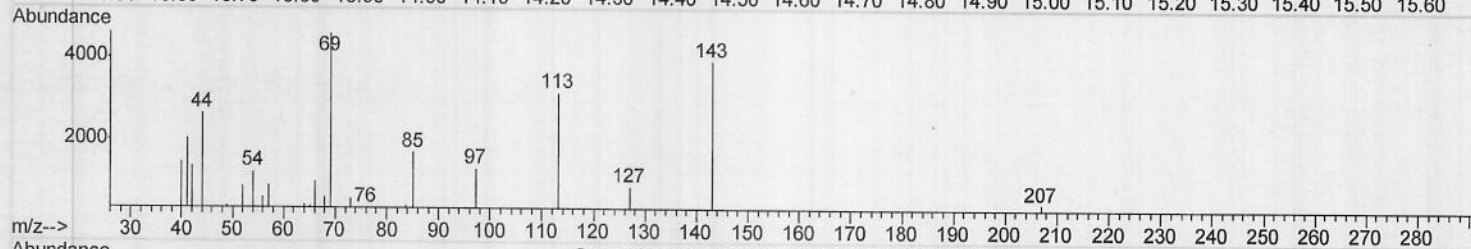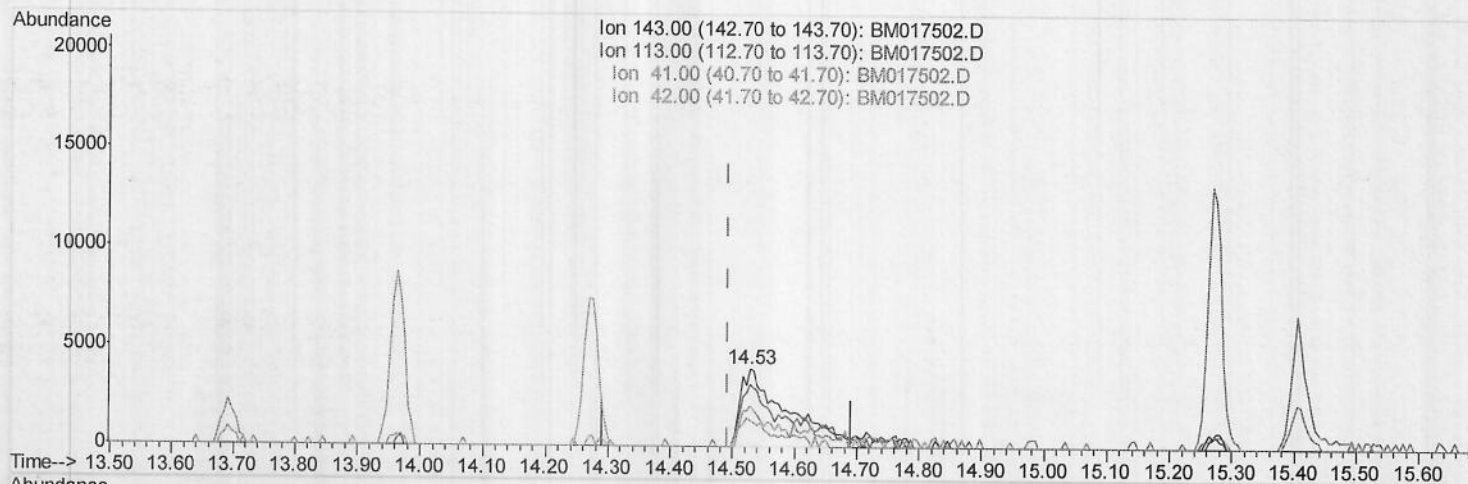

(52) 4-Nitrophenol-d4 (S)

14.527min (+0.035) 3.78ng/ul m

2511/06/18

response 20202

Ion	Exp%	Act%
143.00	100	100
113.00	74.20	79.93
41.00	39.30	51.60#
42.00	25.10	34.36#

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (QT Reviewed)

Data File : BM017502.D
Acq On : 02 Nov 2018 22:26
Operator : MJ/SJ
Sample : J5802-14
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0BE0

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:05 PM

Quant Time: Nov 03 04:19:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 03:58:03 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	155243	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	637021	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	333537	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	687448	20.00	ng/ul	0.00
78) Chrysene-d12	21.23	240	568397	20.00	ng/ul	0.00
86) Perylene-d12	23.42	264	496605	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	5678	1.68	ng/uL	0.00
5) Phenol-d5	6.82	99	98350	6.94	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	265083	32.05	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	283925	25.82	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	172823	15.41	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	162936	32.72	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	177367	31.76	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	286213	27.60	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	19758m)	2.33	ng/ul	0.04
44) Dimethylphthalate-d6	13.69	166	912646	31.91	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	1160204	33.41	ng/ul	0.00
52) 4-Nitrophenol-d4	14.53	143	20202m)	3.78	ng/ul	0.04
58) Fluorene-d10	15.27	176	807331	32.50	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	116450	24.31	ng/ul	0.00
71) Anthracene-d10	17.12	188	1181716	34.73	ng/ul	0.00
79) Pyrene-d10	19.43	212	1202914	45.68	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.28	264	966319	36.85	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

} SJ11/06/18