

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (QT Reviewed)


Data File : BM017508.D
Acq On : 03 Nov 2018 02:03
Operator : MJ/SJ
Sample : J5704-15
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40F5

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:12 PM

Quant Time: Nov 03 04:48:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 03:58:03 2018
Response via : Initial Calibration

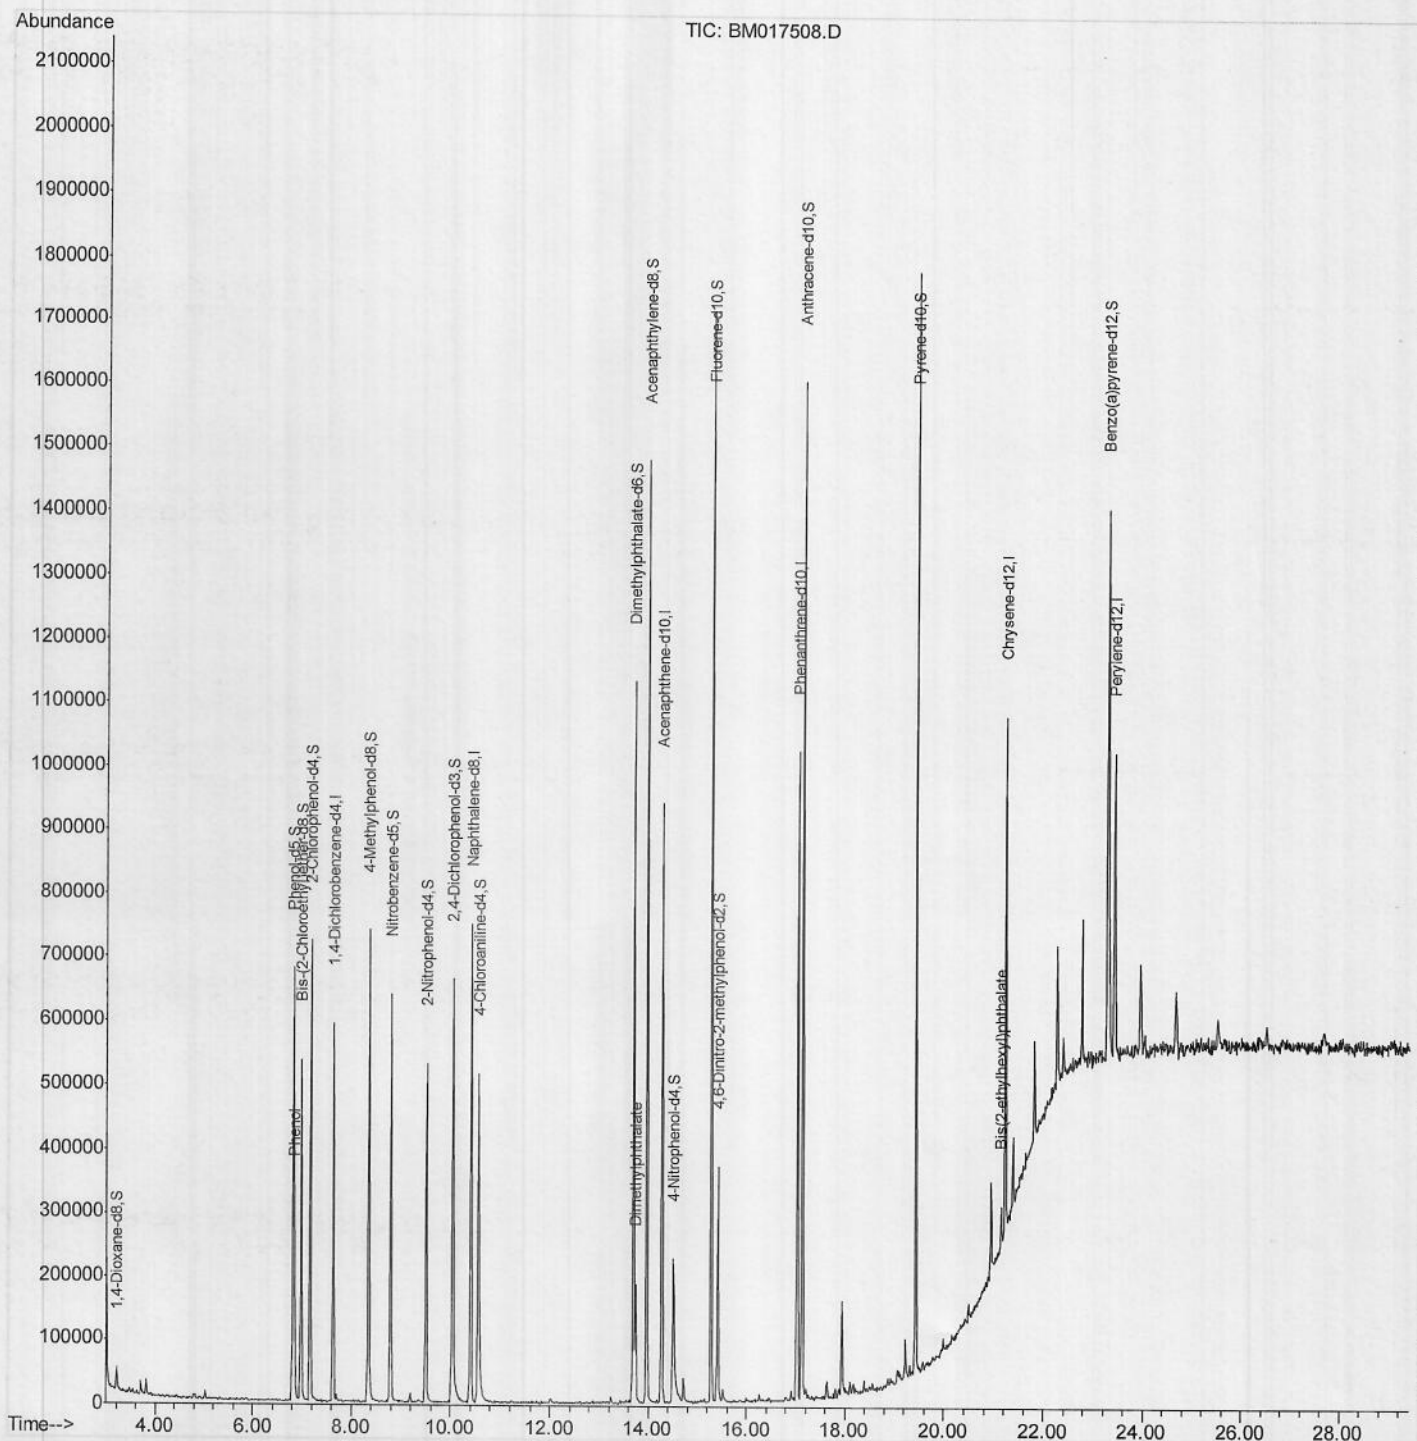

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (Qedit)




Data File : BM017508.D
Acq On : 03 Nov 2018 02:03
Operator : MJ/SJ
Sample : J5704-15
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40F5

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:12 PM

Quant Time: Nov 03 04:04:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 03:58:03 2018
Response via : Initial Calibration

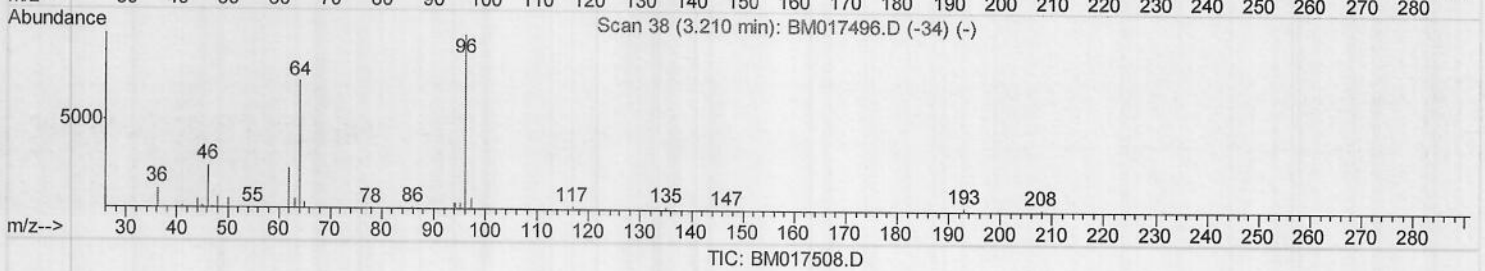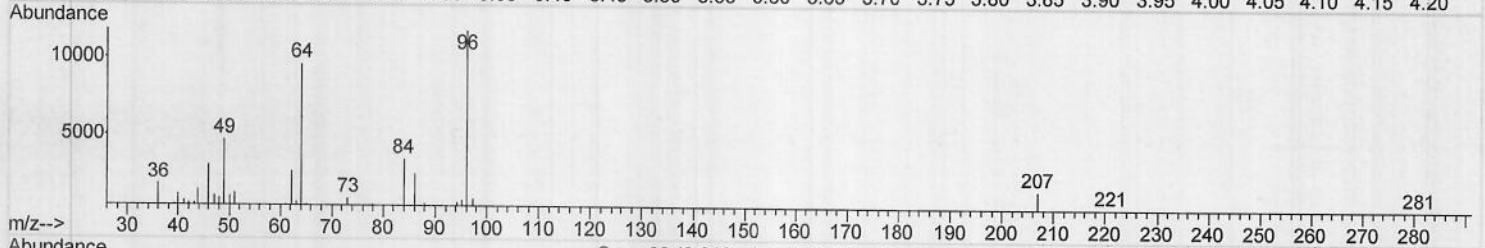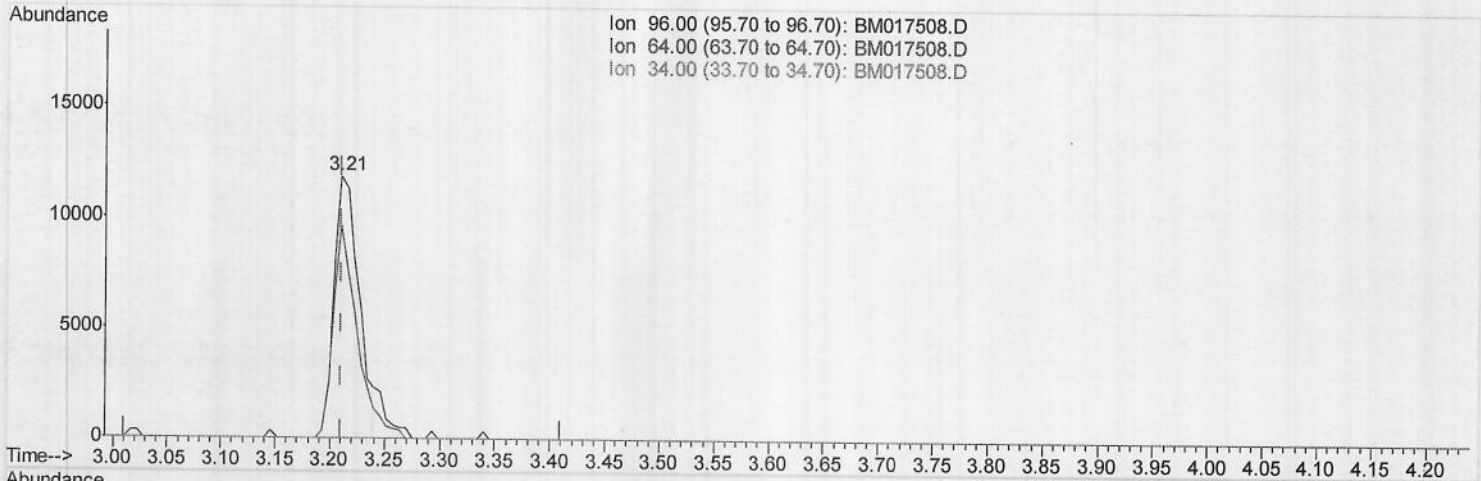

(3) 1,4-Dioxane-d8 (S)

3.210min (-0.000) 5.60ng/uL

response 18756

Ion	Exp%	Act%
96.00	100	100
64.00	78.00	81.62
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (Qedit)




Data File : BM017508.D
Acq On : 03 Nov 2018 02:03
Operator : MJ/SJ
Sample : J5704-15
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
A40F5

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:12 PM

Quant Time: Nov 03 04:04:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 03:58:03 2018
Response via : Initial Calibration

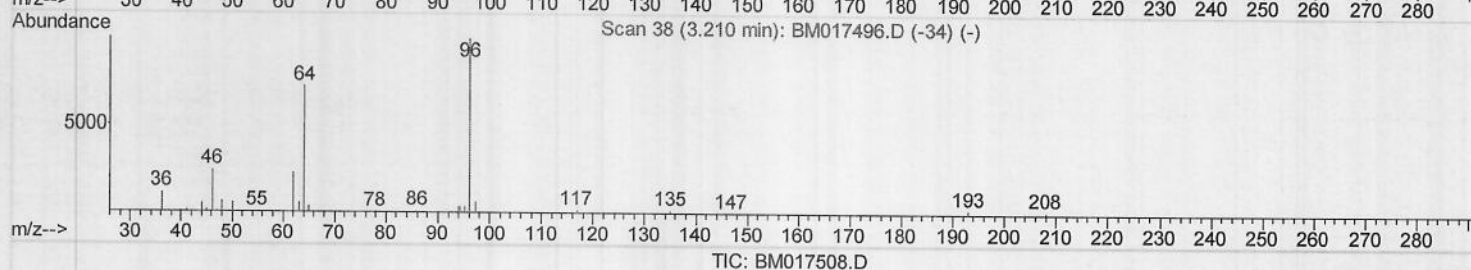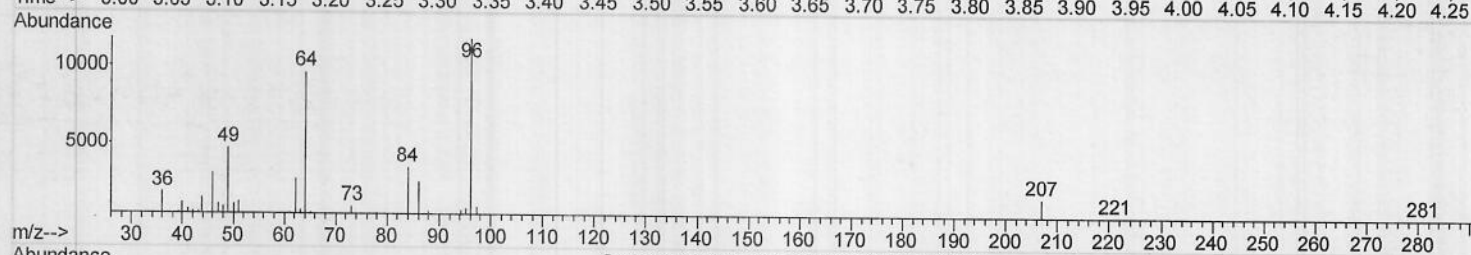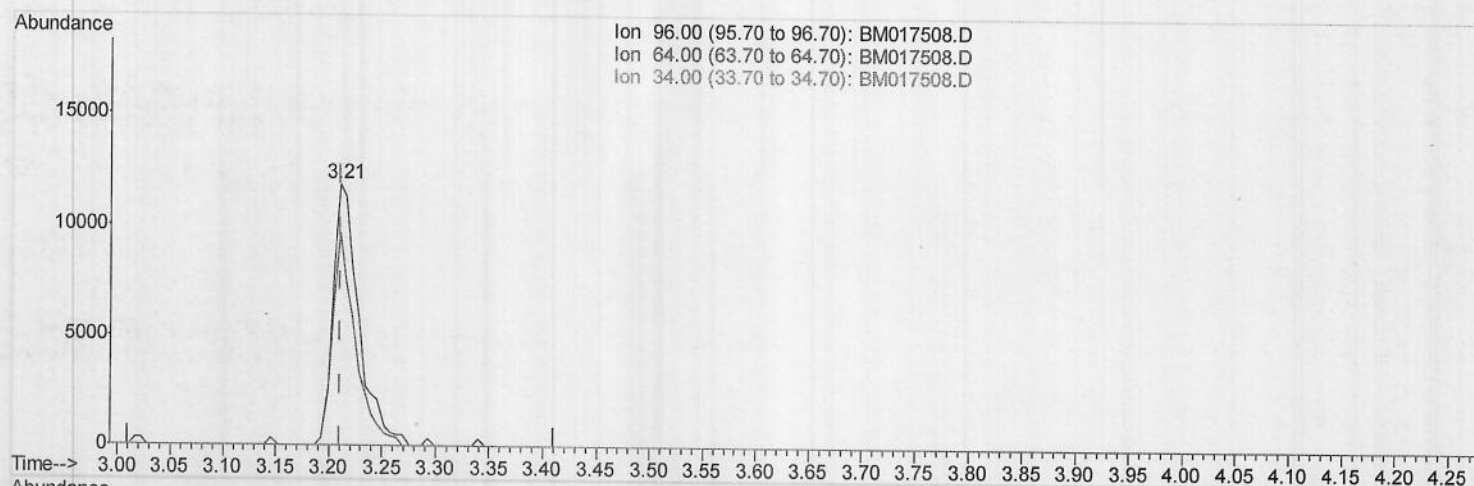

(3) 1,4-Dioxane-d8 (S)

3.210min (-0.000) 6.08ng/uL m

J5711/06/18

response 20355

Ion	Exp%	Act%
96.00	100	100
64.00	78.00	81.62
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
 Quantitation Report (Qedit)
 Data File : BM017508.D
 Acq On : 03 Nov 2018 02:03
 Operator : MJ/SJ
 Sample : J5704-15
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A40F5

Manual Integrations
 APPROVED

Sohil
 11/5/2018 4:06:12 PM

Quant Time: Nov 03 04:04:12 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Nov 03 03:58:03 2018
 Response via : Initial Calibration

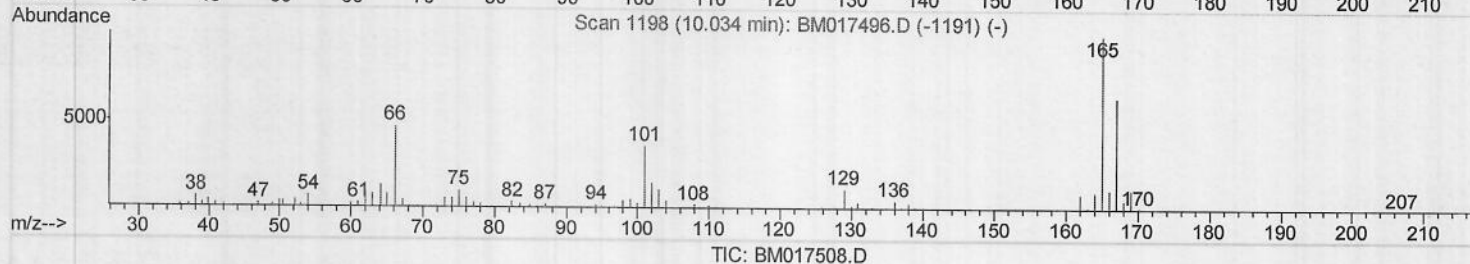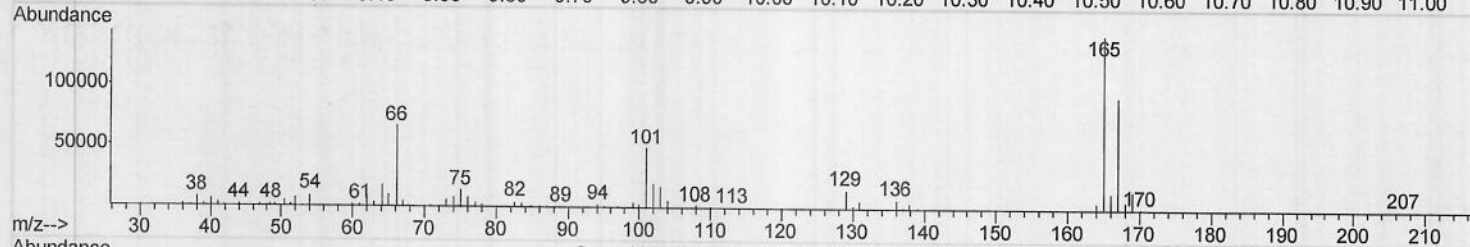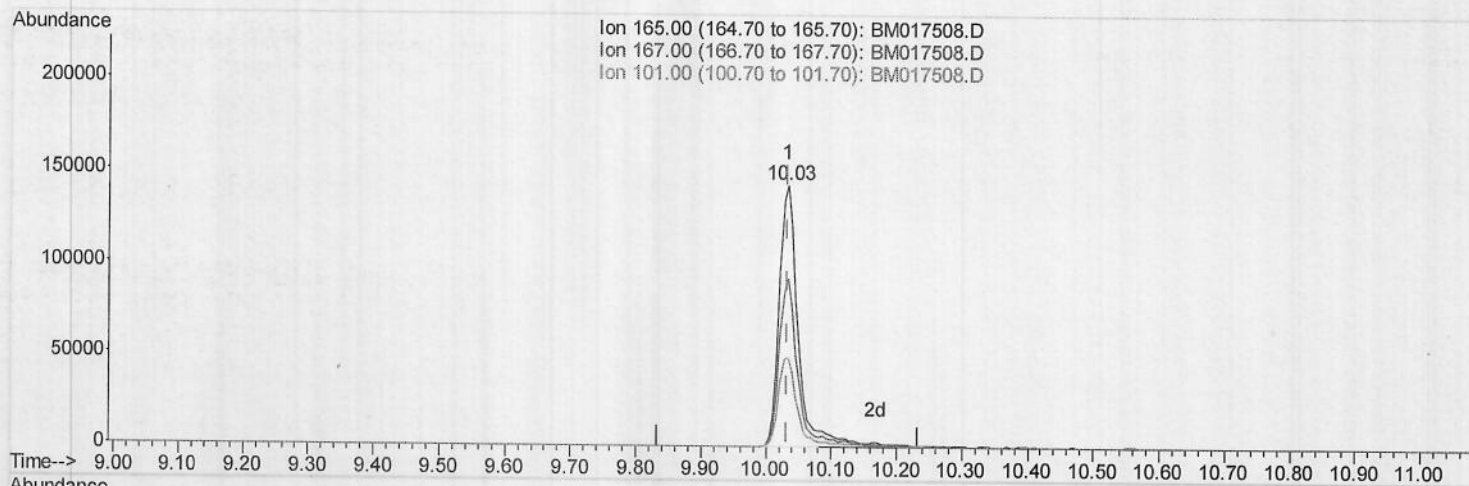

(26) 2,4-Dichlorophenol-d3 (S)

10.034min (-0.000) 26.64ng/ul

response 267405

Ion	Exp%	Act%
165.00	100	100
167.00	63.60	64.51
101.00	34.30	34.21
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (Qedit)




Data File : BM017508.D
Acq On : 03 Nov 2018 02:03
Operator : MJ/SJ
Sample : J5704-15
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40F5

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:12 PM

Quant Time: Nov 03 04:04:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 03:58:03 2018
Response via : Initial Calibration

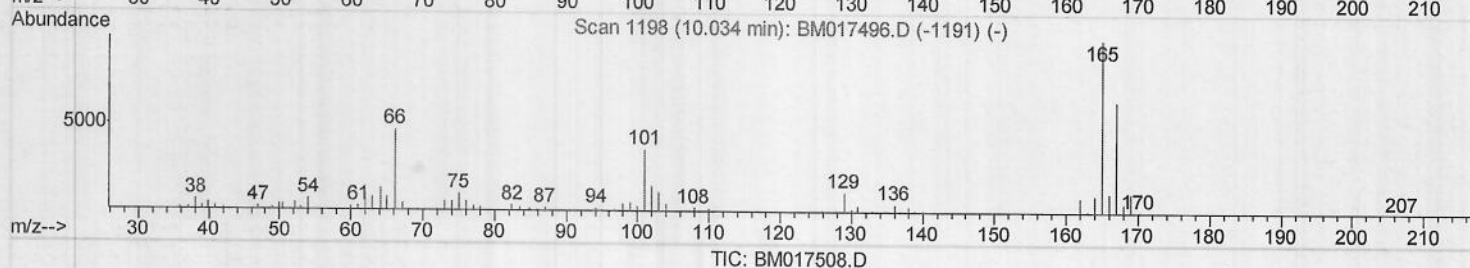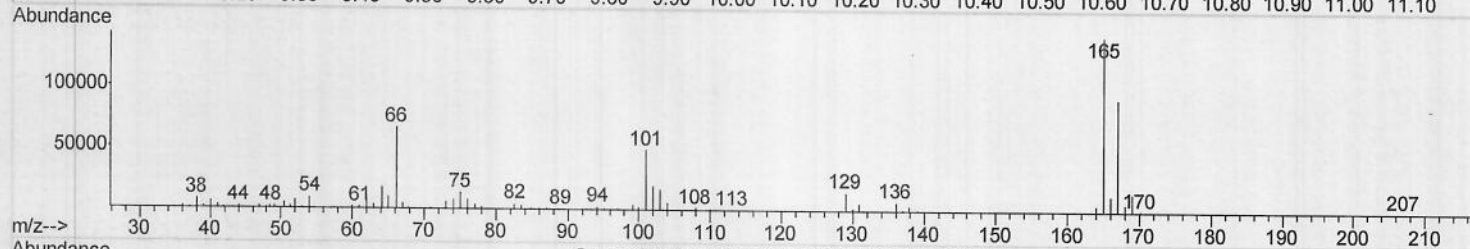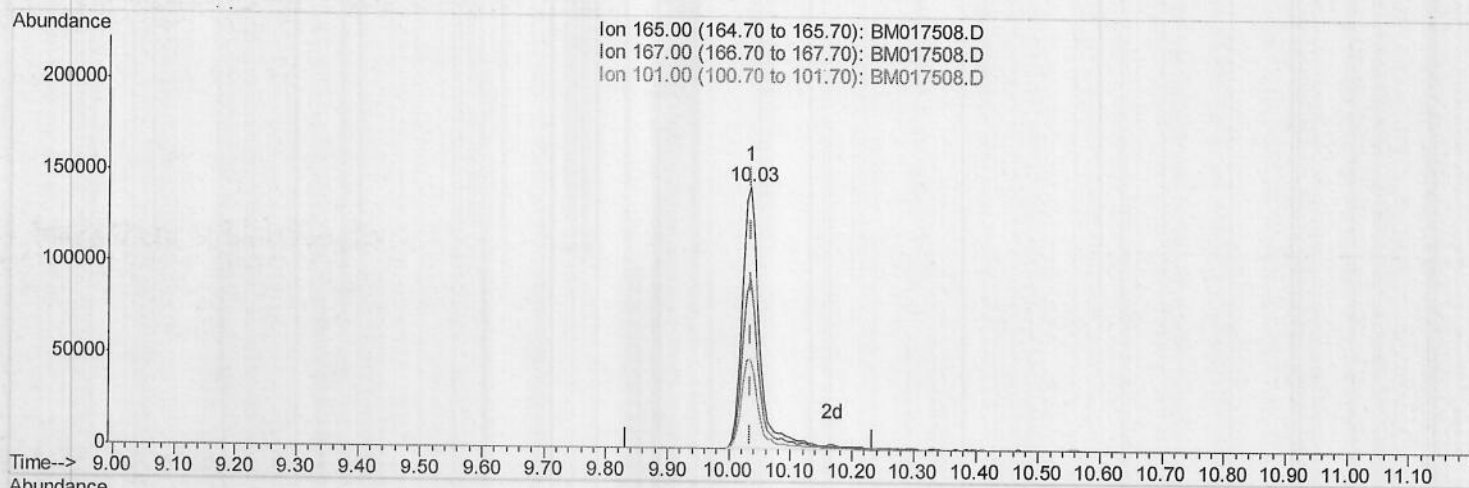

(26) 2,4-Dichlorophenol-d3 (S)

10.034min (-0.000) 29.10ng/ul m)SJ11/06/18

response 292094

Ion	Exp%	Act%
165.00	100	100
167.00	63.60	64.51
101.00	34.30	34.21
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (Qedit)




Data File : BM017508.D
Acq On : 03 Nov 2018 02:03
Operator : MJ/SJ
Sample : J5704-15
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40F5

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:12 PM

Quant Time: Nov 03 04:04:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 03:58:03 2018
Response via : Initial Calibration

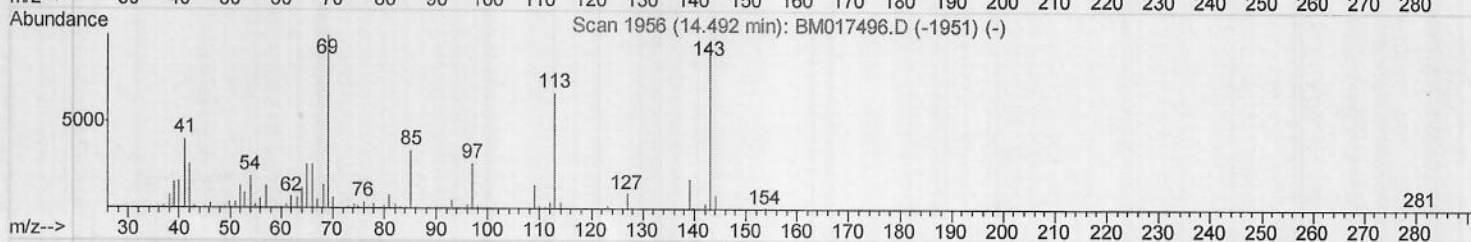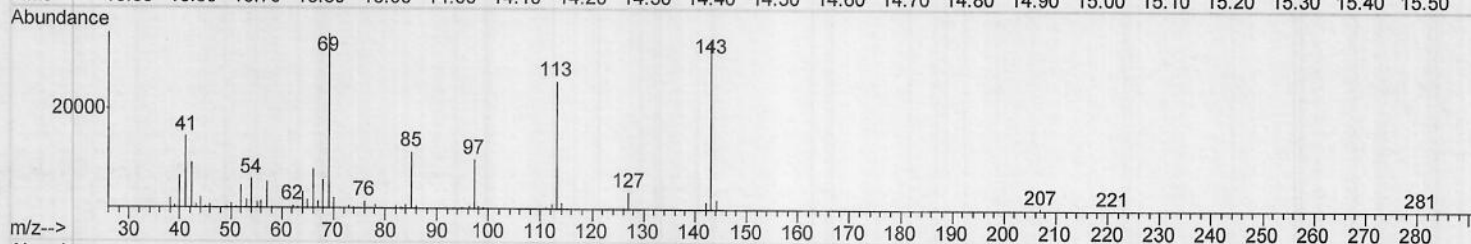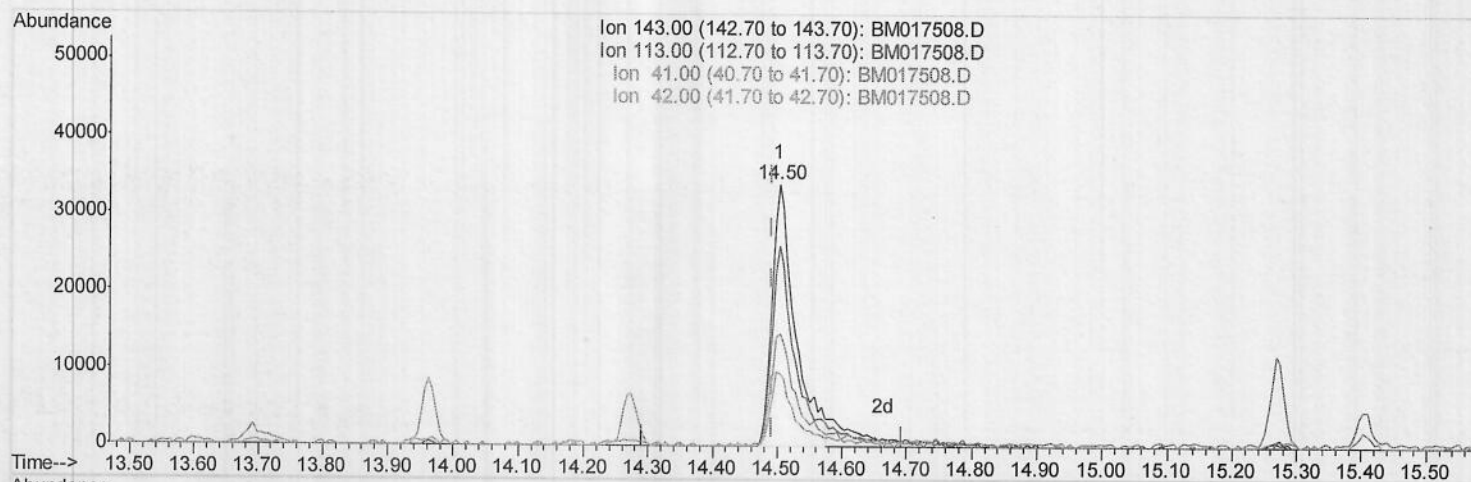

(52) 4-Nitrophenol-d4 (S)
14.504min (+0.012) 17.30ng/ul
response 83887
Ion Exp% Act%
143.00 100 100
113.00 74.20 76.42
41.00 39.30 43.29
42.00 25.10 27.91

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (Qedit)




Data File : BM017508.D
Acq On : 03 Nov 2018 02:03
Operator : MJ/SJ
Sample : J5704-15
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40F5

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:12 PM

Quant Time: Nov 03 04:04:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 03:58:03 2018
Response via : Initial Calibration

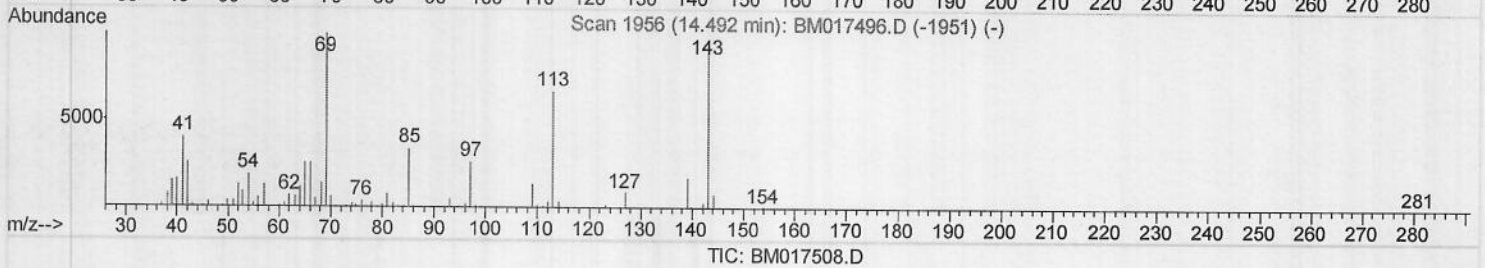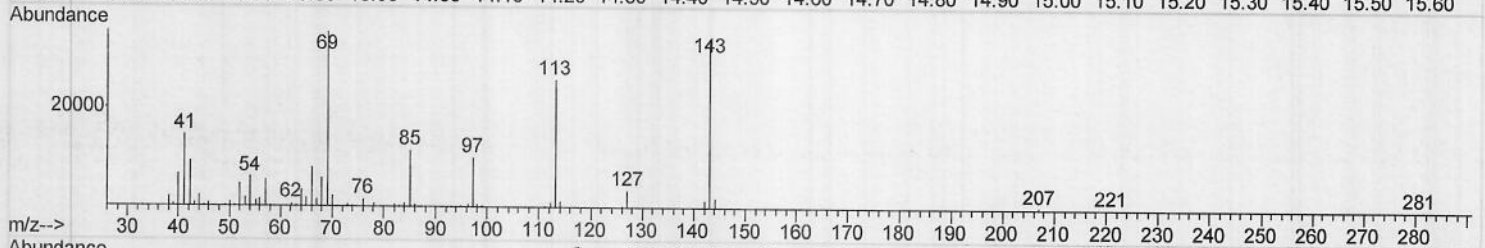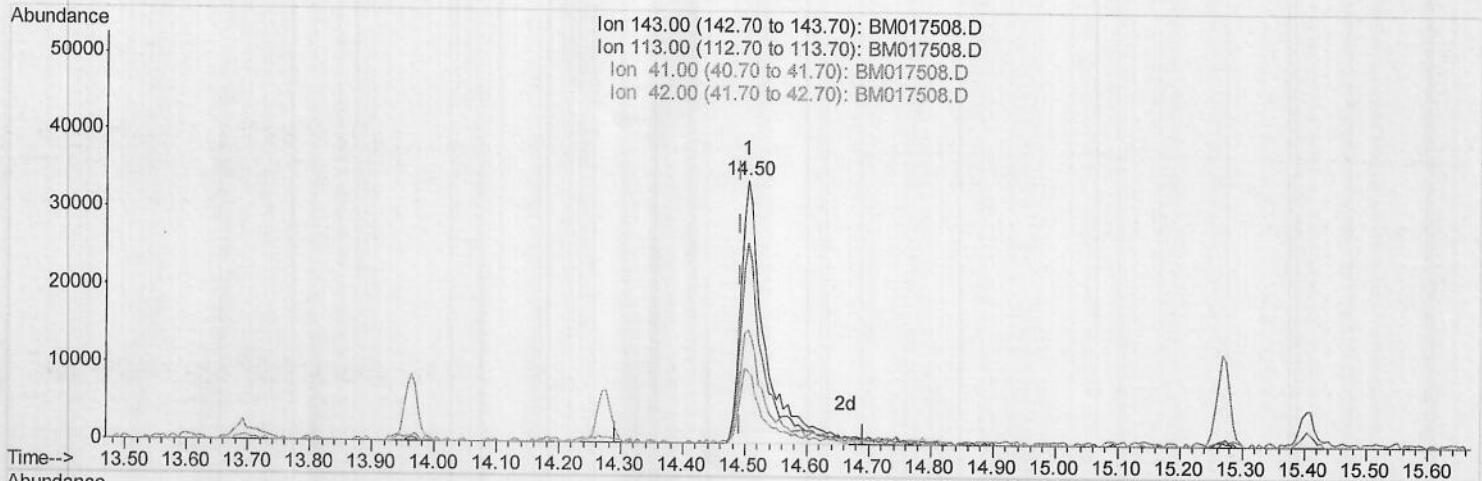

(52) 4-Nitrophenol-d4 (S)

14.504min (+0.012) 19.50ng/ul m

25/11/06/11

response 94561

Ion	Exp%	Act%
143.00	100	100
113.00	74.20	76.42
41.00	39.30	43.29
42.00	25.10	27.91

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\

Quantitation Report (QT Reviewed)

Data File : BM017508.D

Acq On : 03 Nov 2018 02:03

Operator : MJ/SJ

Sample : J5704-15

Misc :

ALS Vial : 23 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

A40F5

Manual Integrations
APPROVED

Sohil

11/5/2018 4:06:12 PM

Quant Time: Nov 03 04:48:35 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Sat Nov 03 03:58:03 2018

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	154053	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	616603	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	302722	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	582961	20.00	ng/ul	0.00
78) Chrysene-d12	21.23	240	402400	20.00	ng/ul	0.00
86) Perylene-d12	23.42	264	346630	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.21	96	20355m)	6.08	ng/uL	0.00
5) Phenol-d5	6.81	99	406861	28.91	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	249807	30.44	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	334612	30.67	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	294982	26.51	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	151782	31.49	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	162335	30.03	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	292094m)	29.10	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	345778	42.19	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	773974	29.81	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	1018441	32.31	ng/ul	0.00
52) 4-Nitrophenol-d4	14.50	143	94561m)	19.50	ng/ul	0.01
58) Fluorene-d10	15.27	176	687258	30.48	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	85588	21.07	ng/ul	0.00
71) Anthracene-d10	17.13	188	898349	31.13	ng/ul	0.00
79) Pyrene-d10	19.43	212	879817	47.19	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.28	264	611033	33.38	ng/ul	0.00

} SJ11/06/18

Target Compounds

					Qvalue
6) Phenol	6.84	94	93153	6.667 ng/ul	93
45) Dimethylphthalate	13.74	163	120530	4.792 ng/ul#	98
84) Bis(2-ethylhexyl)phthalate	21.15	149	17170	1.260 ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed