

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (QT Reviewed)


Data File : BM017510.D
Acq On : 03 Nov 2018 03:15
Operator : MJ/SJ
Sample : J5704-07
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40H1

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:15 PM

Quant Time: Nov 03 05:12:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 03:58:03 2018
Response via : Initial Calibration

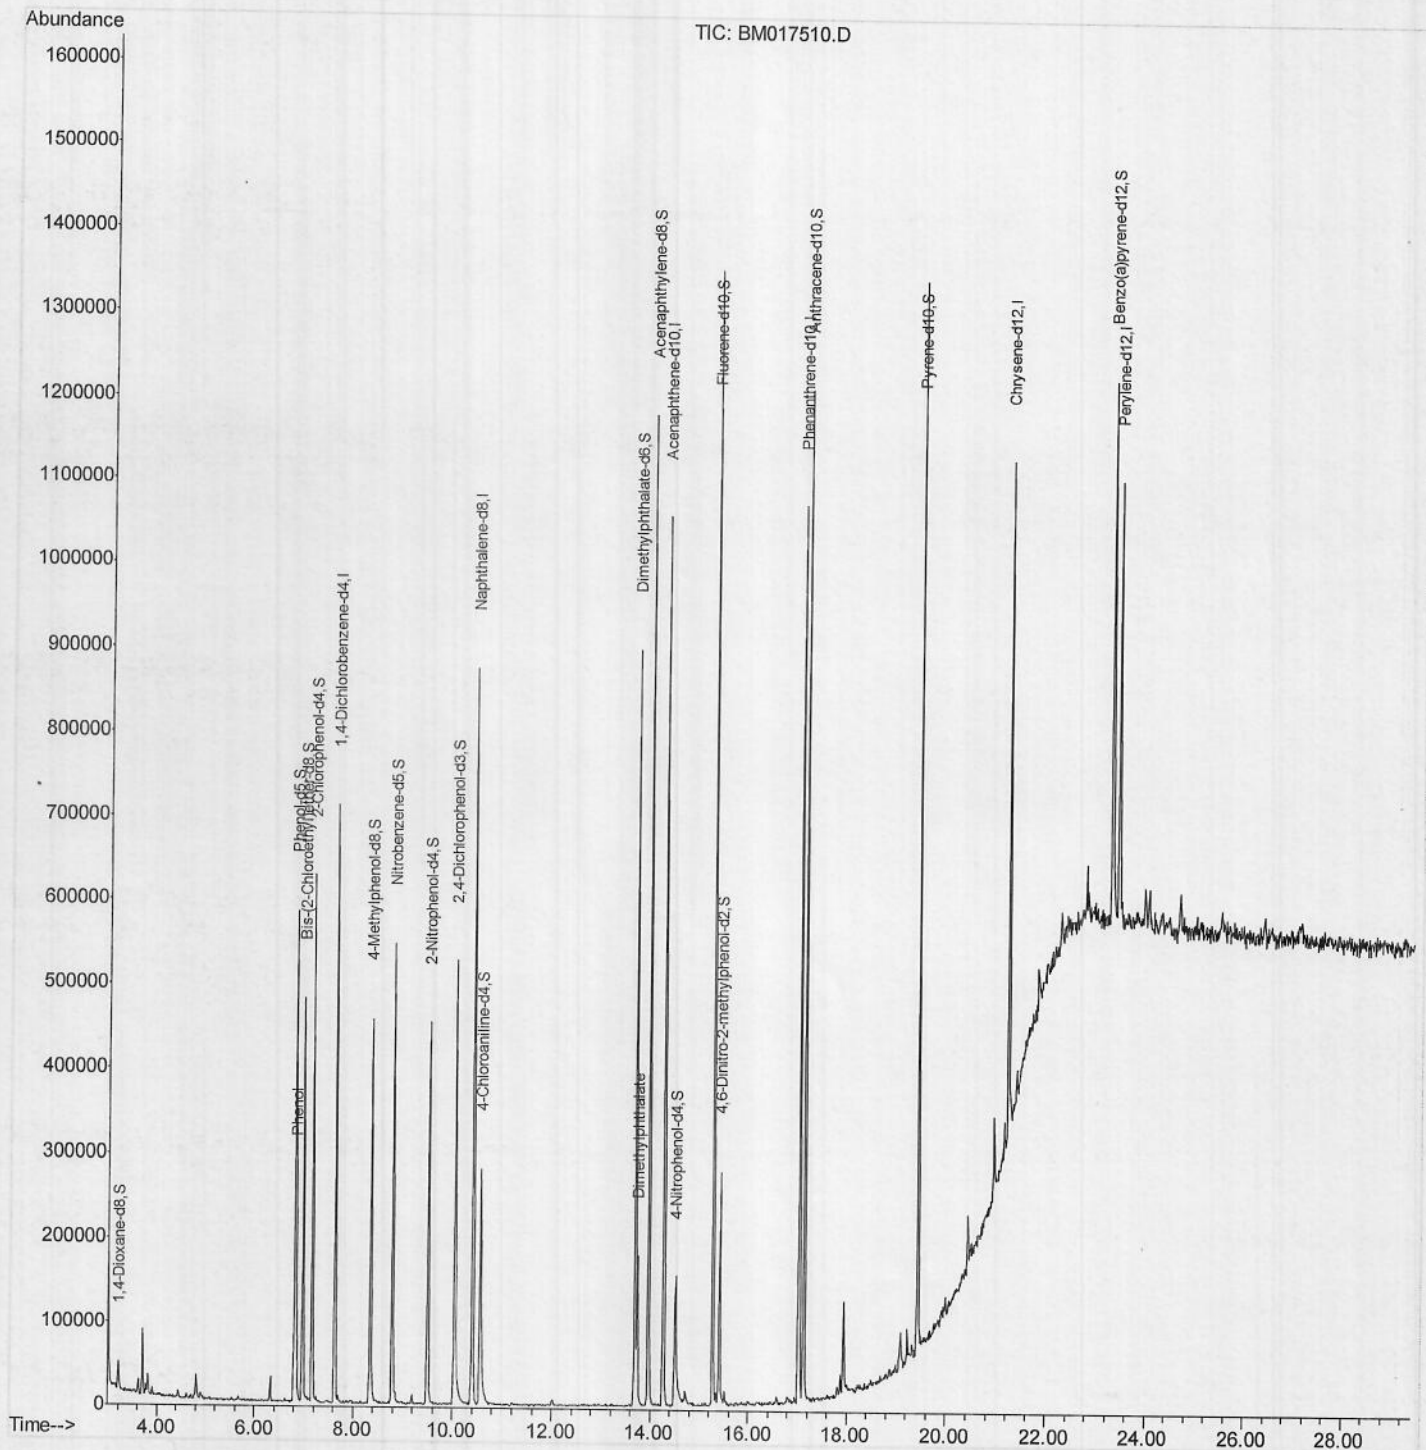

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (Qedit)




Data File : BM017488.D
Acq On : 02 Nov 2018 09:38
Operator : MJ/SJ
Sample : J5701-13ME
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40H1

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:15 PM

Quant Time: Nov 03 02:33:15 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 02:25:47 2018
Response via : Initial Calibration

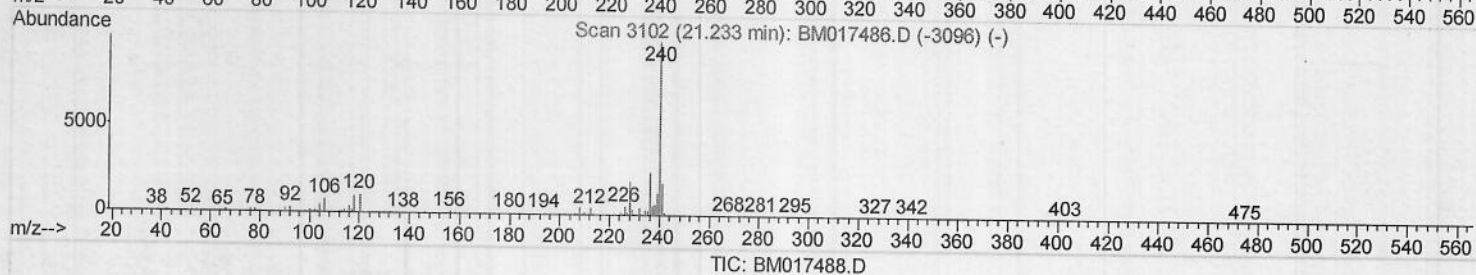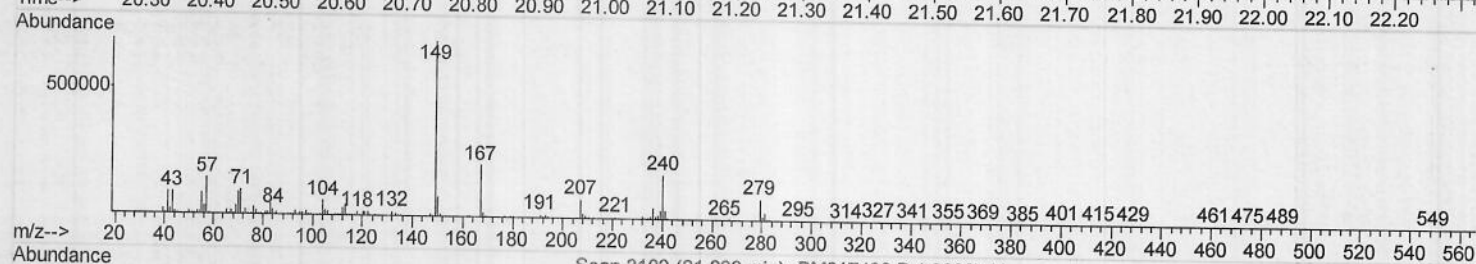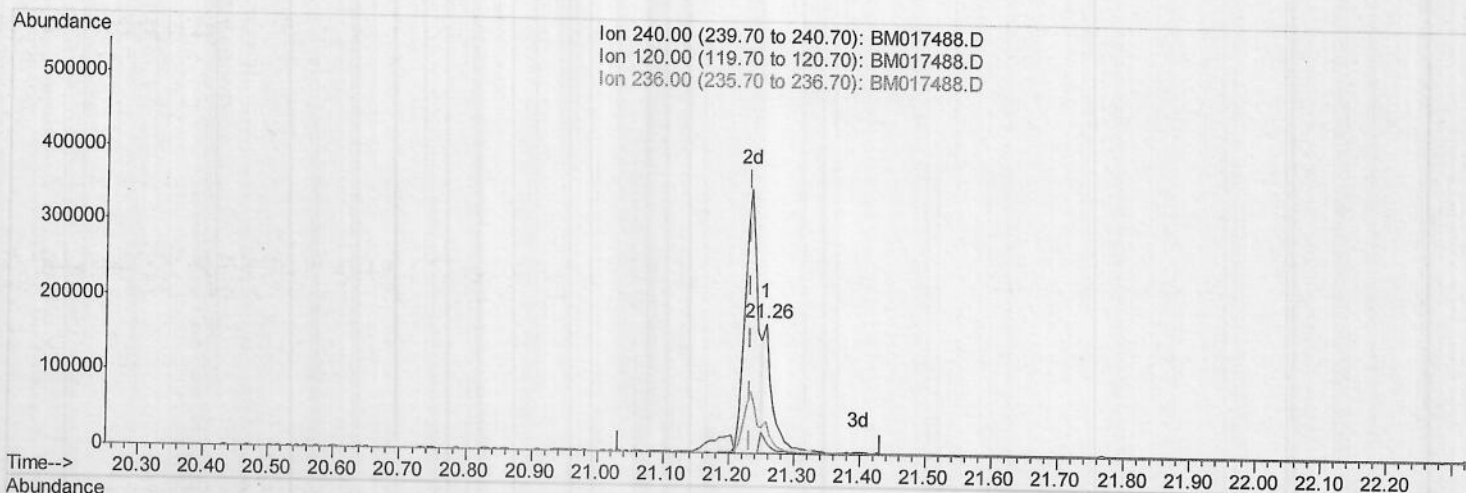

(78) Chrysene-d12 (I)

21.256min (+0.024) 20.00ng/ul

response 148907

Ion	Exp%	Act%
240.00	100	100
120.00	9.50	9.14
236.00	25.00	25.16
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (Qedit)


Data File : BM017488.D
Acq On : 02 Nov 2018 09:38
Operator : MJ/SJ
Sample : J5701-13ME
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40H1

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:15 PM

Quant Time: Nov 03 02:33:15 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 02:25:47 2018
Response via : Initial Calibration

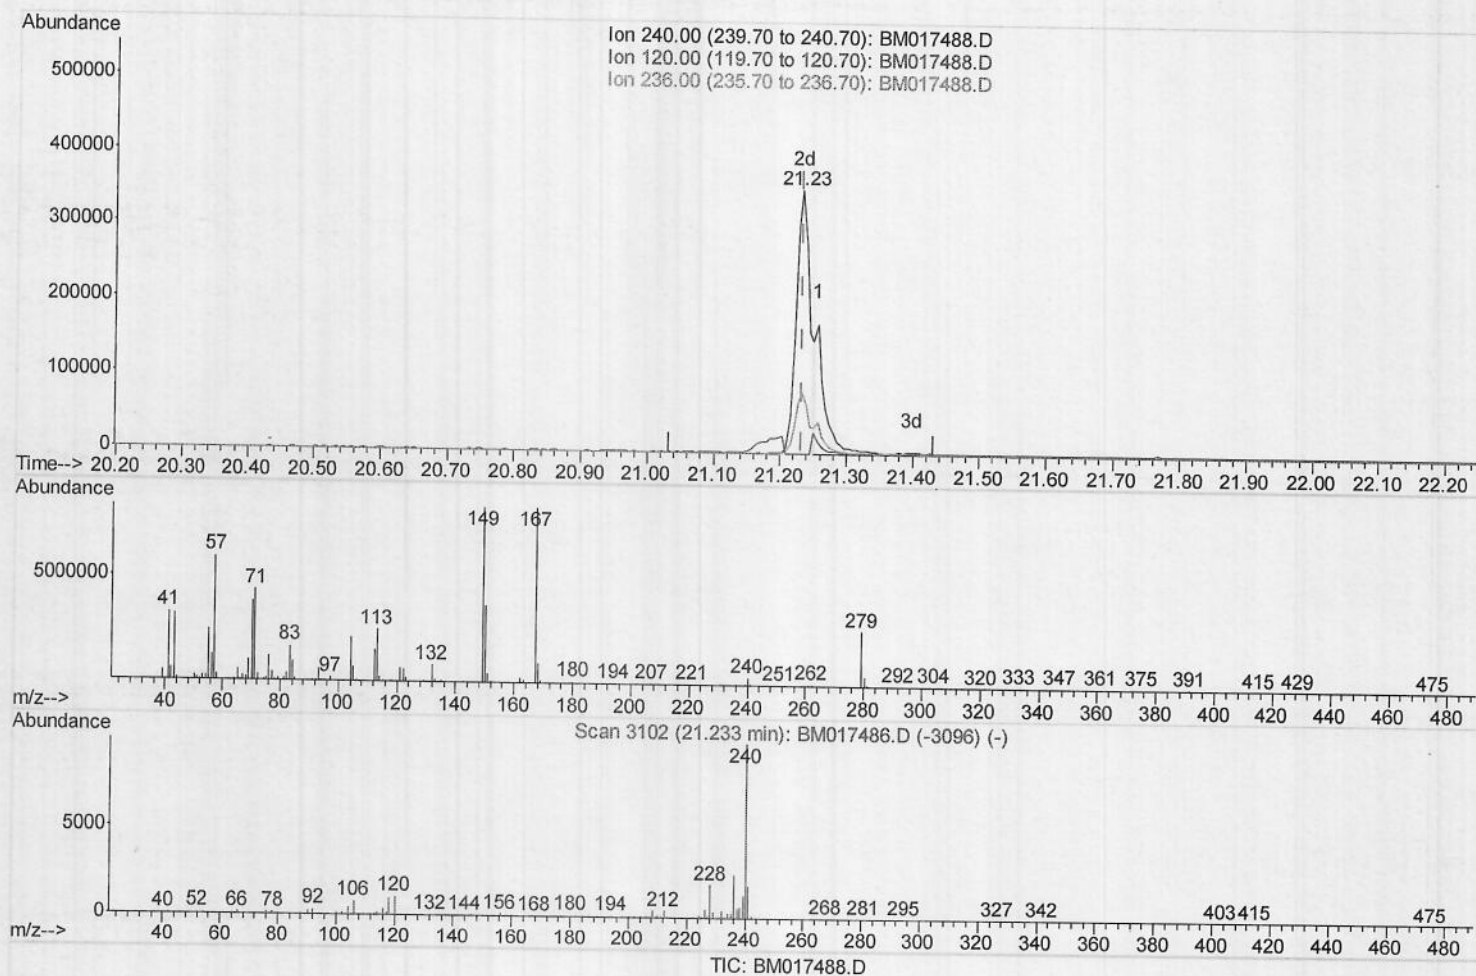

(78) Chrysene-d12 (I)

21.233min (-0.000) 20.00ng/ul m J511/06/18

response 511424

Ion	Exp%	Act%
240.00	100	100
120.00	9.50	0.00#
236.00	25.00	23.72
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (Qedit)




Data File : BM017488.D
Acq On : 02 Nov 2018 09:38
Operator : MJ/SJ
Sample : J5701-13ME
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40H1

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:15 PM

Quant Time: Nov 03 02:43:00 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 02:25:47 2018
Response via : Initial Calibration

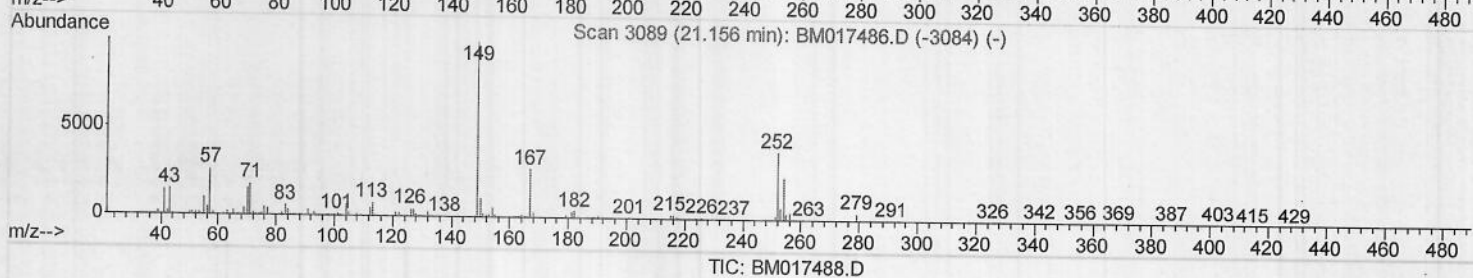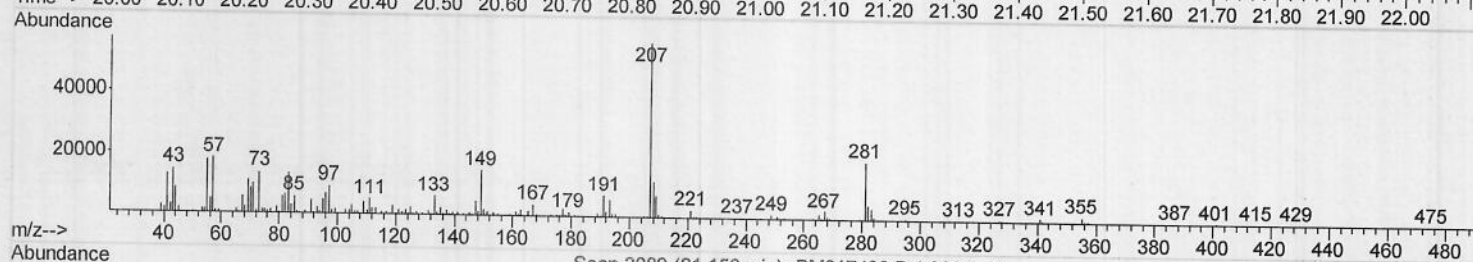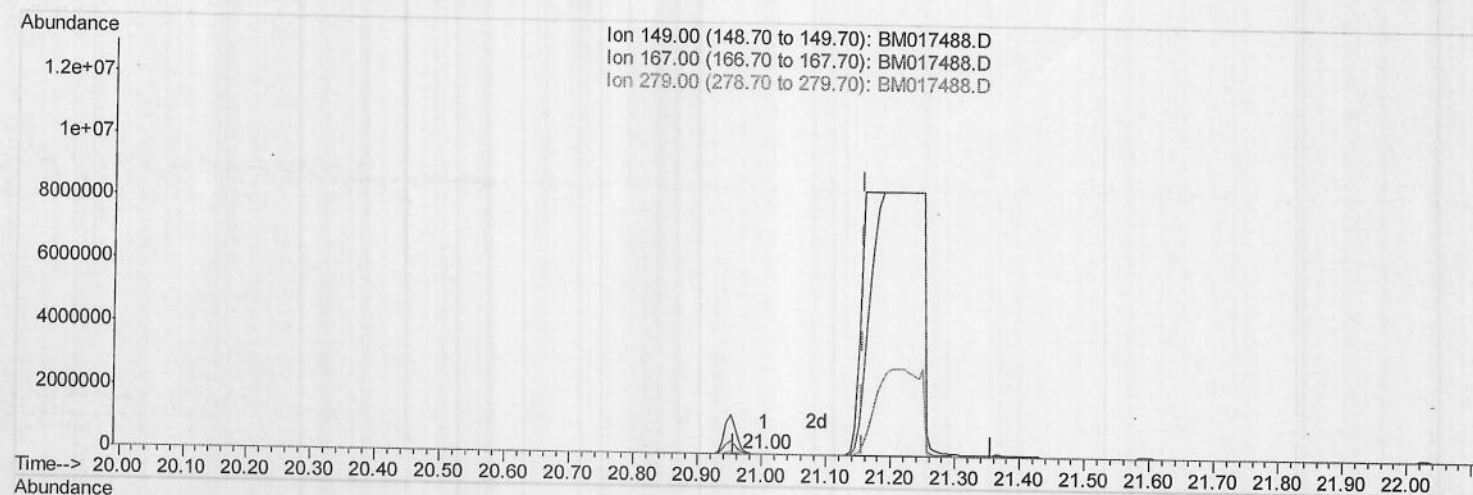

TIC: BM017488.D

(84) Bis(2-ethylhexyl)phthalate

21.003min (-0.153) 0.54ng/ul

response 9401

Ion	Exp%	Act%
149.00	100	100
167.00	28.80	26.14
279.00	5.10	5.32
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (Qedit)




Data File : BM017488.D
Acq On : 02 Nov 2018 09:38
Operator : MJ/SJ
Sample : J5701-13ME
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40H1

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:15 PM

Quant Time: Nov 03 02:43:00 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 02:25:47 2018
Response via : Initial Calibration

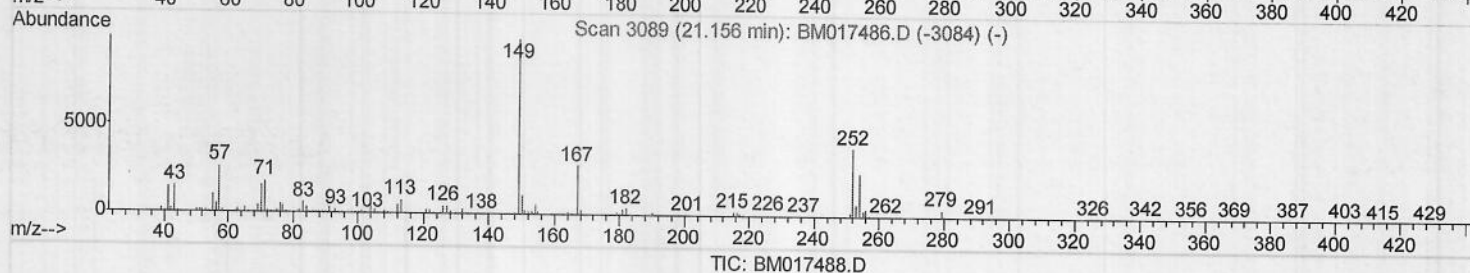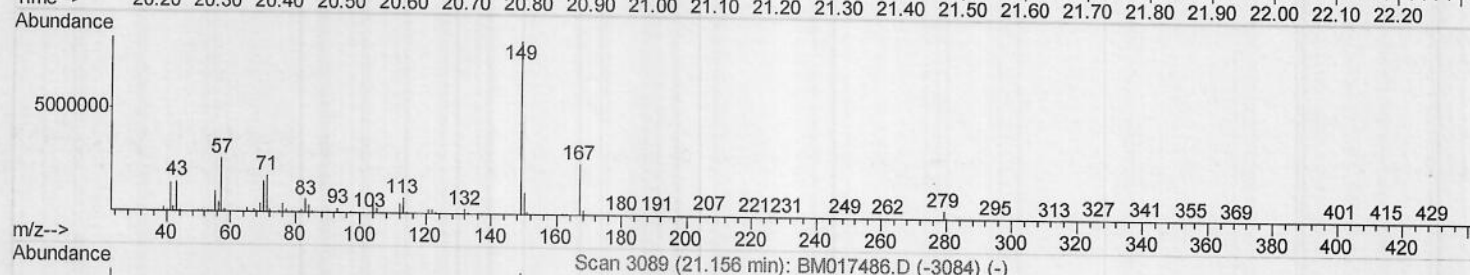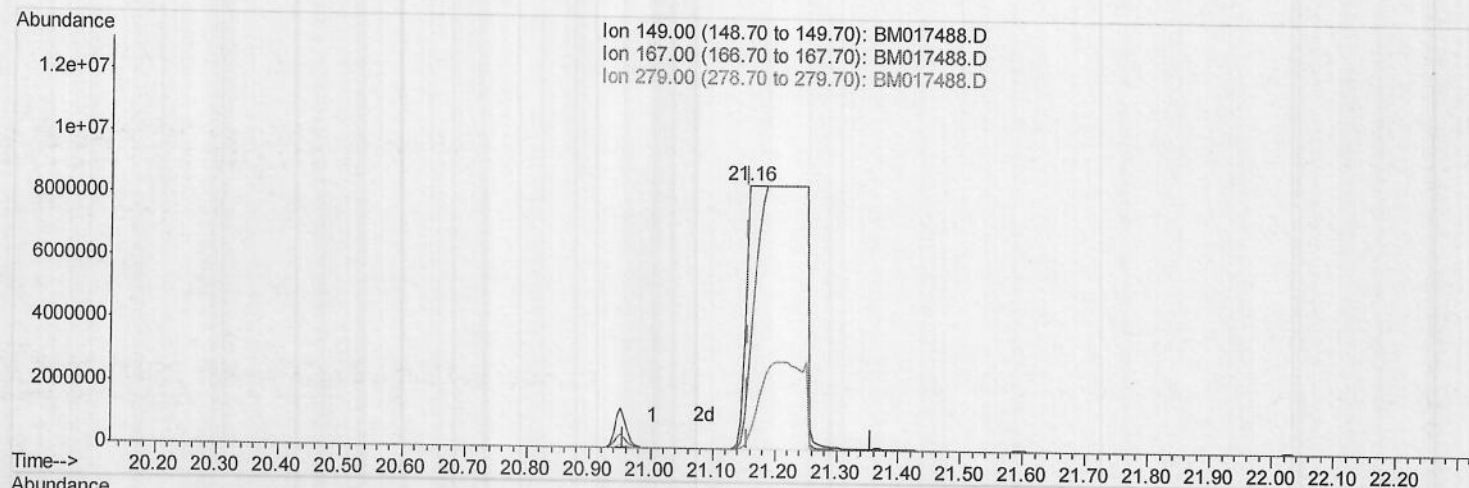

(84) Bis(2-ethylhexyl)phthalate

21.156min (-0.000) 3040.28ng/ul m

J5701/06/18

response 52673514

Ion	Exp%	Act%
149.00	100	100
167.00	28.80	29.45
279.00	5.10	4.51
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM110218\
 Data File : BM017488.D
 Acq On : 02 Nov 2018 09:38
 Operator : MJ/SJ
 Sample : J5701-13ME
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A40H1

Quant Time: Nov 03 01:43:30 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Nov 03 02:25:47 2018
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 11/5/2018 4:06:15 PM

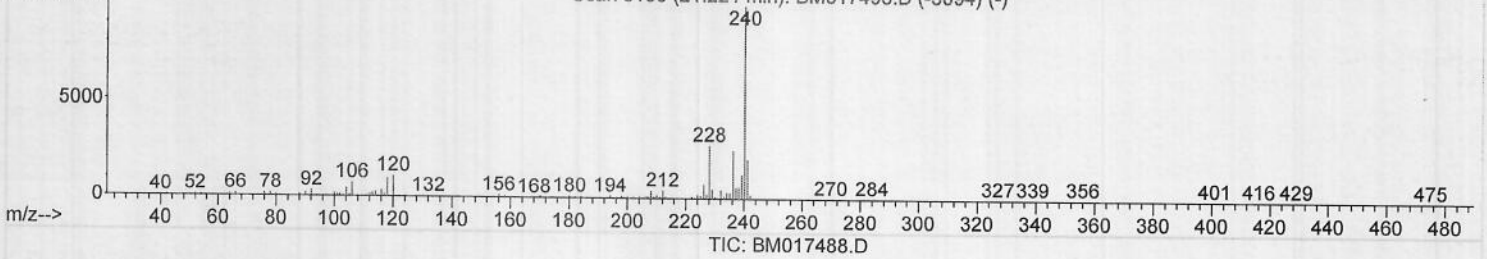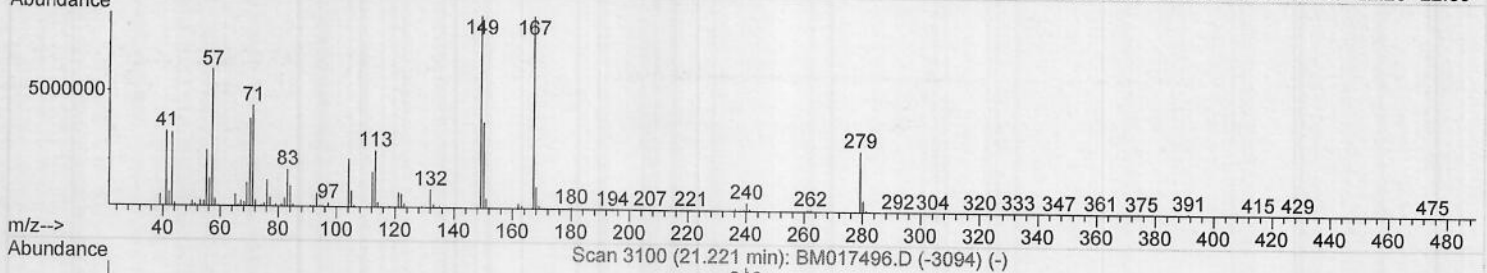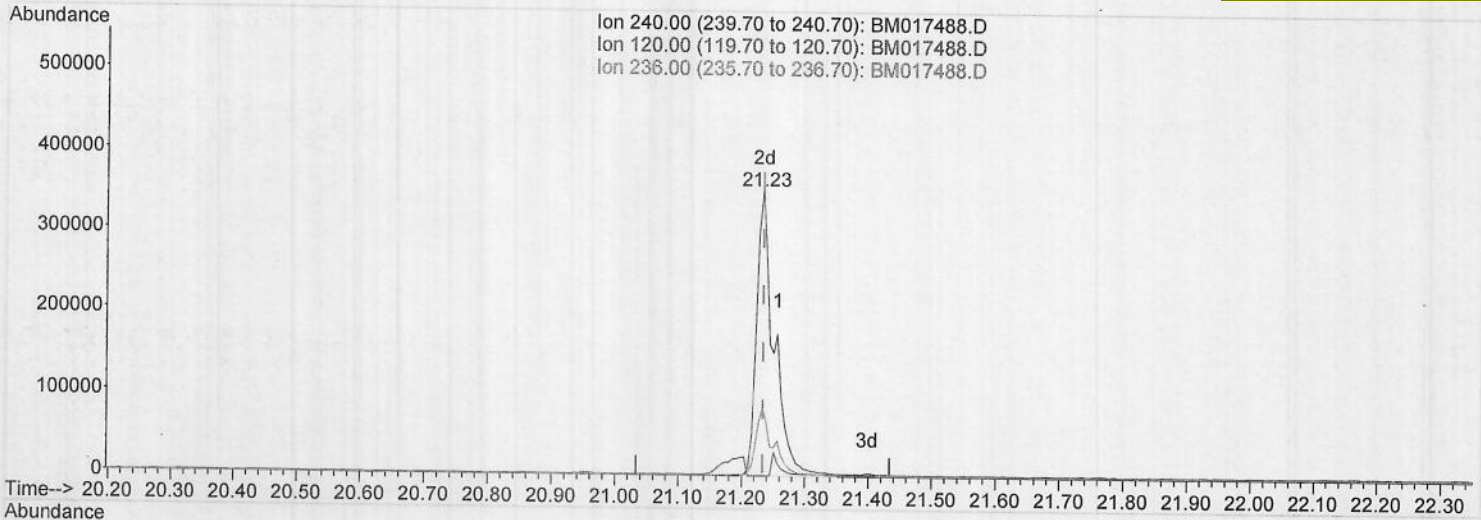

(78) Chrysene-d12 (I)

21.233min (-0.000) 20.00ng/ul m J5701/06/18

response 679147

Ion	Exp%	Act%
240.00	100	100
120.00	9.50	0.00#
236.00	25.00	23.72
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (Qedit)


Data File : BM017510.D
Acq On : 03 Nov 2018 03:15
Operator : MJ/SJ
Sample : J5704-07
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40H1

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:15 PM

Quant Time: Nov 03 04:04:34 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 03:58:03 2018
Response via : Initial Calibration

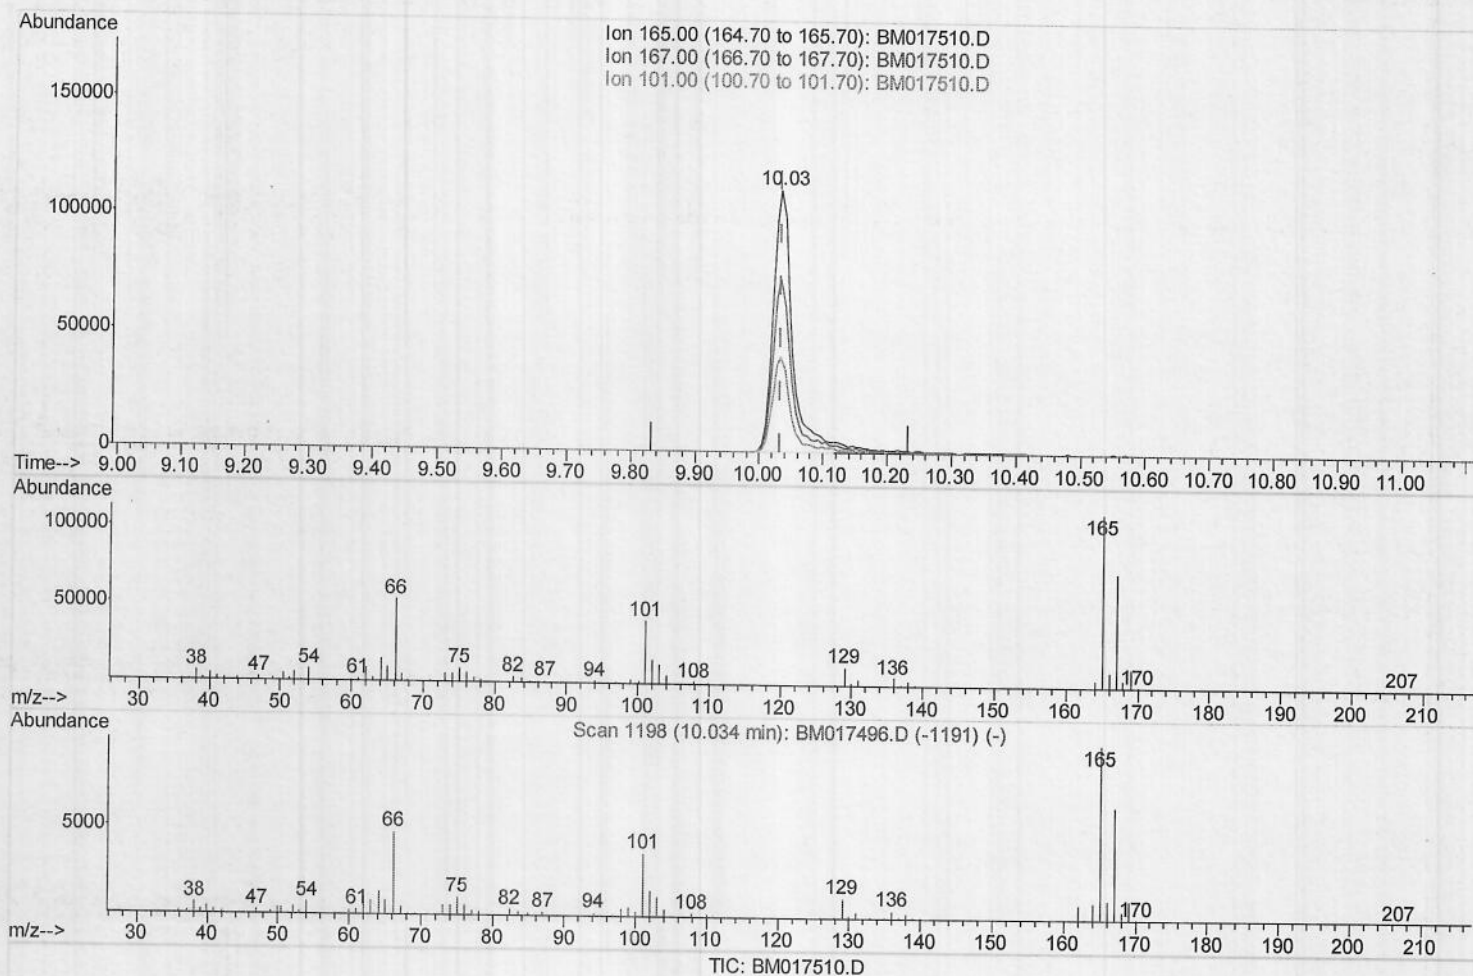

(26) 2,4-Dichlorophenol-d3 (S)

10.034min (+0.000) 19.34ng/ul

response 229778

Ion	Exp%	Act%
165.00	100	100
167.00	63.60	65.72
101.00	34.30	36.32
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (Qedit)




Data File : BM017510.D
Acq On : 03 Nov 2018 03:15
Operator : MJ/SJ
Sample : J5704-07
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40H1

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:15 PM

Quant Time: Nov 03 04:04:34 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 03:58:03 2018
Response via : Initial Calibration

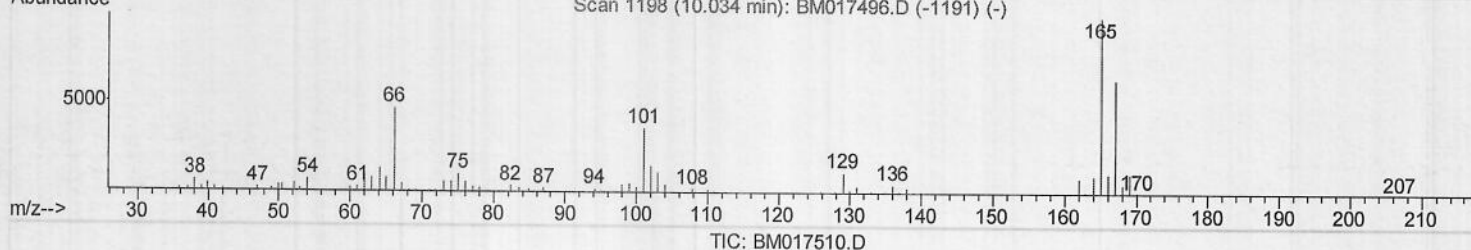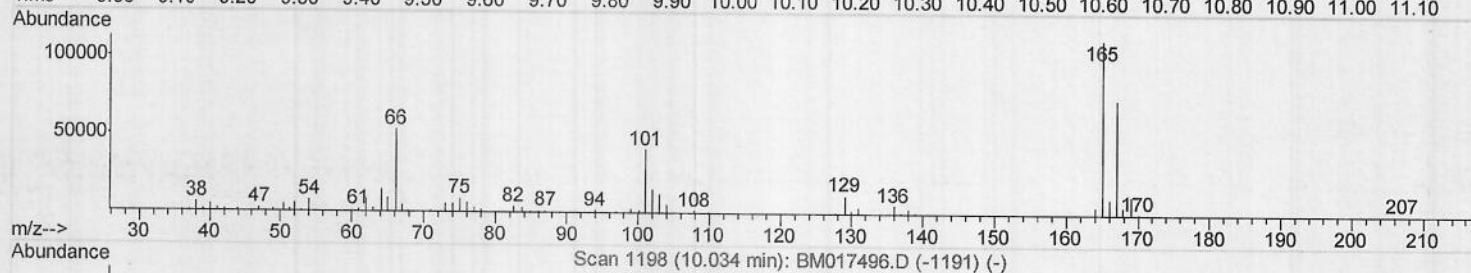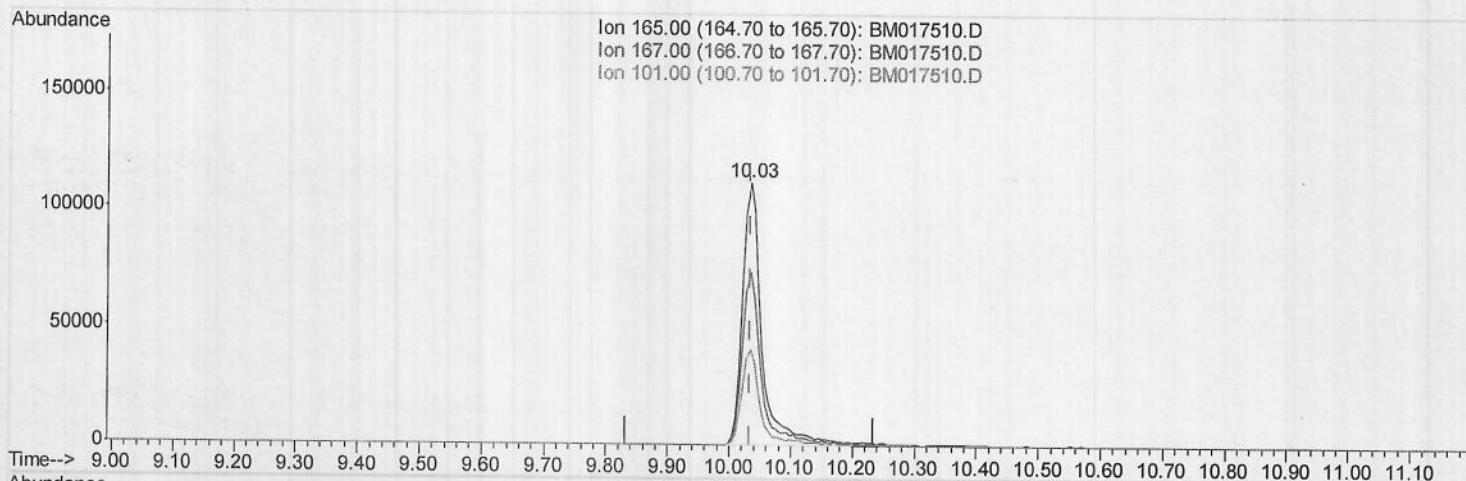

(26) 2,4-Dichlorophenol-d3 (S)

10.034min (+0.000) 20.34ng/ul m

2571106118

response 241600

Ion	Exp%	Act%
165.00	100	100
167.00	63.60	65.72
101.00	34.30	36.32
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (Qedit)




Data File : BM017510.D
Acq On : 03 Nov 2018 03:15
Operator : MJ/SJ
Sample : J5704-07
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40H1

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:15 PM

Quant Time: Nov 03 04:04:34 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 03:58:03 2018
Response via : Initial Calibration

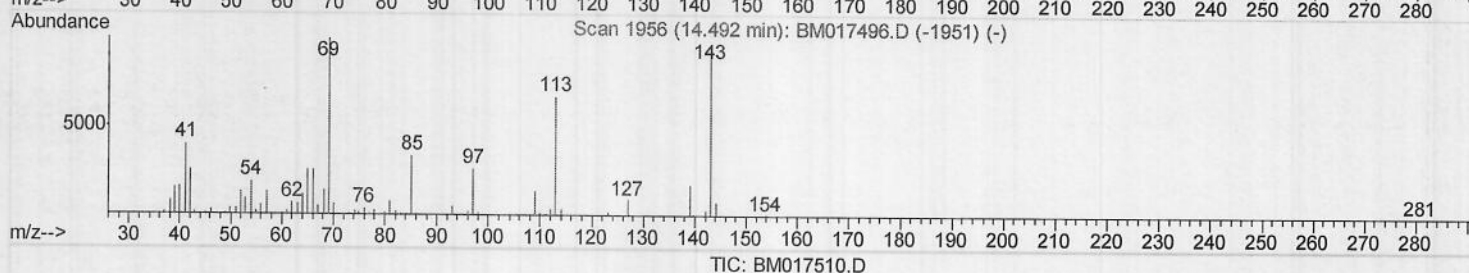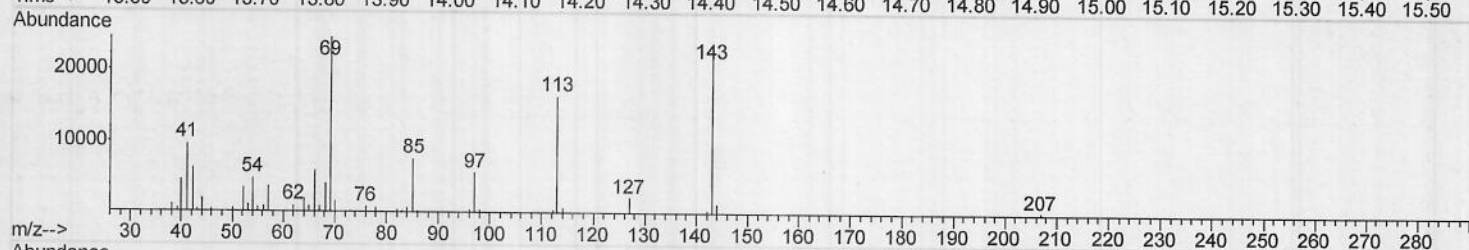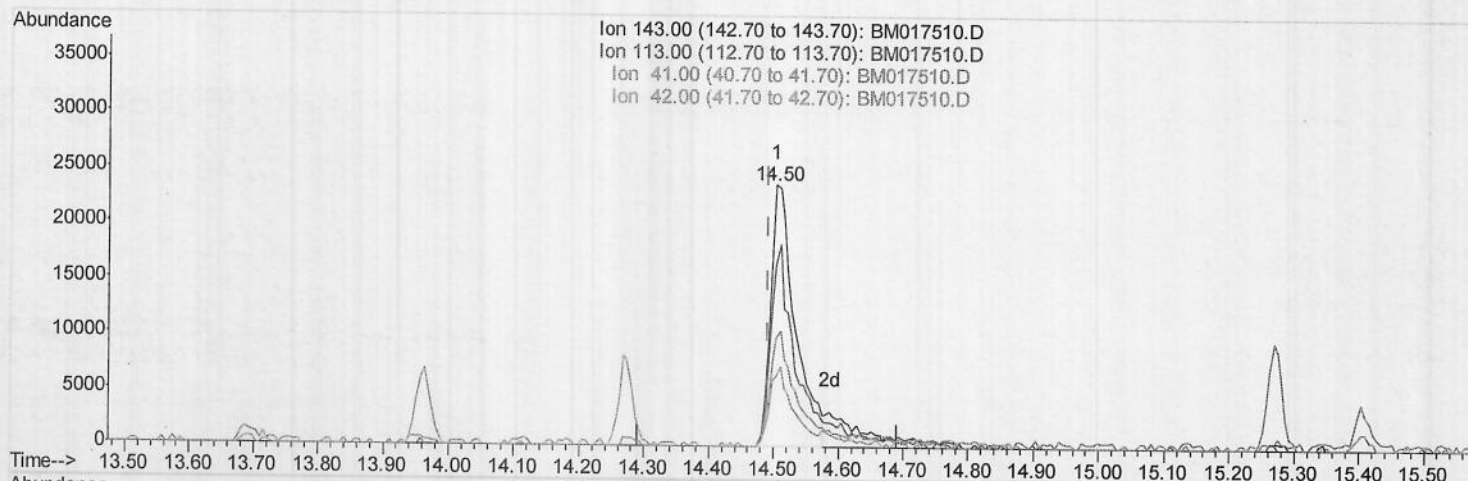

(52) 4-Nitrophenol-d4 (S)

14.504min (+0.012) 11.14ng/ul

response 61687

Ion	Exp%	Act%
143.00	100	100
113.00	74.20	69.79
41.00	39.30	41.30
42.00	25.10	26.96

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Quantitation Report (Qedit)




Data File : BM017510.D
Acq On : 03 Nov 2018 03:15
Operator : MJ/SJ
Sample : J5704-07
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40H1

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:15 PM

Quant Time: Nov 03 04:04:34 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 03:58:03 2018
Response via : Initial Calibration

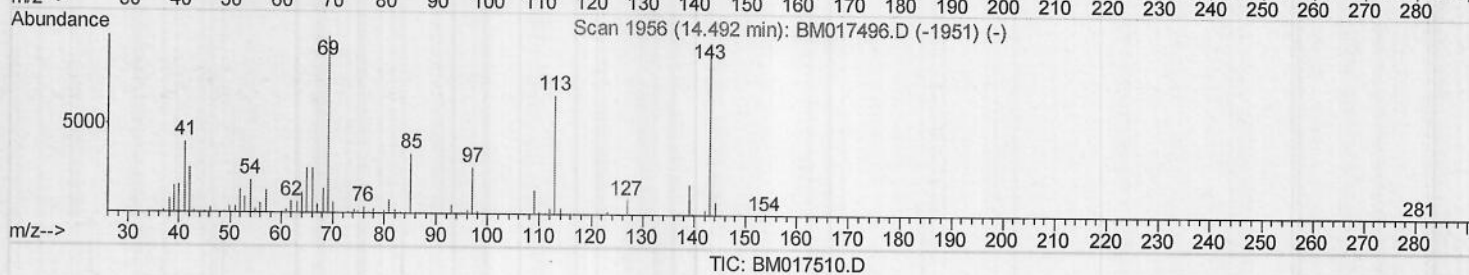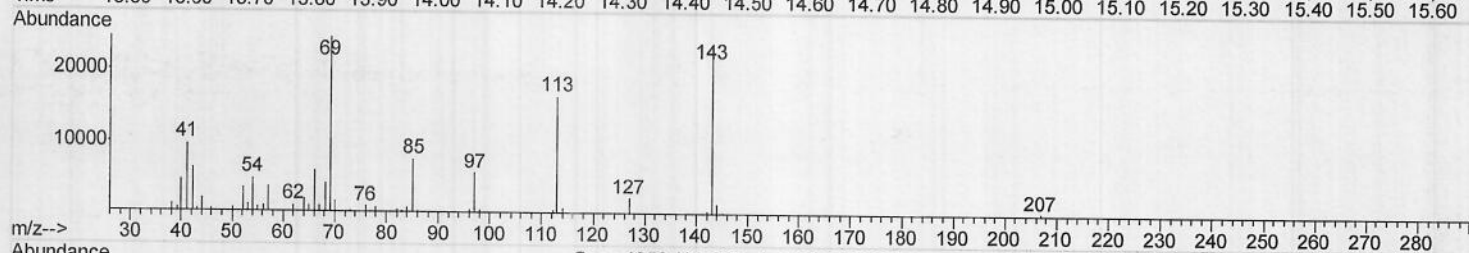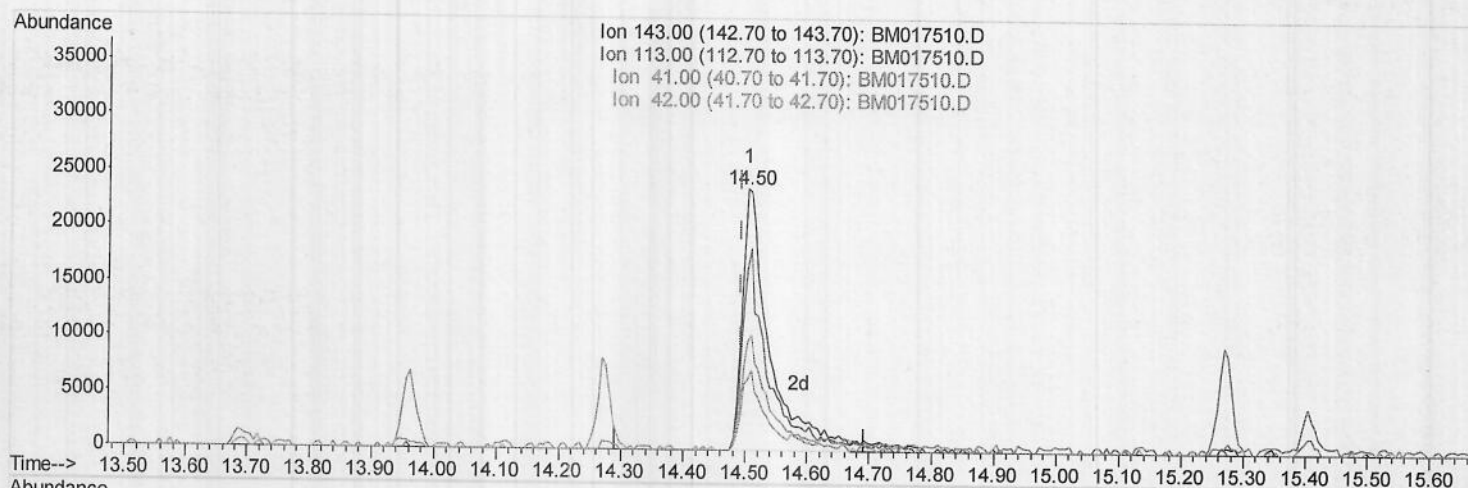

(52) 4-Nitrophenol-d4 (S)

14.504min (+0.012) 12.99ng/ul m

SJ11/06/18

response 71954

Ion	Exp%	Act%
143.00	100	100
113.00	74.20	69.79
41.00	39.30	41.30
42.00	25.10	26.96

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\

Quantitation Report (QT Reviewed)

Data File : BM017510.D

Acq On : 03 Nov 2018 03:15

Operator : MJ/SJ

Sample : J5704-07

Misc :

ALS Vial : 25 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

A40H1

Manual Integrations
APPROVED

Sohil

11/5/2018 4:06:15 PM

Quant Time: Nov 03 05:12:23 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Sat Nov 03 03:58:03 2018

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	187382	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	729716	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	345634	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	617629	20.00	ng/ul	0.00
78) Chrysene-d12	21.23	240	400586	20.00	ng/ul	0.00
86) Perylene-d12	23.42	264	352517	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.21	96	17574	4.32	ng/uL	0.00
5) Phenol-d5	6.81	99	350615	20.48	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	217615	21.80	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	287718	21.68	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	188681	13.94	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	135003	23.67	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	144099	22.53	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	241600m)	20.34	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	202225	20.85	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	631265	21.30	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	840437	23.35	ng/ul	0.00
52) 4-Nitrophenol-d4	14.50	143	71954m)	12.99	ng/ul	0.01
58) Fluorene-d10	15.27	176	557837	21.67	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.41	200	59999	13.94	ng/ul	0.00
71) Anthracene-d10	17.12	188	702878	22.99	ng/ul	0.00
79) Pyrene-d10	19.43	212	650809	35.07	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.28	264	453111	24.34	ng/ul	0.00
Target Compounds						
6) Phenol	6.84	94	81809	4.813	ng/ul#	89
45) Dimethylphthalate	13.74	163	119944	4.177	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

} SJ 11/06/18