

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110218\
 Data File : BM017490.D
 Acq On : 02 Nov 2018 10:52
 Operator : MJ/SJ
 Sample : J5701-13MEDL 30X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A40G2MEDL

Manual Integrations
 APPROVED

Sohil
 11/5/2018 4:05:55 PM

Quant Time: Nov 03 01:57:45 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Nov 03 02:25:47 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	208759	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	959861	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.28	164	598961	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1476480	20.00	ng/ul	0.00
78) Chrysene-d12	21.23	240	1589988	20.00	ng/ul	0.00
86) Perylene-d12	23.44	264	1412918	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	1132	0.25	ng/uL	0.02
5) Phenol-d5	6.83	99	16135m	0.85	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	6.99	67	11104	1.00	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	13843	0.94	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	6710	0.45	ng/ul	0.02
19) Nitrobenzene-d5	8.80	128	5851m	0.78	ng/ul	0.01
22) 2-Nitrophenol-d4	9.52	143	5330	0.63	ng/ul	0.01
26) 2,4-Dichlorophenol-d3	10.10	165	10191m	0.65	ng/ul	0.06
29) 4-Chloroaniline-d4	10.61	131	17851m	1.40	ng/ul	0.05
44) Dimethylphthalate-d6	13.71	166	57536	1.12	ng/ul	0.01
47) Acenaphthylene-d8	13.97	160	64559	1.04	ng/ul	0.00
52) 4-Nitrophenol-d4	14.66	143	370	0.04	ng/ul	0.15
58) Fluorene-d10	15.29	176	59464	1.33	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.45	200	2092	0.20	ng/ul	0.04
71) Anthracene-d10	17.14	188	108430	1.48	ng/ul	0.00
79) Pyrene-d10	19.44	212	103081	1.40	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.30	264	95046	1.27	ng/ul	0.00

Target Compounds

					Ovalue	
84) Bis(2-ethylhexyl)phthalate	21.16	149	12340220	229.104	ng/ul#	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110218\
Data File : BM017490.D
Acq On : 02 Nov 2018 10:52
Operator : MJ/SJ
Sample : J5701-13MEDL 30X
Misc :
ALS Vial : 6 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
A40G2MEDL

Manual Integrations
APPROVED

Sohil
11/5/2018 4:05:55 PM

Quant Time: Nov 03 01:57:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 02:25:47 2018
Response via : Initial Calibration

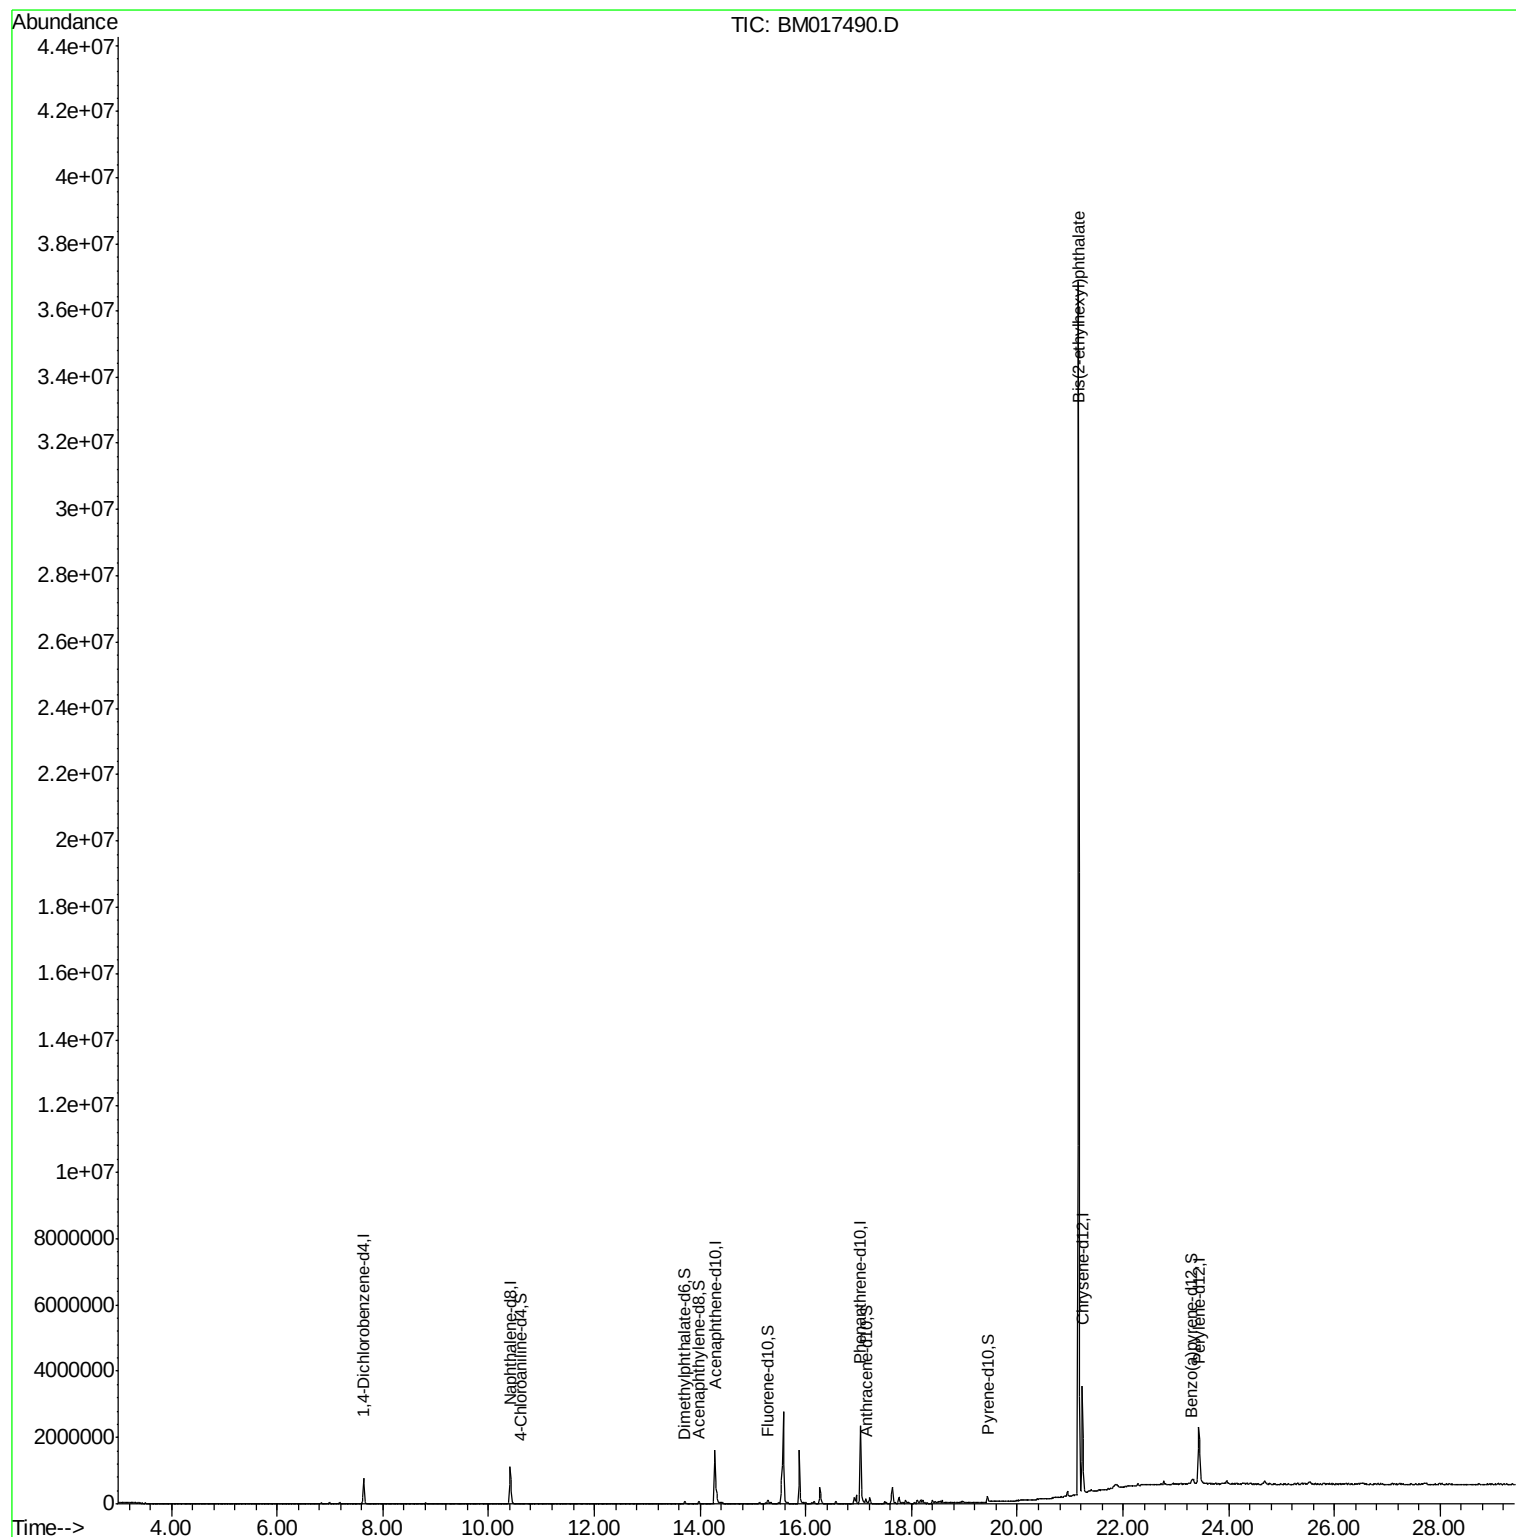

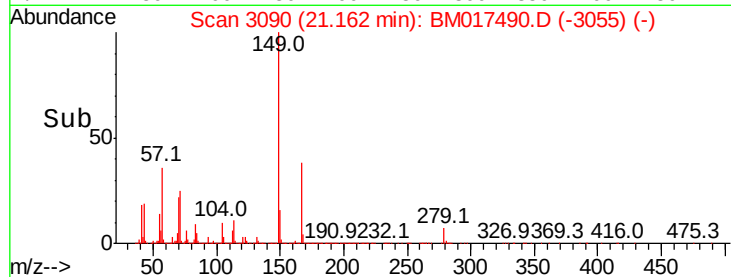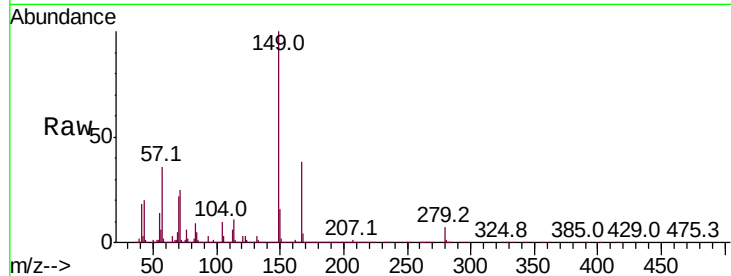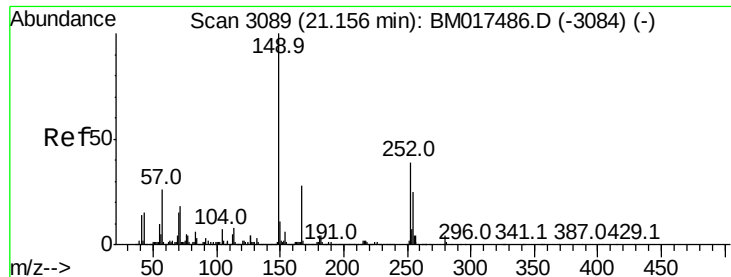

#84

Bis(2-ethylhexyl)phthalate

Concen: 229.104 ng/ul

RT: 21.16 min Scan# 3090

Delta R.T. 0.01 min

Lab File: BM017490.D

Acq: 02 Nov 2018 10:52

Instrument :

BNA_M

ClientSampleId :

A40G2MEDL

Tot Ion:149 Resp:12340220

Ion Ratio Lower Upper

149 100

167 38.3 23.0 34.6#

279 6.7 4.1 6.1#

Manual Integrations

APPROVED

Sohil

11/5/2018 4:05:55 PM

