

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110218\
 Data File : BM017504.D
 Acq On : 02 Nov 2018 23:38
 Operator : MJ/SJ
 Sample : J5704-25MS
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A40K3MS

Manual Integrations
 APPROVED

Sohil
 11/5/2018 4:06:08 PM

Quant Time: Nov 03 03:30:09 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Nov 03 03:58:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	173538	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	681746	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	308892	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	549077	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	384604	20.00	ng/ul	0.00
86) Perylene-d12	23.42	264	349632	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.21	96	22926	6.08	ng/uL	0.00
5) Phenol-d5	6.81	99	488590	30.82	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	284074	30.73	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	394202	32.07	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	346860	27.67	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	176647	33.15	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	192026	32.13	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	334219	30.11	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	312978	34.54	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	777002	29.33	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	1066795	33.17	ng/ul	0.00
52) 4-Nitrophenol-d4	14.50	143	104017	21.02	ng/ul	0.00
58) Fluorene-d10	15.27	176	680300	29.57	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	90281	23.60	ng/ul	0.00
71) Anthracene-d10	17.12	188	865590	31.85	ng/ul	0.00
79) Pyrene-d10	19.43	212	804537	45.15	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.28	264	612507	33.17	ng/ul	0.00

Target Compounds

					Ovalue
6) Phenol	6.84	94	583652	37.080	ng/ul 99
10) 2-Chlorophenol	7.20	128	377048	30.540	ng/ul 98
15) N-Nitroso-di-n-propylamine	8.43	70	264564	27.889	ng/ul 97
33) 4-Chloro-3-methylphenol	11.70	107	312474	26.724	ng/ul 95
45) Dimethylphthalate	13.74	163	148432	5.784	ng/ul 99
50) Acenaphthene	14.34	153	750550	34.726	ng/ul 98
53) 4-Nitrophenol	14.51	109	88621	23.618	ng/ul 92
55) 2,4-Dinitrotoluene	14.66	165	199232	25.927	ng/ul 94
59) Fluorene	15.33	166	58544	2.320	ng/ul 98
69) Pentachlorophenol	16.68	266	92394	21.268	ng/ul 97
70) Phenanthrene	17.07	178	680363	21.578	ng/ul 100
72) Anthracene	17.16	178	167555	5.232	ng/ul 98
75) Carbazole	17.44	167	73451	2.623	ng/ul 98
77) Fluoranthene	19.09	202	757229	20.952	ng/ul 100
80) Pyrene	19.46	202	1656648	74.177	ng/ul 99
83) Benzo(a)anthracene	21.21	228	283363	12.040	ng/ul 98
84) Bis(2-ethylhexyl)phthalate	21.15	149	17881	1.372	ng/ul# 97
85) Chrysene	21.26	228	294034	13.138	ng/ul 99
88) Benzo(b)fluoranthene	22.77	252	239439	11.699	ng/ul# 95
89) Benzo(k)fluoranthene	22.80	252	101422m	5.073	ng/ul
91) Benzo(a)pyrene	23.33	252	181694	9.087	ng/ul 97
92) Indeno(1,2,3-cd)pyrene	25.61	276	96452	3.965	ng/ul 99
93) Dibenzo(a,h)anthracene	25.62	278	32195	1.585	ng/ul# 94

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110218\
Data File : BM017504.D
Acq On : 02 Nov 2018 23:38
Operator : MJ/SJ
Sample : J5704-25MS
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40K3MS

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:08 PM

Quant Time: Nov 03 03:30:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 03:58:03 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
94) Benzo(q,h,i)perylene	26.29	276	80977	3.918	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110218\
Data File : BM017504.D
Acq On : 02 Nov 2018 23:38
Operator : MJ/SJ
Sample : J5704-25MS
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
A40K3MS

Quant Time: Nov 03 03:30:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 03 03:58:03 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:08 PM

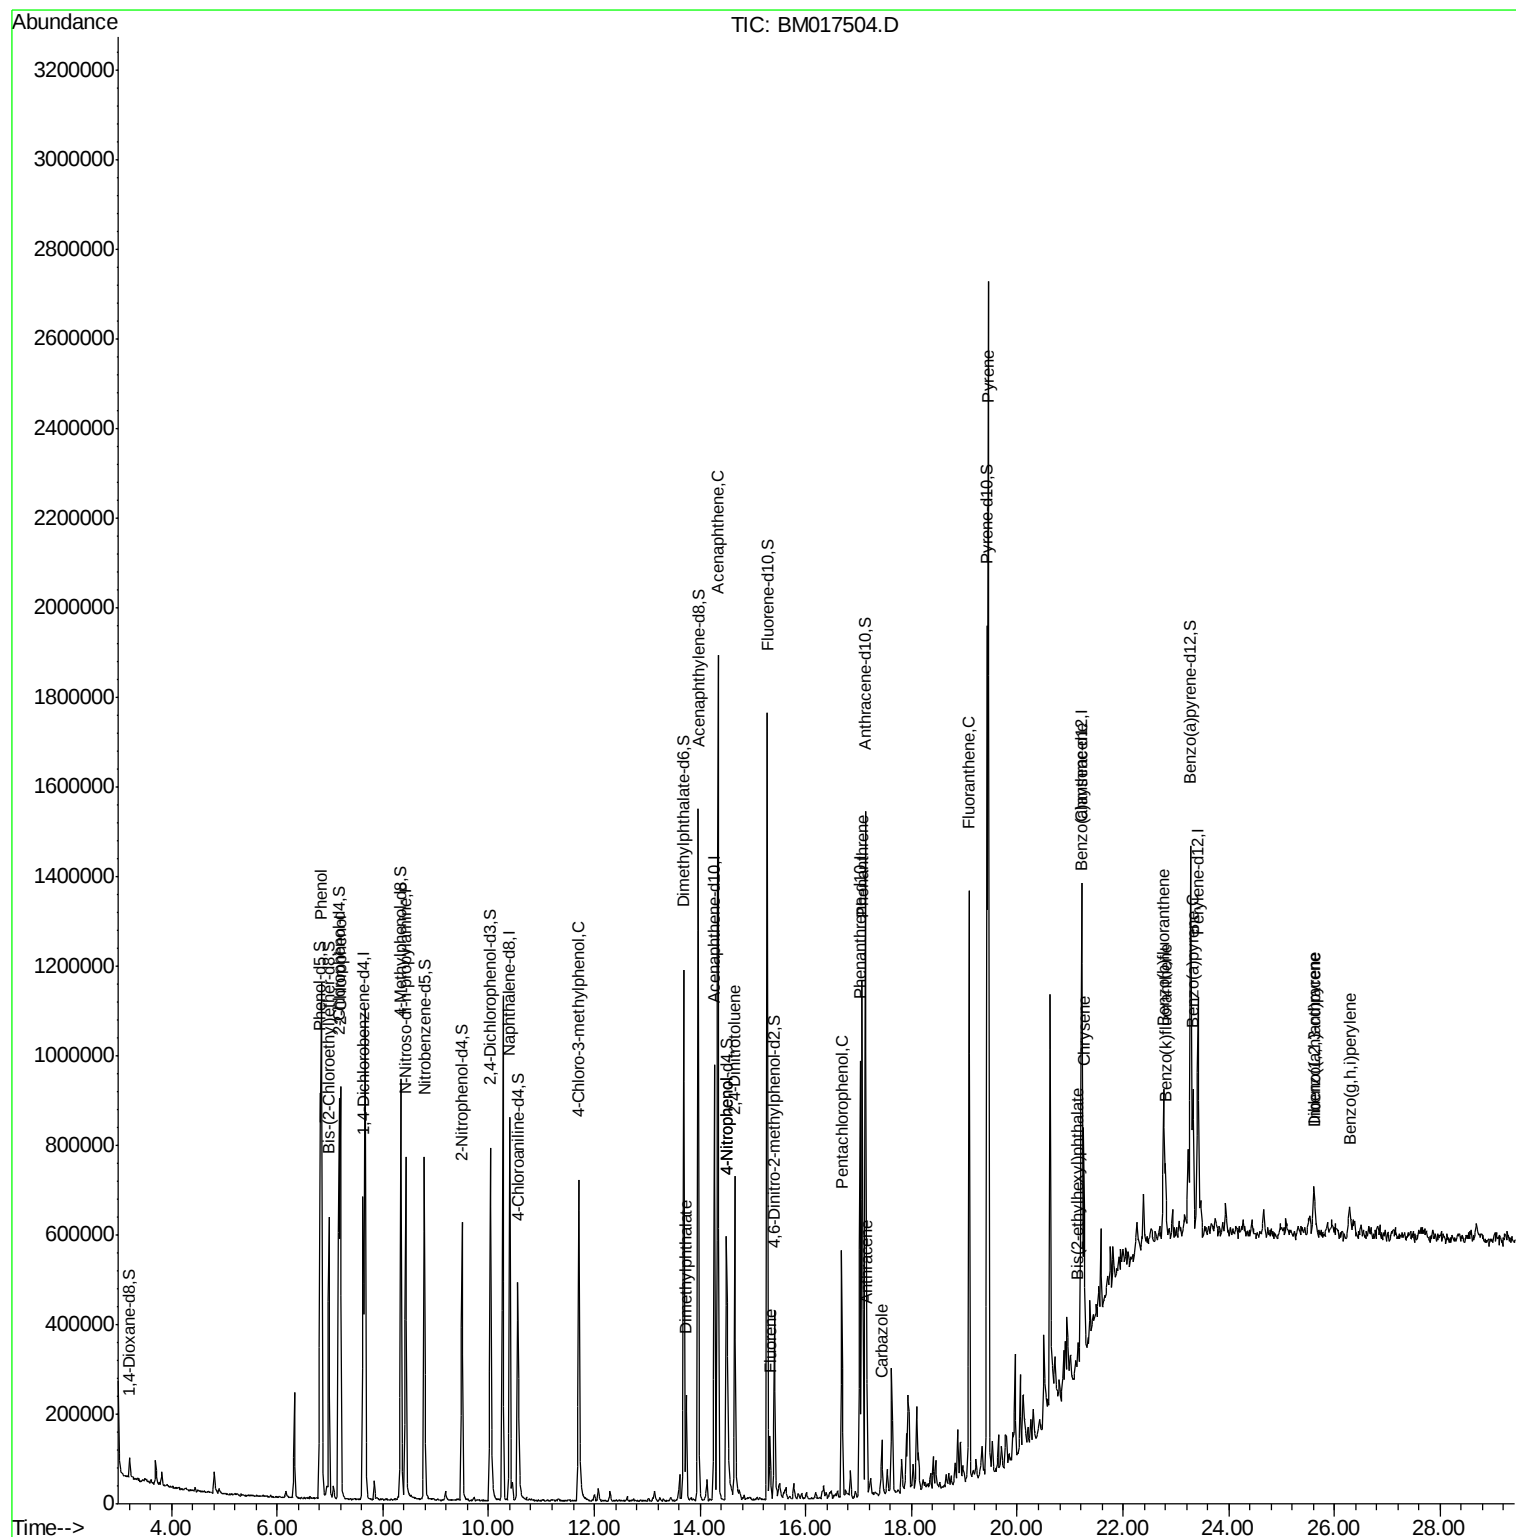

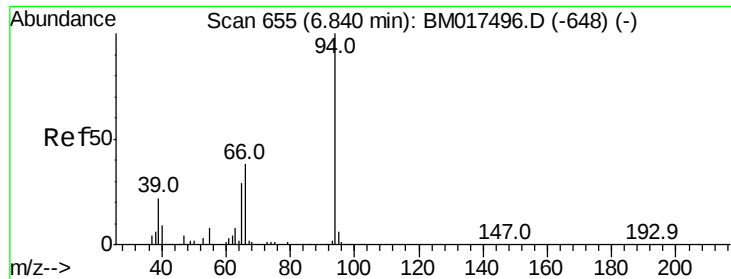

#6

Phenol

Concen: 37.080 ng/ul

RT: 6.84 min Scan# 655

Delta R.T. -0.00 min

Lab File: BM017504.D

Acq: 02 Nov 2018 23:38

Instrument :

BNA_M





ClientSampled :

A40K3MS

Tot Ion	94	Resp	583652
Ion Ratio	Lower	Upper	
94	100		
65	29.2	24.0	36.0
66	39.6	31.1	46.7

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:08 PM

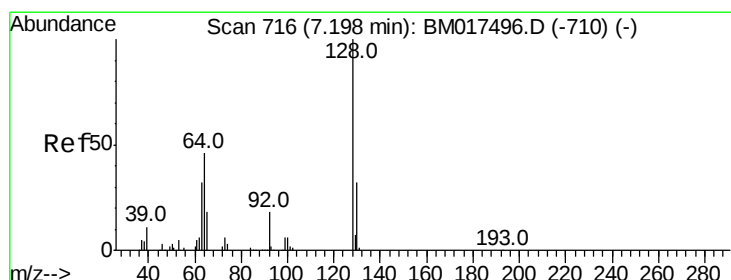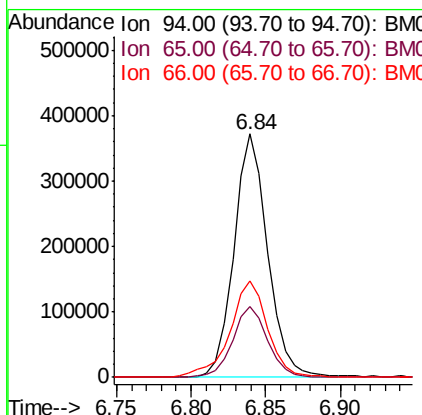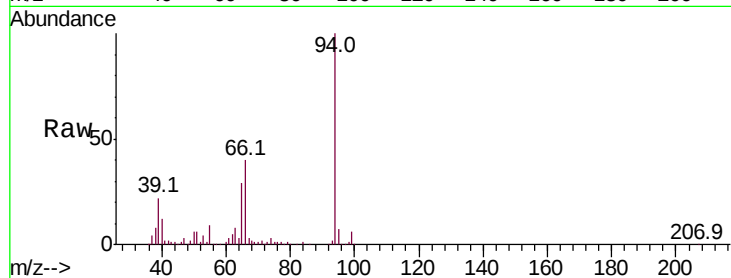

#10

2-Chlorophenol

Concen: 30.540 ng/ul




RT: 7.20 min Scan# 716




Delta R.T. -0.00 min

Lab File: BM017504.D

Acq: 02 Nov 2018 23:38

Tgt Ion	128	Resp	377048
Ion Ratio	Lower	Upper	
128	100		
64	47.0	36.2	54.2
130	32.3	26.0	39.0

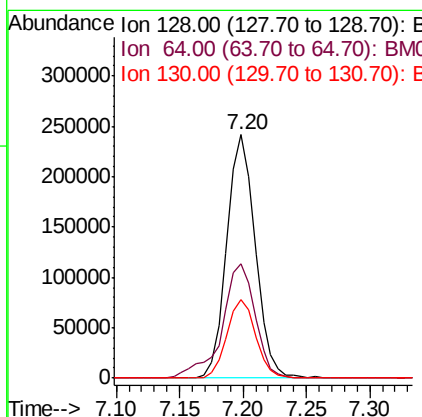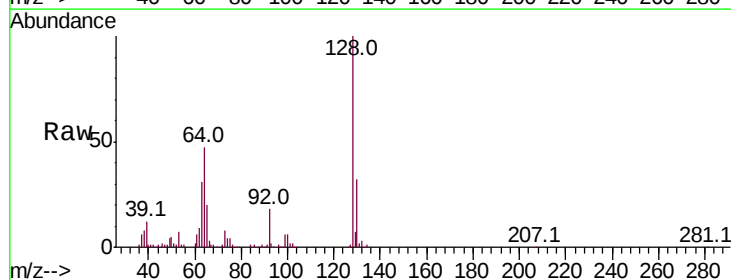

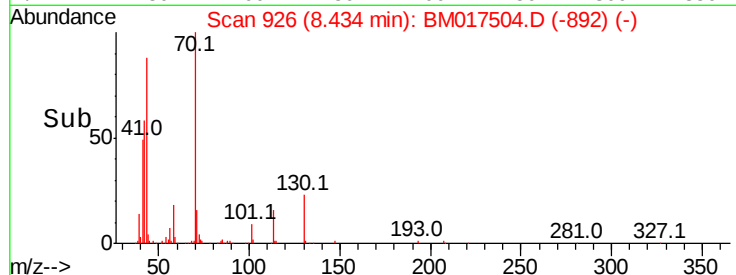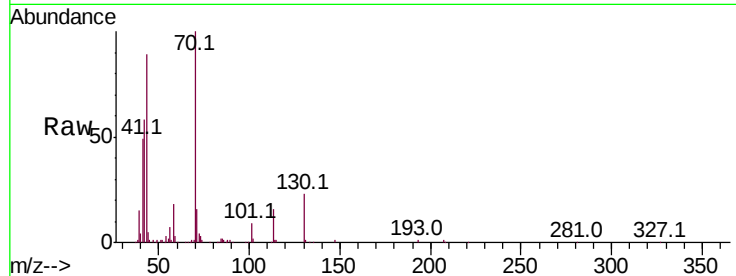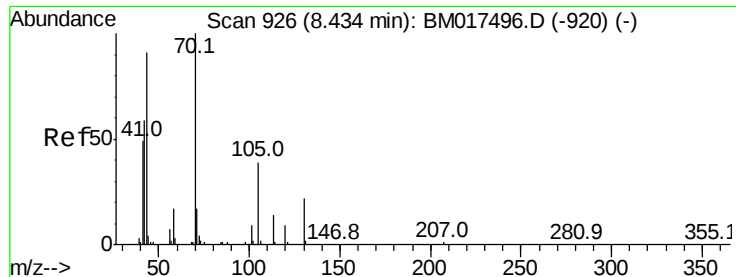

#15

N-Nitroso-di-n-propylamine

Concen: 27.889 ng/ul

RT: 8.43 min Scan# 926

Delta R.T. -0.00 min

Lab File: BM017504.D

Acq: 02 Nov 2018 23:38

Instrument :

BNA_M





ClientSampleId :

A40K3MS

Tot Ion	Ratio	Lower	Upper
70	100		
42	58.0	43.7	65.5
101	9.3	8.0	12.0
130	22.5	17.8	26.8

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:08 PM

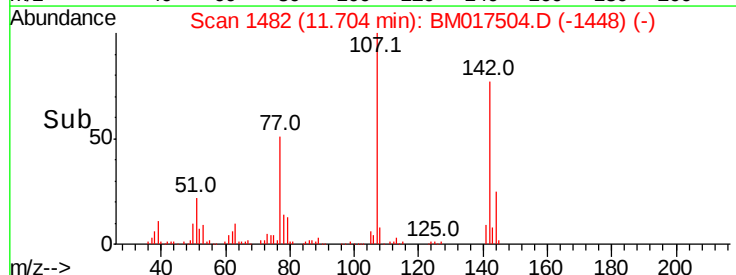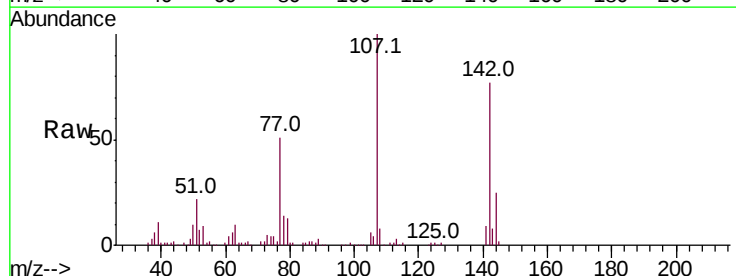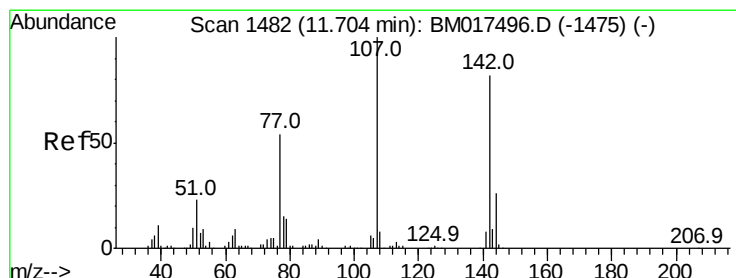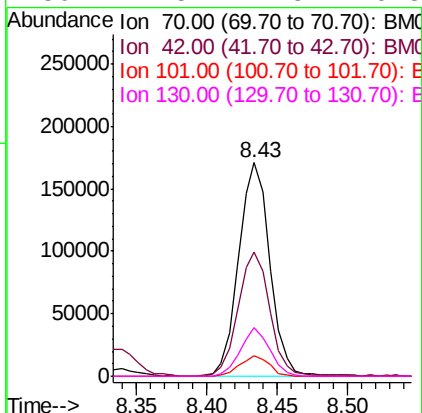

#33

4-Chloro-3-methylphenol

Concen: 26.724 ng/ul


RT: 11.70 min Scan# 1482


Delta R.T. -0.00 min

Lab File: BM017504.D

Acq: 02 Nov 2018 23:38

Tgt Ion	Ratio	Lower	Upper
107	100		
144	25.1	21.8	32.6
142	76.6	65.0	97.4

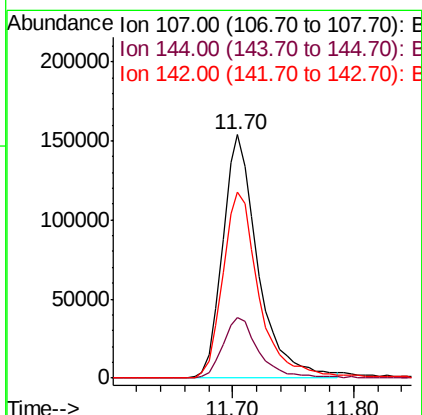

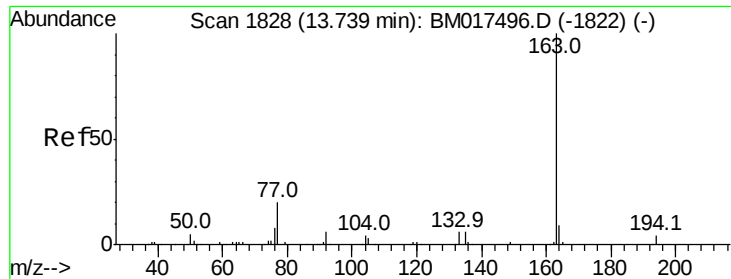


#45
Dimethylphthalate
Concen: 5.784 ng/ul
RT: 13.74 min Scan# 1828
Delta R.T. -0.00 min
Lab File: BM017504.D
Acq: 02 Nov 2018 23:38

Instrument :
BNA_M
ClientSampleId :
A40K3MS




Tot Ion	Ratio	Resp	Lower	Upper
163	100	148432		
194	4.3	3.2	4.8	
164	10.3	8.1	12.1	

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:08 PM

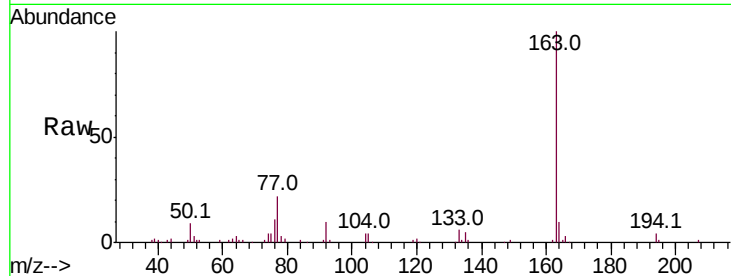


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

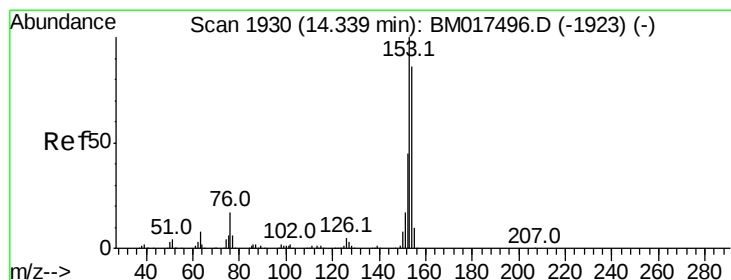
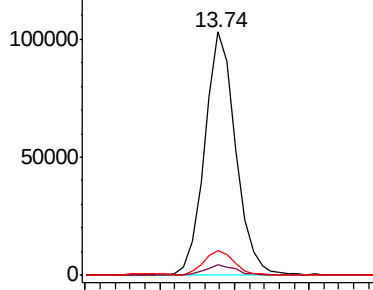



#50
Acenaphthene
Concen: 34.726 ng/ul
RT: 14.34 min Scan# 1930
Delta R.T. -0.00 min
Lab File: BM017504.D
Acq: 02 Nov 2018 23:38

Tgt Ion	Ratio	Resp	Lower	Upper
153	100	750550		
152	45.0	36.9	55.3	
154	88.6	72.2	108.4	

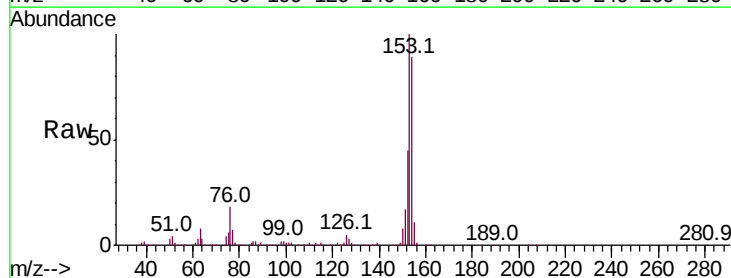

Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E

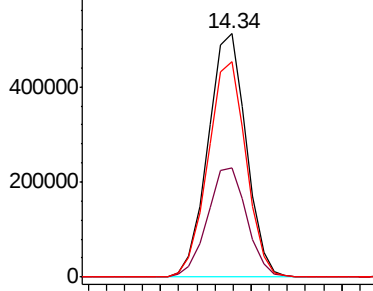







#53
4-Nitrophenol
Concen: 23.618 ng/ul
RT: 14.51 min Scan# 1959
Delta R.T. -0.00 min
Lab File: BM017504.D
Acq: 02 Nov 2018 23:38

Instrument :
BNA_M
ClientSampleId :
A40K3MS

Tot Ion	Ratio	Lower	Upper
109	100		
139	133.9	103.4	155.0
65	139.7	101.0	151.6




Manual Integrations
APPROVED


Sohil
11/5/2018 4:06:08 PM

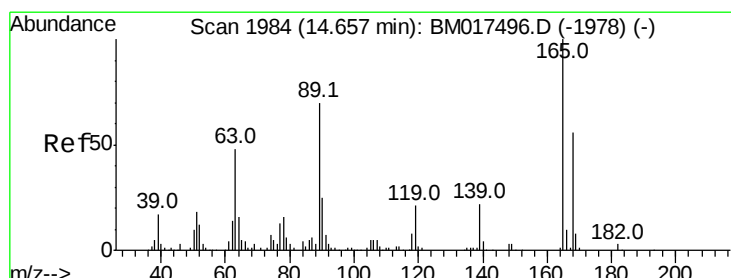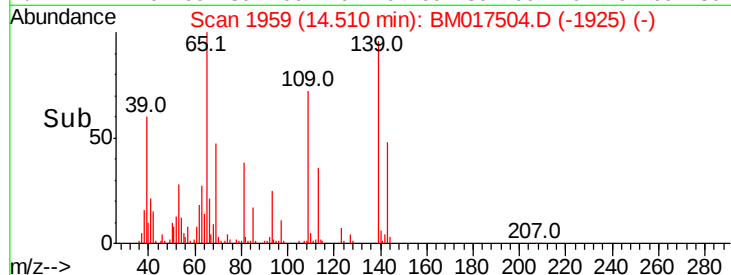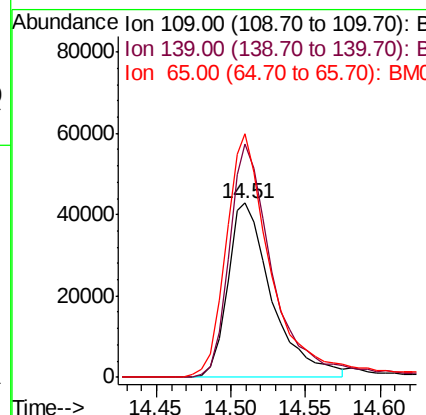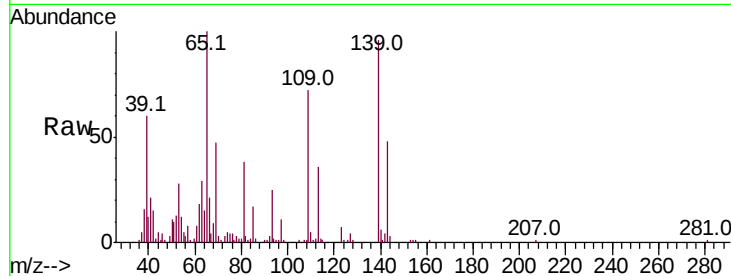

#55
2,4-Dinitrotoluene
Concen: 25.927 ng/ul
RT: 14.66 min Scan# 1984
Delta R.T. -0.00 min
Lab File: BM017504.D
Acq: 02 Nov 2018 23:38

Tgt Ion	Ratio	Lower	Upper
165	100		
63	46.1	33.9	50.9
182	2.7	2.2	3.4

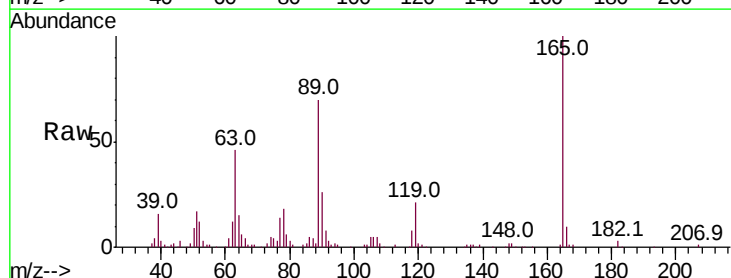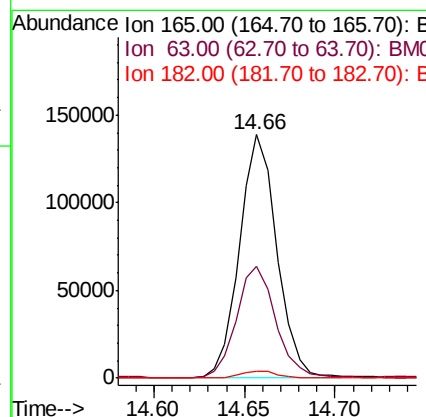

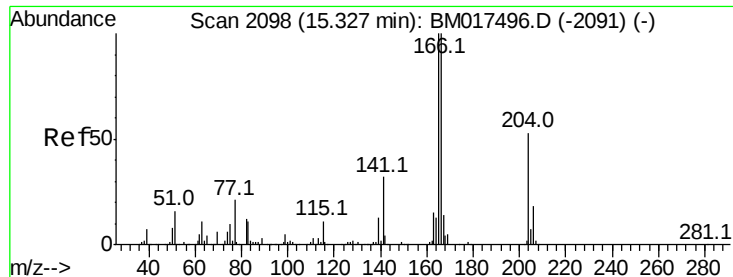





#59
 Fluorene
 Concen: 2.320 ng/ul
 RT: 15.33 min Scan# 2098
 Delta R.T. -0.00 min
 Lab File: BM017504.D
 Acq: 02 Nov 2018 23:38

Instrument :
 BNA_M
 ClientSampled :
 A40K3MS

Tot Ion	Ratio	Lower	Upper
166	100		
165	95.2	77.5	116.3
167	14.7	10.8	16.2




Manual Integrations
 APPROVED


Sohil
 11/5/2018 4:06:08 PM

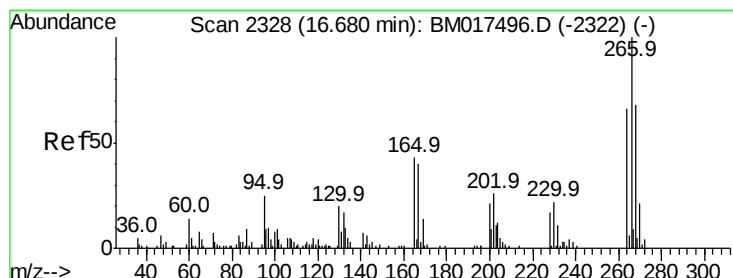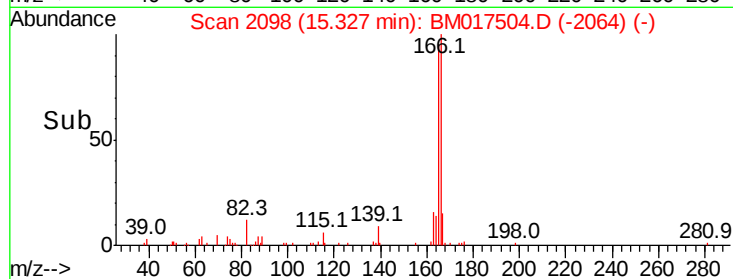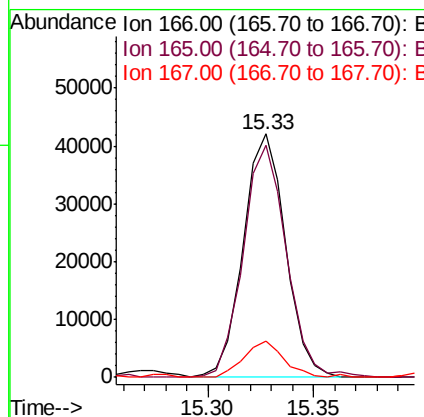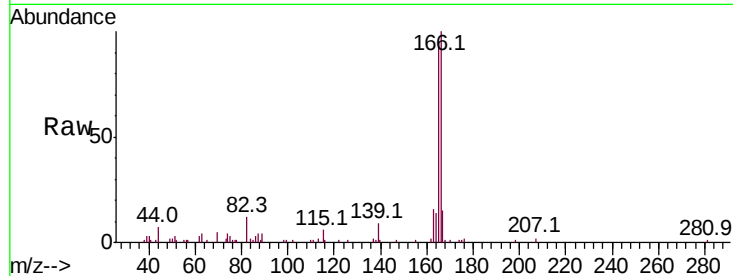

#69
 Pentachlorophenol
 Concen: 21.268 ng/ul
 RT: 16.68 min Scan# 2328
 Delta R.T. -0.00 min
 Lab File: BM017504.D
 Acq: 02 Nov 2018 23:38

Tgt Ion	Ratio	Lower	Upper
266	100		
264	64.2	49.2	73.8
268	66.1	50.9	76.3

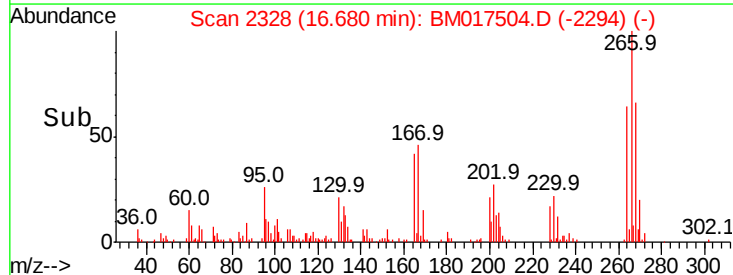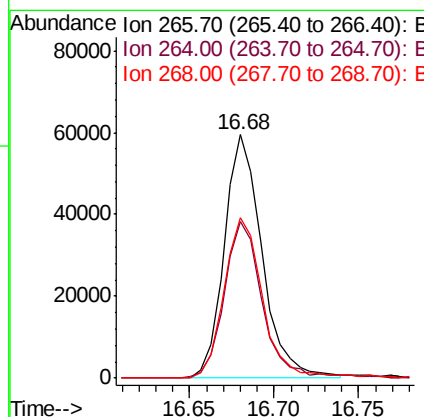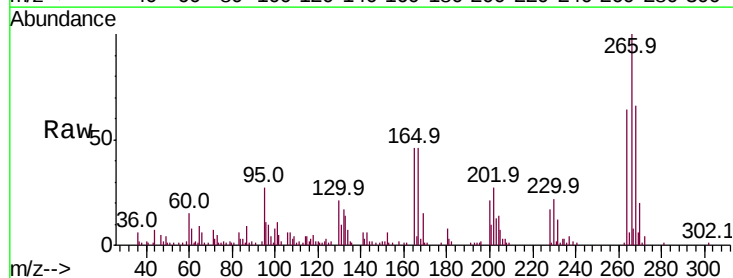

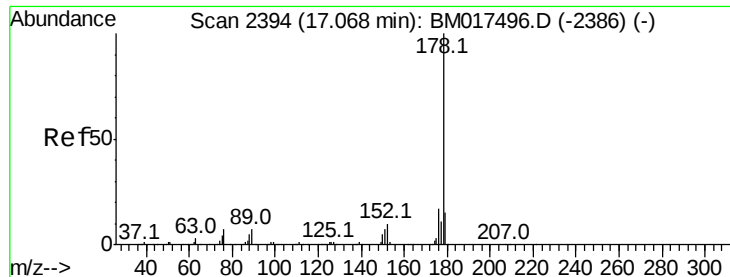





#70
Phenanthrene
Concen: 21.578 ng/ul
RT: 17.07 min Scan# 2394
Delta R.T. -0.00 min
Lab File: BM017504.D
Acq: 02 Nov 2018 23:38

Instrument :
BNA_M
ClientSampleId :
A40K3MS

Tot Ion	Ratio	Lower	Upper
178	100		
179	15.3	12.2	18.2
176	18.6	14.9	22.3




Manual Integrations
APPROVED


Sohil
11/5/2018 4:06:08 PM

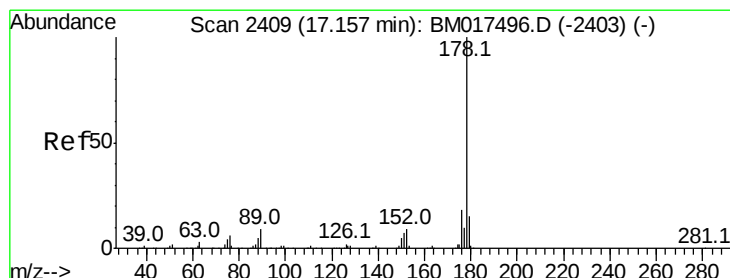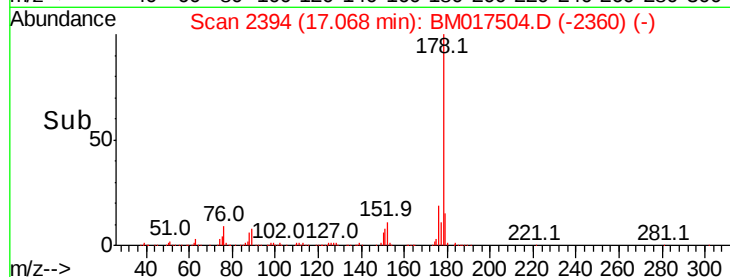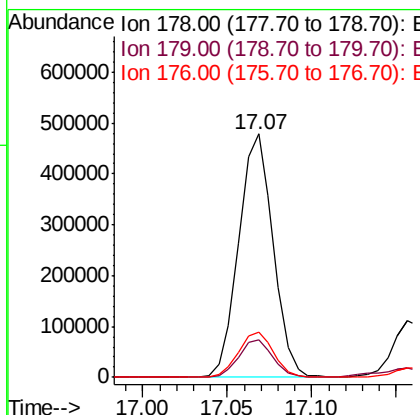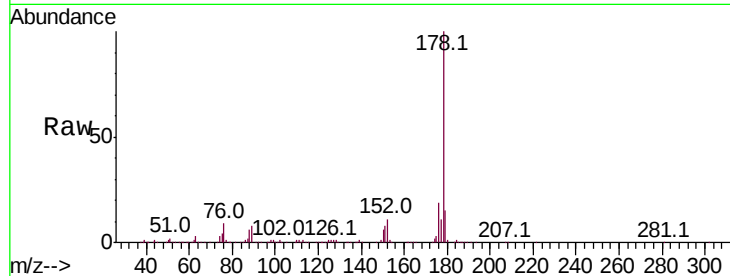

#72
Anthracene
Concen: 5.232 ng/ul
RT: 17.16 min Scan# 2409
Delta R.T. -0.00 min
Lab File: BM017504.D
Acq: 02 Nov 2018 23:38

Tgt Ion	Ratio	Lower	Upper
178	100		
179	16.5	12.2	18.2
176	17.0	14.2	21.2

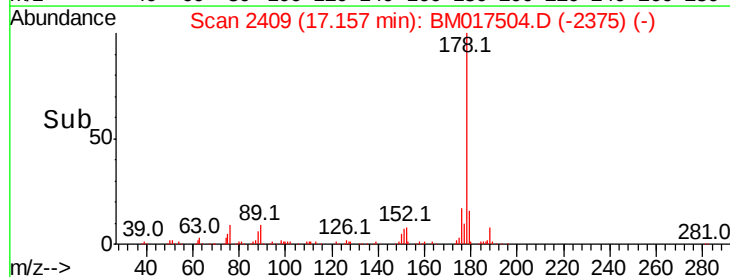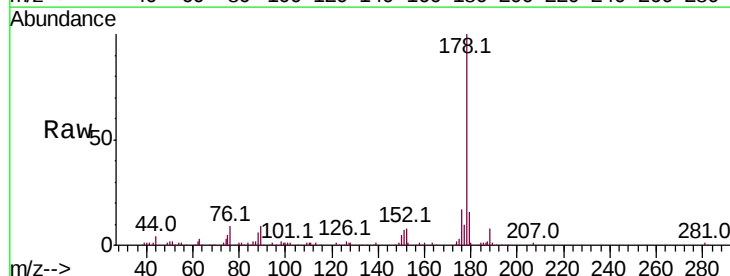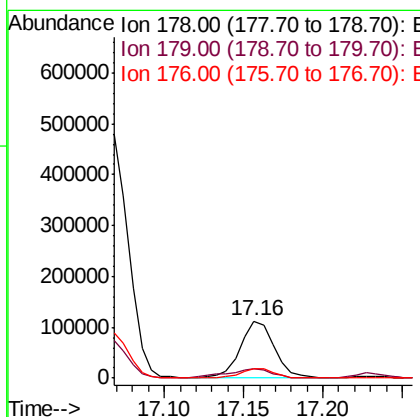

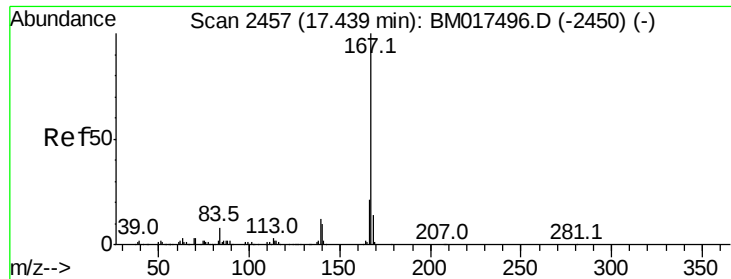





#75
 Carbazole
 Concen: 2.623 ng/ul
 RT: 17.44 min Scan# 2457
 Delta R.T. -0.00 min
 Lab File: BM017504.D
 Acq: 02 Nov 2018 23:38

Instrument :
 BNA_M
 ClientSampleId :
 A40K3MS

Tot Ion	Ratio	Lower	Upper
167	100		
166	20.8	17.5	26.3
139	13.4	10.0	15.0




Manual Integrations
 APPROVED


Sohil
 11/5/2018 4:06:08 PM

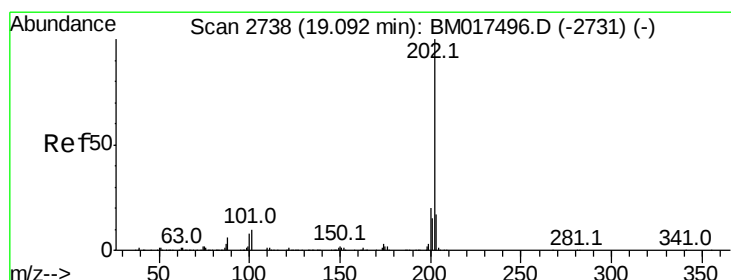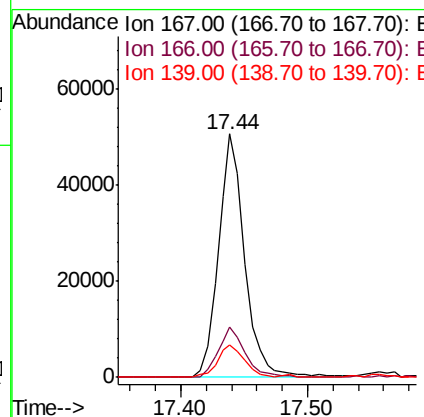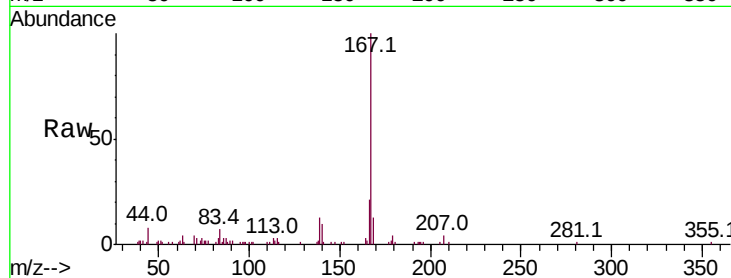

#77
 Fluoranthene
 Concen: 20.952 ng/ul
 RT: 19.09 min Scan# 2738
 Delta R.T. -0.00 min
 Lab File: BM017504.D
 Acq: 02 Nov 2018 23:38

Tgt Ion	Ratio	Lower	Upper
202	100		
101	10.4	8.2	12.4
100	8.0	6.3	9.5

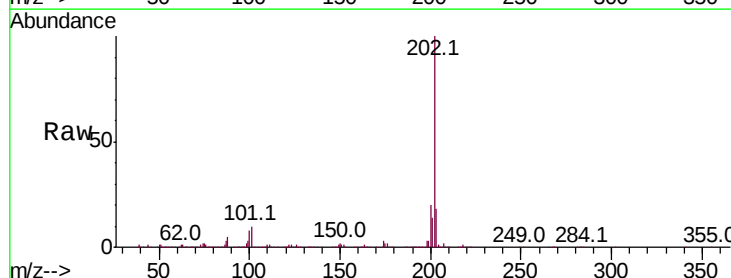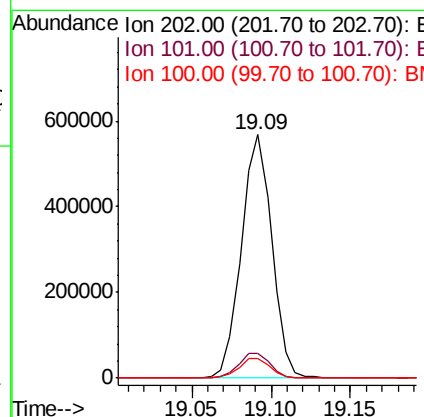

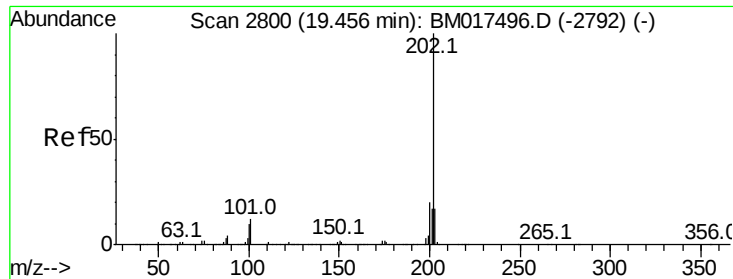


#80
Pvrene
Concen: 74.177 ng/ul
RT: 19.46 min Scan# 2800
Delta R.T. -0.00 min
Lab File: BM017504.D
Acq: 02 Nov 2018 23:38

Instrument :
BNA_M
ClientSampleId :
A40K3MS

Tot Ion	Ratio	Lower	Upper
202	100		
101	12.2	9.5	14.3
100	10.2	8.1	12.1

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:08 PM



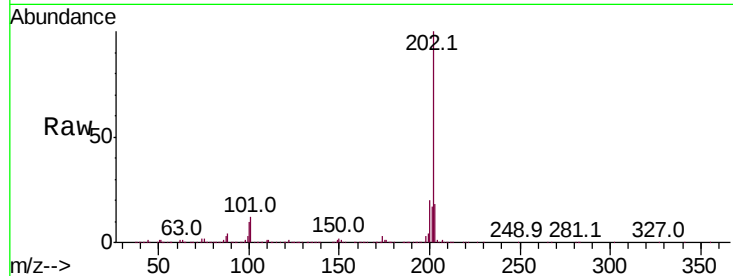


Abundance

Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

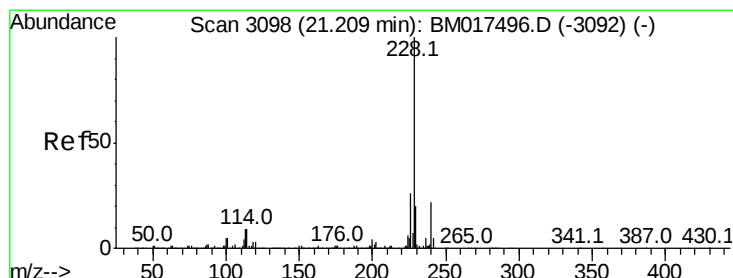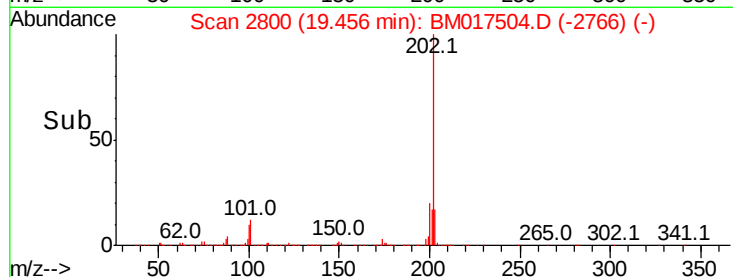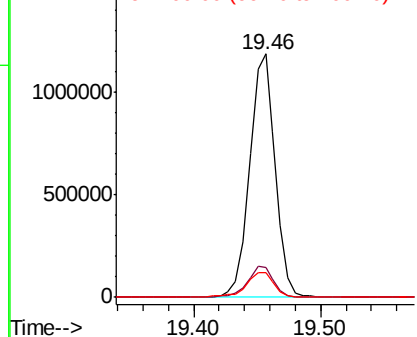

#83
Benzo(a)anthracene
Concen: 12.040 ng/ul
RT: 21.21 min Scan# 3098
Delta R.T. -0.00 min
Lab File: BM017504.D
Acq: 02 Nov 2018 23:38




Tgt Ion	Ratio	Lower	Upper
228	100		
229	21.2	15.6	23.4
226	26.5	20.8	31.2


Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

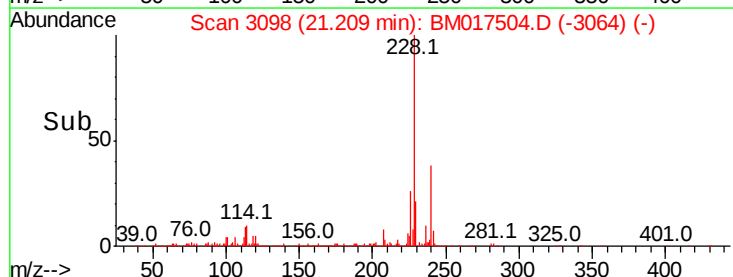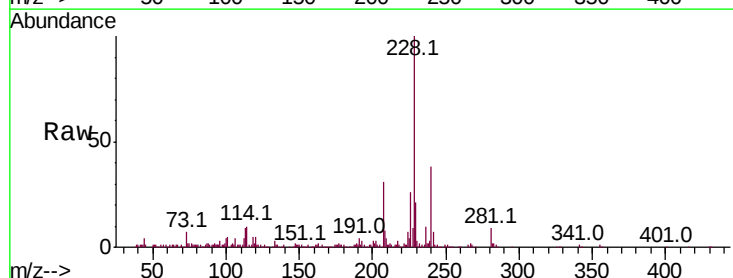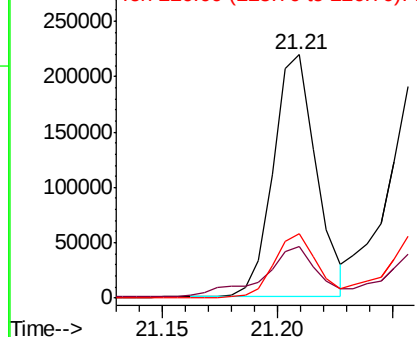

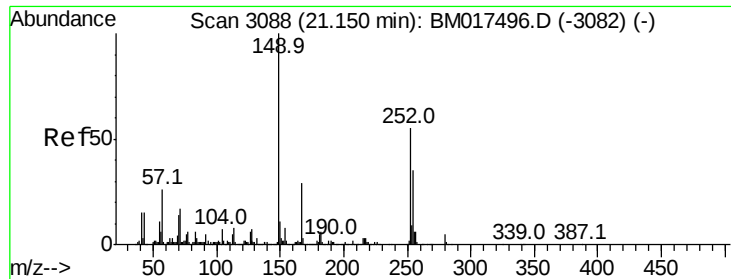

#84

Bis(2-ethylhexyl)phthalate

Concen: 1.372 ng/ul

RT: 21.15 min Scan# 3088

Delta R.T. -0.00 min

Lab File: BM017504.D

Acq: 02 Nov 2018 23:38

Instrument :

BNA_M


ClientSampleId :

A40K3MS




Tot Ion:	149	Resp:	17881
Ion Ratio	Lower	Upper	
149	100		
167	30.6	23.0	34.6
279	6.4	4.1	6.1#

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:08 PM

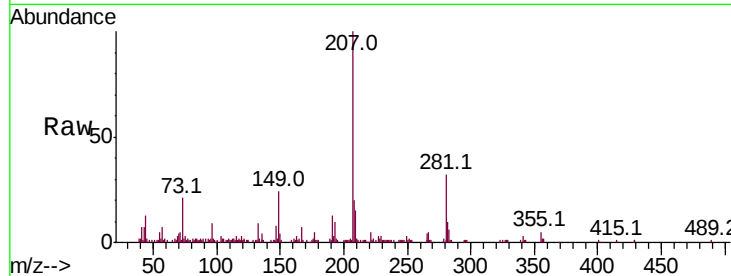

Abundance Ion 149.00 (148.70 to 149.70): E
Ion 167.00 (166.70 to 167.70): E
Ion 279.00 (278.70 to 279.70): E

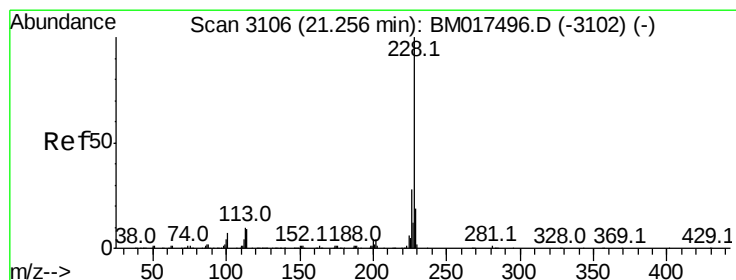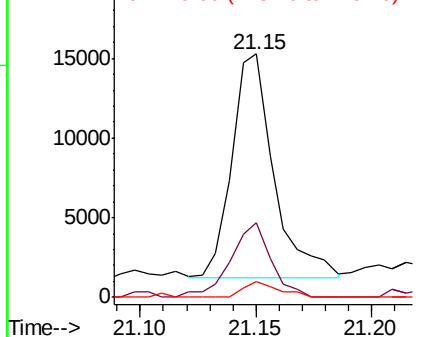

#85

Chrysene

Concen: 13.138 ng/ul


RT: 21.26 min Scan# 3106

Delta R.T. -0.00 min



Lab File: BM017504.D


Acq: 02 Nov 2018 23:38

Tgt Ion:	228	Resp:	294034
Ion Ratio	Lower	Upper	
228	100		
226	29.3	23.3	34.9
229	20.7	15.6	23.4

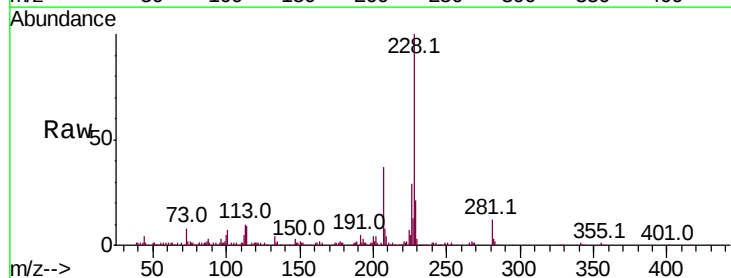

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

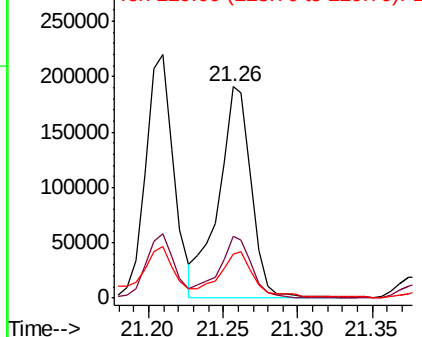

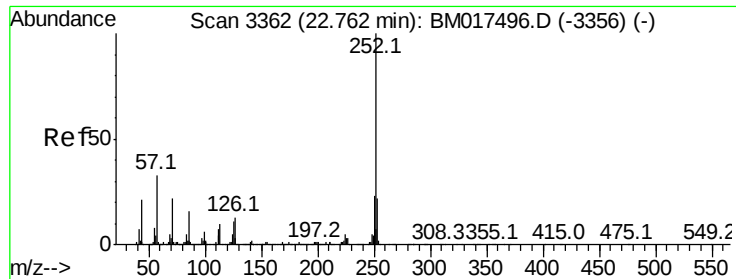

#88

Benzo(b)fluoranthene

Concen: 11.699 ng/ul

RT: 22.77 min Scan# 3363

Delta R.T. 0.01 min

Lab File: BM017504.D

Acq: 02 Nov 2018 23:38

Instrument :

BNA_M





ClientSampled :

A40K3MS

Tot Ion	Ratio	Lower	Upper
252	100		
253	24.4	17.6	26.4
125	10.9	7.2	10.8

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:08 PM

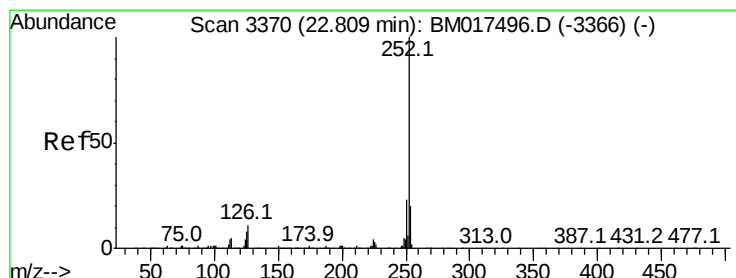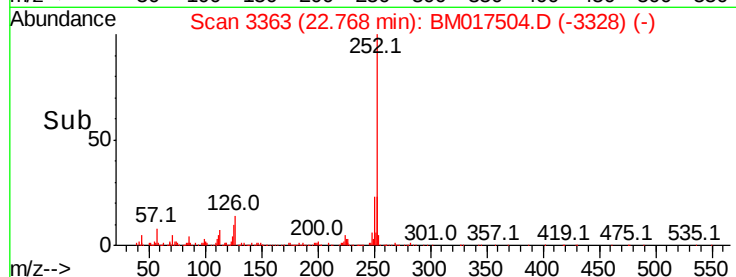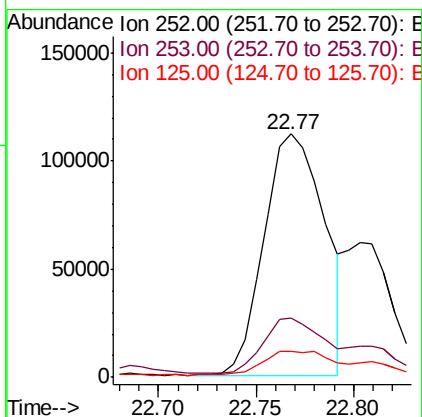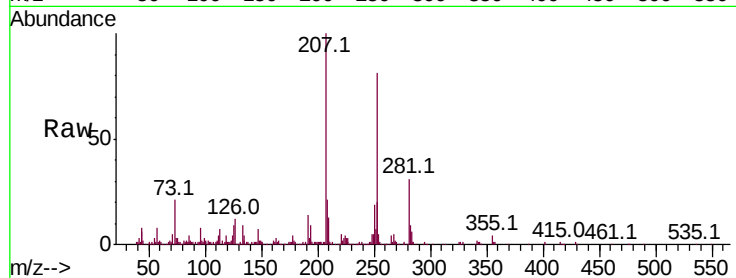

#89

Benzo(k)fluoranthene

Concen: 5.073 ng/ul m




RT: 22.80 min Scan# 3369


Delta R.T. -0.01 min

Lab File: BM017504.D

Acq: 02 Nov 2018 23:38

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.4	17.7	26.5
125	10.6	7.8	11.6

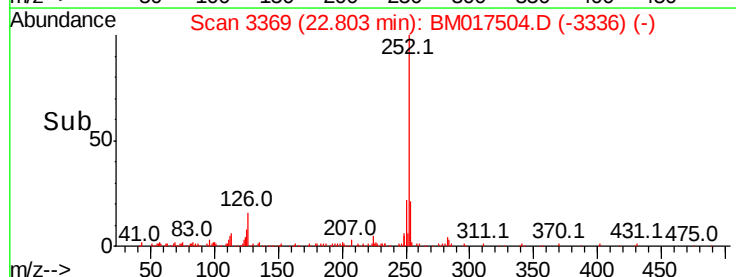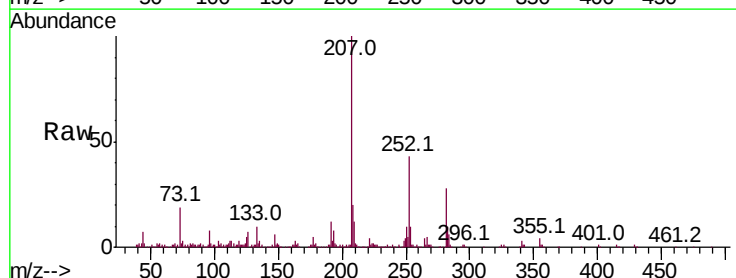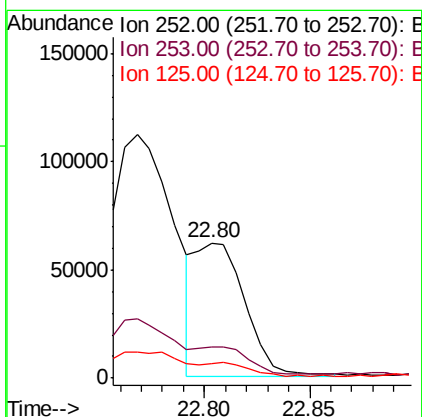

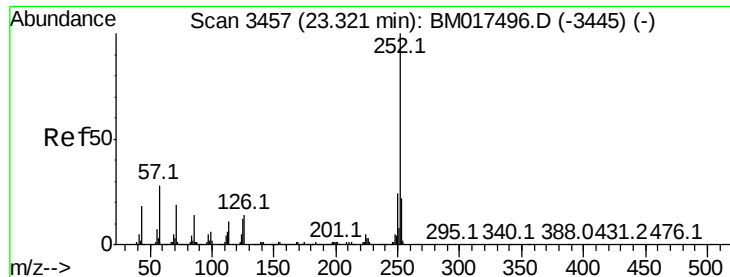

#91

Benzo(a)pyrene

Concen: 9.087 ng/ul

RT: 23.33 min Scan# 3458

Delta R.T. 0.01 min

Lab File: BM017504.D

Acq: 02 Nov 2018 23:38

Instrument :

BNA_M


ClientSampleId :

A40K3MS




Tot Ion:	252	Resp:	181694
Ion Ratio	Lower	Upper	
252	100		
253	23.8	17.6	26.4
125	11.5	8.3	12.5

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:08 PM

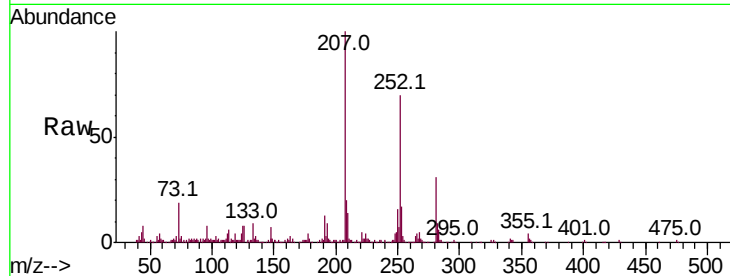

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

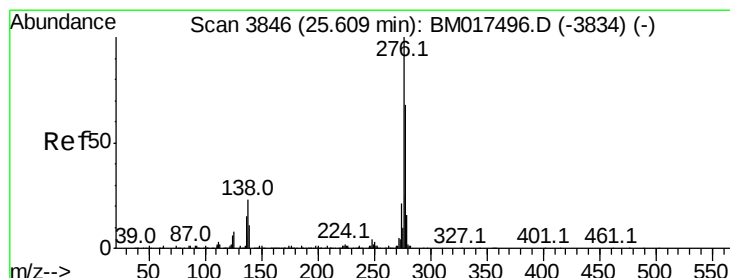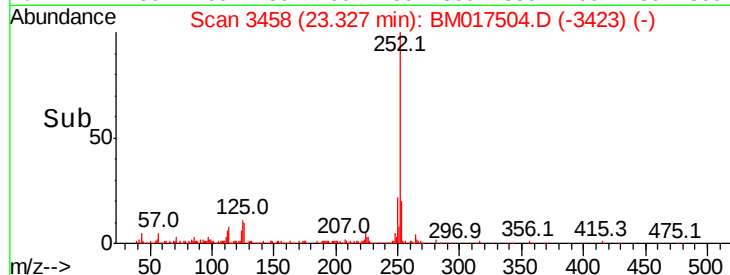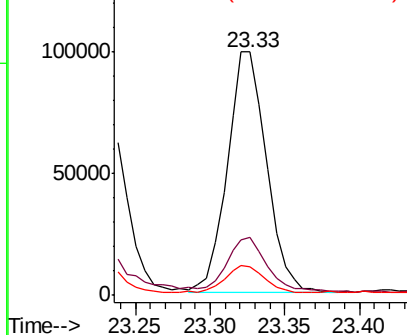

#92

Indeno(1,2,3-cd)pyrene

Concen: 3.965 ng/ul

RT: 25.61 min Scan# 3847




Delta R.T. 0.01 min


Lab File: BM017504.D

Acq: 02 Nov 2018 23:38

Tgt Ion:	276	Resp:	96452
Ion Ratio	Lower	Upper	
276	100		
138	21.4	18.1	27.1
277	24.7	19.6	29.4

Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E

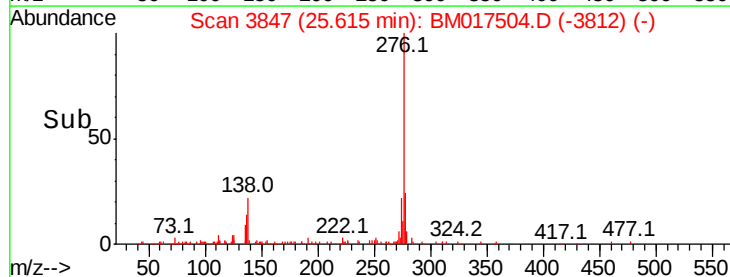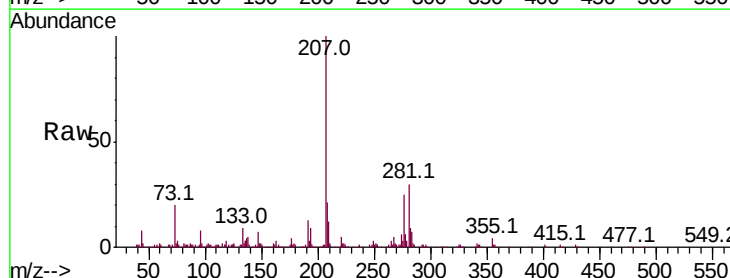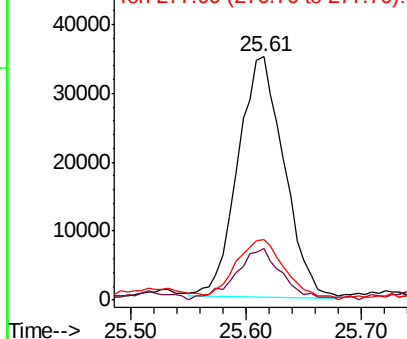

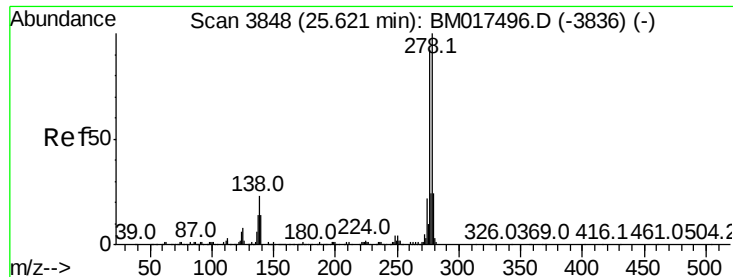





#93
Dibenzo(a,h)anthracene
Concen: 1.585 ng/ul
RT: 25.62 min Scan# 3848
Delta R.T. -0.00 min
Lab File: BM017504.D
Acq: 02 Nov 2018 23:38

Instrument :
BNA_M
ClientSampled :
A40K3MS

Tot Ion	Ratio	Lower	Upper
278	100		
139	20.2	12.7	19.1#
279	25.5	19.0	28.4

Manual Integrations
APPROVED

Sohil
11/5/2018 4:06:08 PM

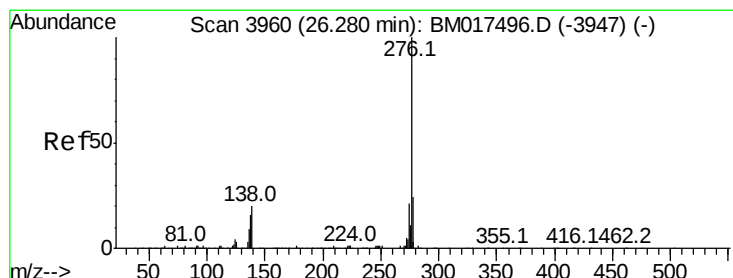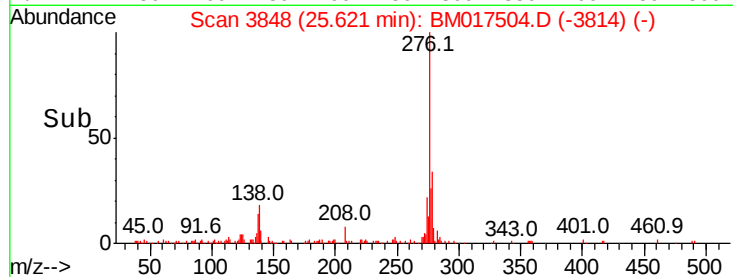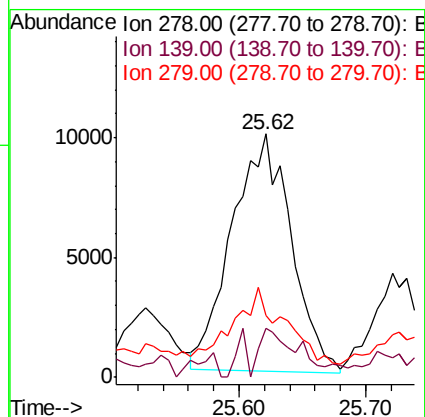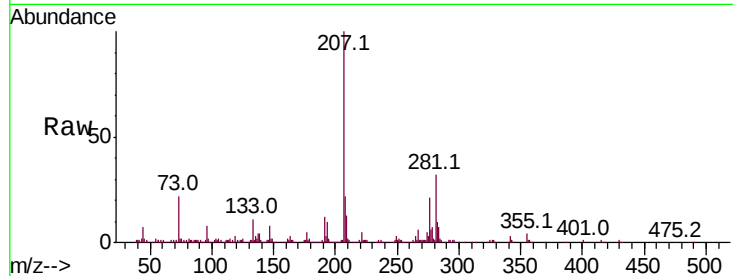

#94
Benzo(g,h,i)perylene
Concen: 3.918 ng/ul
RT: 26.29 min Scan# 3961
Delta R.T. 0.01 min
Lab File: BM017504.D
Acq: 02 Nov 2018 23:38

Tgt Ion	Ratio	Lower	Upper
276	100		
138	18.4	16.6	25.0
277	23.4	18.9	28.3

