

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110218\
 Data File : BM017507.D
 Acq On : 03 Nov 2018 01:27
 Operator : MJ/SJ
 Sample : J5704-23
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A40J1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	35	38	46	rVB	31555	48467	2.56%	0.196%
2	3.710	119	123	130	rVB	28593	44342	2.34%	0.179%
3	3.816	137	141	149	rVB	26898	42015	2.22%	0.170%
4	4.069	182	184	189	rVB3	4448	4690	0.25%	0.019%
5	4.128	192	194	199	rVB5	3062	2603	0.14%	0.011%
6	4.451	246	249	251	rBV3	3777	4720	0.25%	0.019%
7	4.675	286	287	290	rBV3	2512	2698	0.14%	0.011%
8	4.798	304	308	309	rBV2	6272	7989	0.42%	0.032%
9	5.498	425	427	431	rBV4	1847	2439	0.13%	0.010%
10	5.563	436	438	444	rVB4	2146	2631	0.14%	0.011%
11	5.669	453	456	461	rBV5	3330	5983	0.32%	0.024%
12	5.875	489	491	494	rVB3	2133	2475	0.13%	0.010%
13	6.310	562	565	568	rBV3	2579	4172	0.22%	0.017%
14	6.722	634	635	639	rVB3	2381	2455	0.13%	0.010%
15	6.810	644	650	665	rVV2	566660	1179493	62.27%	4.767%
16	6.975	672	678	693	rVB	441143	711578	37.57%	2.876%
17	7.169	704	711	721	rBV	606770	1014917	53.58%	4.102%
18	7.628	782	789	799	rBV	652553	1084406	57.25%	4.383%
19	7.698	799	801	805	rVB5	7251	9132	0.48%	0.037%
20	7.775	811	814	816	rBV2	2190	2423	0.13%	0.010%
21	8.339	902	910	924	rBV	575579	1036964	54.75%	4.191%
22	8.539	943	944	950	rVB3	2326	3186	0.17%	0.013%
23	8.781	978	985	997	rBV	520982	919552	48.55%	3.717%
24	9.075	1033	1035	1040	rBV5	2565	4869	0.26%	0.020%
25	9.181	1049	1053	1059	rBV3	9135	12578	0.66%	0.051%
26	9.498	1098	1107	1118	rBV	422575	737422	38.93%	2.980%
27	10.033	1190	1198	1220	rBV	528406	1074742	56.74%	4.344%
28	10.398	1253	1260	1273	rVB	850906	1441992	76.13%	5.828%
29	10.551	1280	1286	1306	rBV	373306	885637	46.76%	3.579%
30	10.698	1309	1311	1315	rVB5	4437	5020	0.27%	0.020%
31	11.416	1431	1433	1438	rBV3	1491	2414	0.13%	0.010%
32	11.669	1473	1476	1478	rBV2	2760	2952	0.16%	0.012%
33	12.016	1531	1535	1546	rBV5	6621	15201	0.80%	0.061%
34	12.127	1549	1554	1556	rVB3	1893	2537	0.13%	0.010%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110218\
 Data File : BM017507.D
 Acq On : 03 Nov 2018 01:27
 Operator : MJ/SJ
 Sample : J5704-23
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A40J1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
 Title : SVOA CALIBRATION

35	12.486	1612	1615	1616	rBV3	1842	2442	0.13%	0.010%
36	12.622	1634	1638	1643	rBV6	3188	5051	0.27%	0.020%
37	13.104	1714	1720	1721	rVB5	2432	2634	0.14%	0.011%
38	13.580	1799	1801	1805	rVB4	3443	3253	0.17%	0.013%
39	13.692	1814	1820	1825	rBV	781193	1189406	62.79%	4.807%
40	13.739	1825	1828	1838	rVB	126227	193593	10.22%	0.782%
41	13.963	1859	1866	1877	rBV	1079087	1630853	86.10%	6.591%
42	14.186	1901	1904	1906	rBV3	2628	2652	0.14%	0.011%
43	14.274	1912	1919	1928	rBV2	978971	1548361	81.74%	6.258%
44	14.510	1953	1959	1980	rBV3	104699	337399	17.81%	1.364%
45	14.721	1991	1995	2003	rBV3	20551	34913	1.84%	0.141%
46	15.086	2053	2057	2059	rBV3	3502	4278	0.23%	0.017%
47	15.274	2082	2089	2101	rBV	1211527	1894139	100.00%	7.656%
48	15.404	2106	2111	2122	rBV2	197695	347192	18.33%	1.403%
49	15.521	2127	2131	2134	rVB6	11464	15721	0.83%	0.064%
50	15.692	2158	2160	2164	rBV3	2962	3570	0.19%	0.014%
51	16.004	2211	2213	2216	rBV3	3914	3611	0.19%	0.015%
52	16.233	2250	2252	2256	rVB3	3902	3995	0.21%	0.016%
53	16.274	2258	2259	2262	rBV2	4066	3435	0.18%	0.014%
54	16.945	2371	2373	2375	rBV3	3633	3984	0.21%	0.016%
55	17.027	2380	2387	2393	rBV	973827	1452259	76.67%	5.870%
56	17.127	2398	2404	2418	rVB	1035650	1638182	86.49%	6.621%
57	17.262	2425	2427	2430	rBV3	4296	5331	0.28%	0.022%
58	17.674	2496	2497	2499	rBV2	4956	3732	0.20%	0.015%
59	17.804	2517	2519	2524	rVB6	8282	10393	0.55%	0.042%
60	17.933	2536	2541	2552	rBV3	61720	116127	6.13%	0.469%
61	19.427	2790	2795	2803	rBV	1179821	1656310	87.44%	6.694%
62	21.227	3096	3101	3109	rBV	815083	1170785	61.81%	4.732%
63	23.280	3447	3450	3462	rVB	632623	1133843	59.86%	4.583%


Sum of corrected areas: 24742138

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110218\
Data File : BM017507.D
Acq On : 03 Nov 2018 01:27
Operator : MJ/SJ
Sample : J5704-23
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40J1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

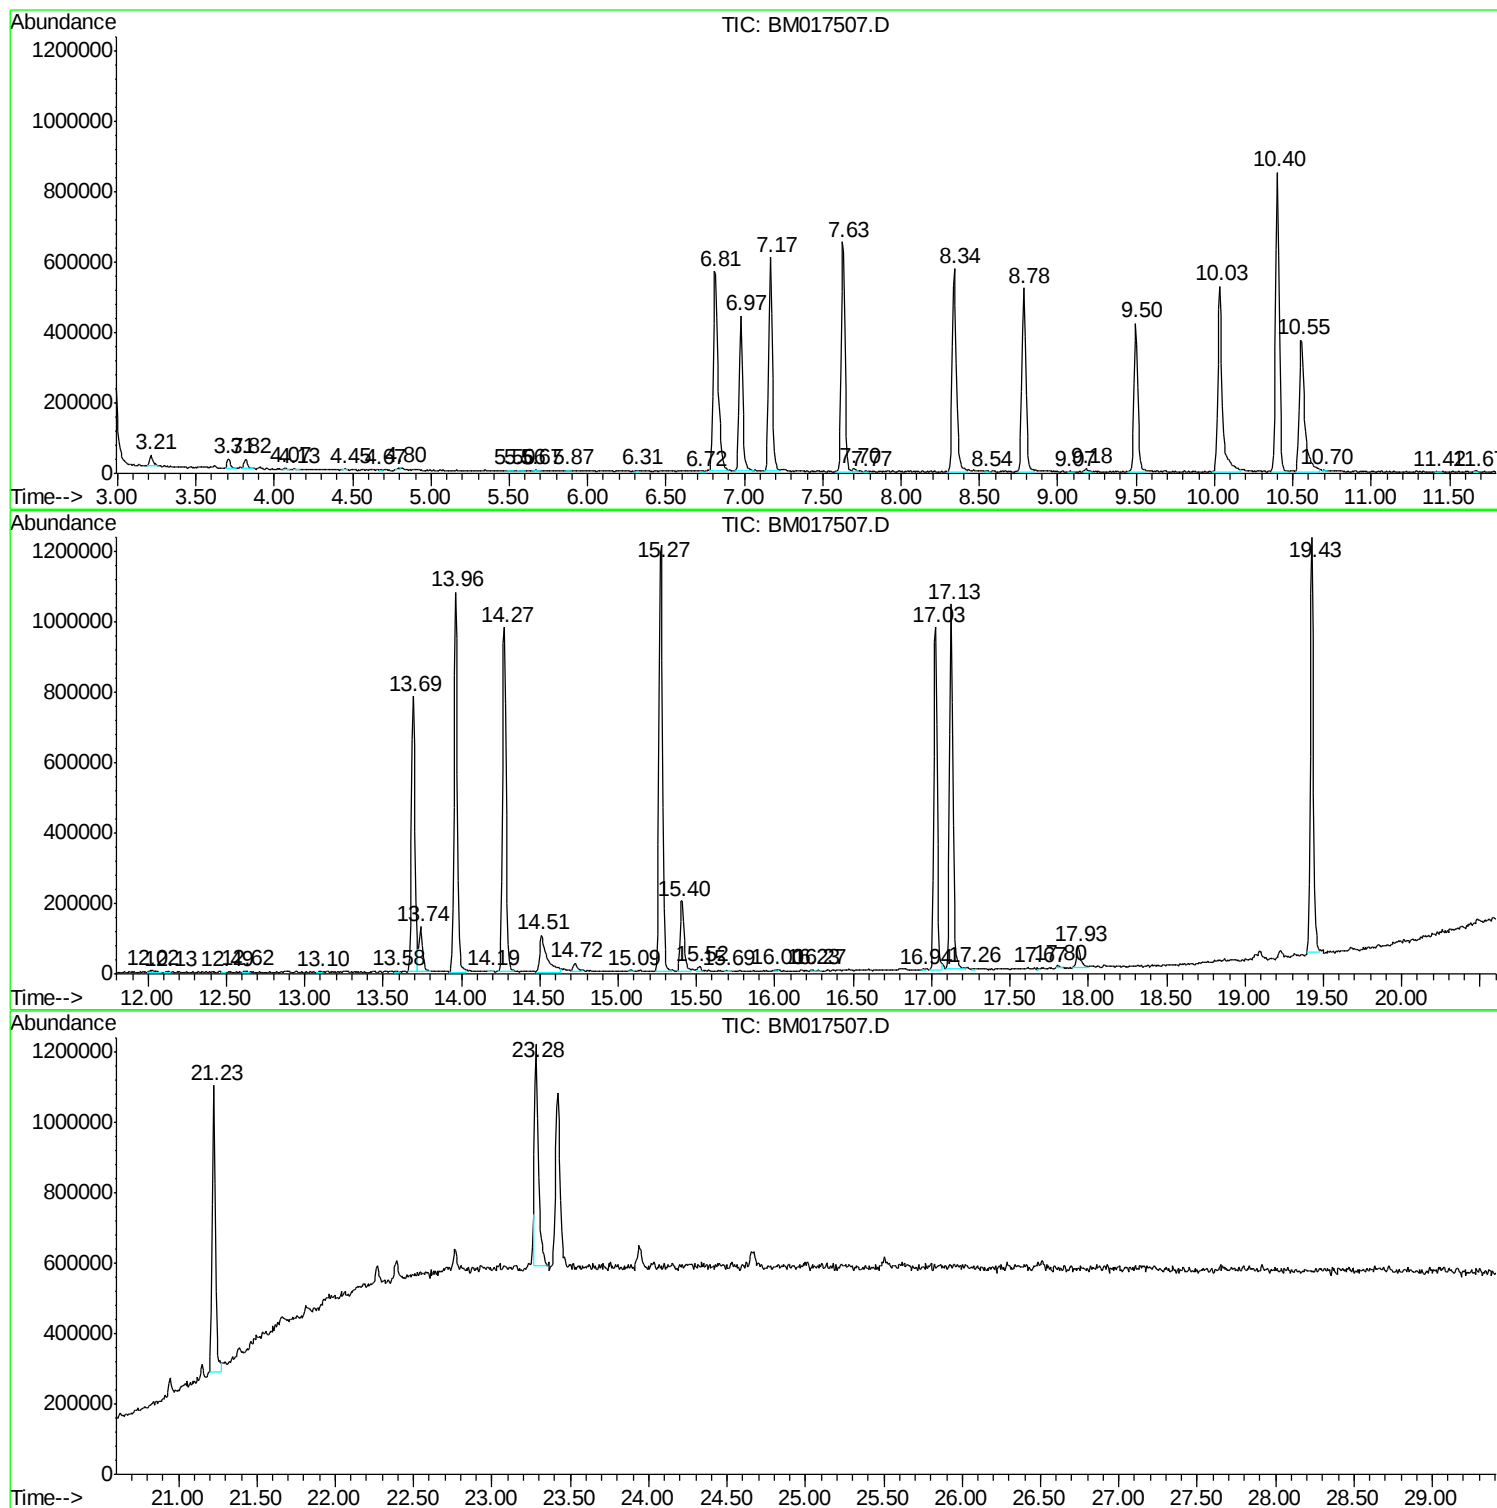

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Data File : BM017507.D
Acq On : 03 Nov 2018 01:27
Operator : MJ/SJ
Sample : J5704-23
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40J1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110218\
Data File : BM017507.D
Acq On : 03 Nov 2018 01:27
Operator : MJ/SJ
Sample : J5704-23
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A40J1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc