
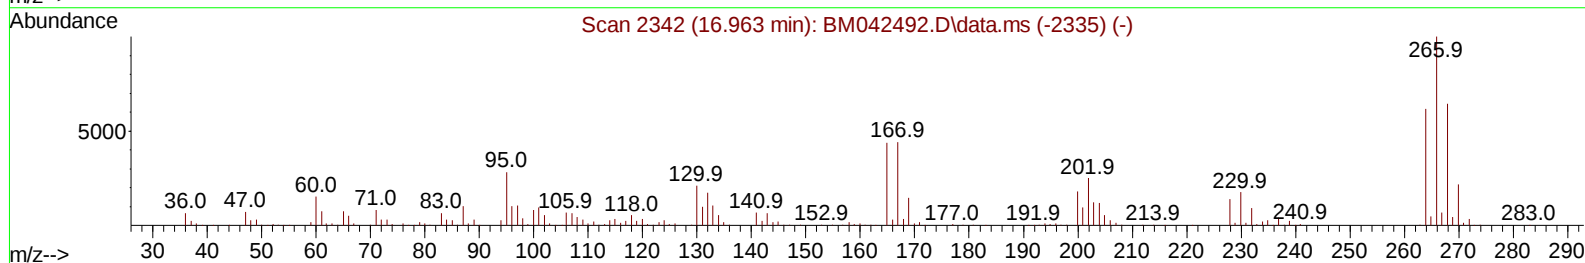
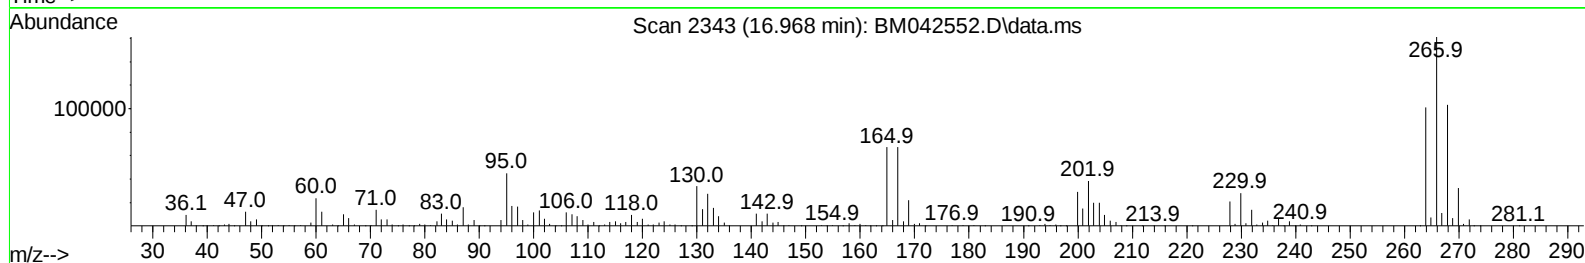


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110223\
Data File : BM042552.D
Acq On : 02 Nov 2023 09:27
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 23:00:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 31 02:55:18 2023
Response via : Initial Calibration

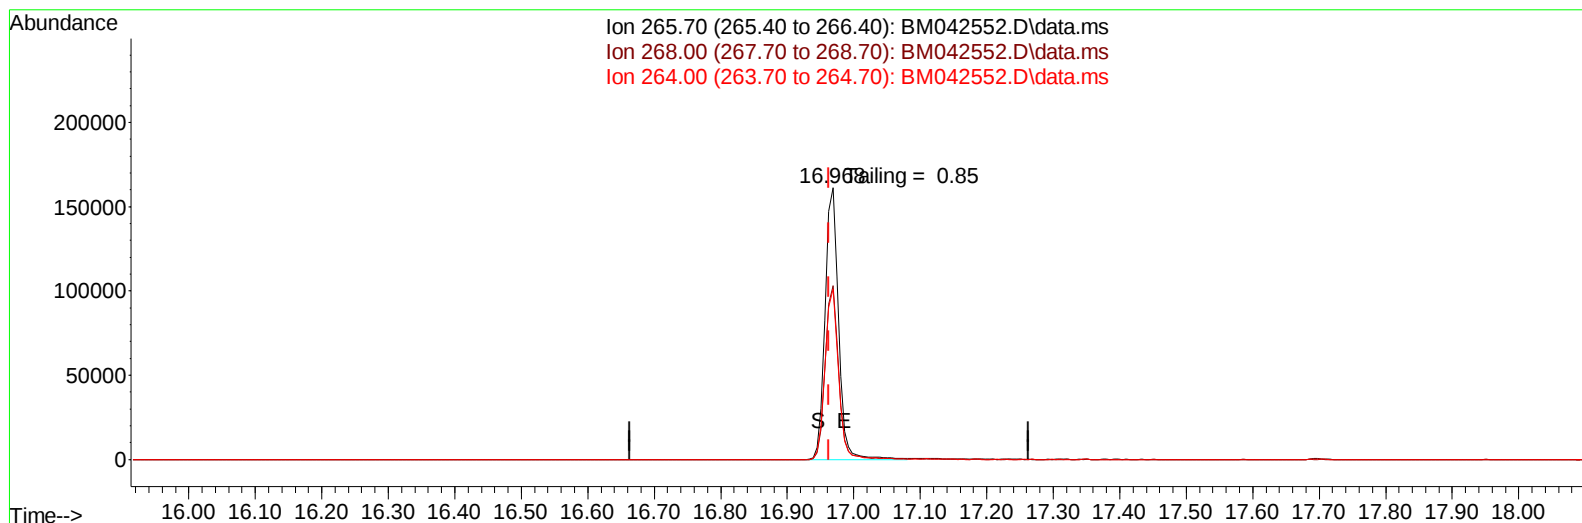

TIC: BM042552.D\data.ms

(70) Pentachlorophenol (C)




16.968min (+ 0.005) 324615.78 ng

response 224400

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	64.02
264.00	61.80	62.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110223\
Data File : BM042552.D
Acq On : 02 Nov 2023 09:27
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 23:00:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 31 02:55:18 2023
Response via : Initial Calibration

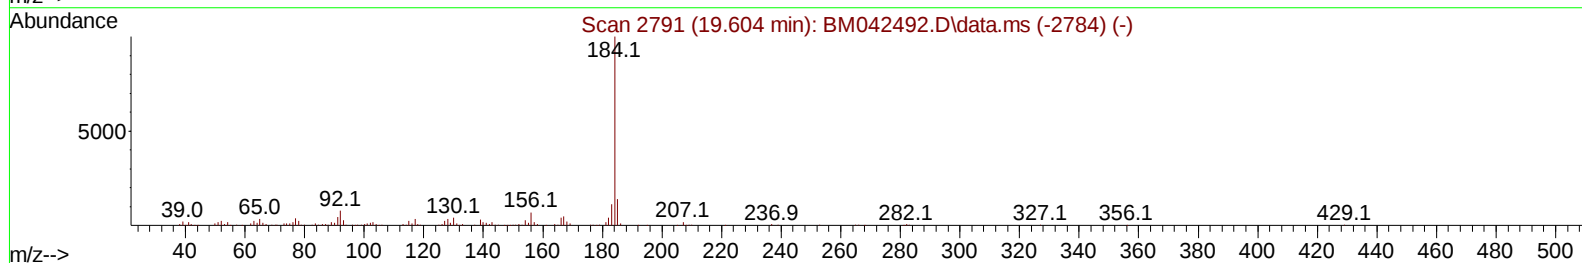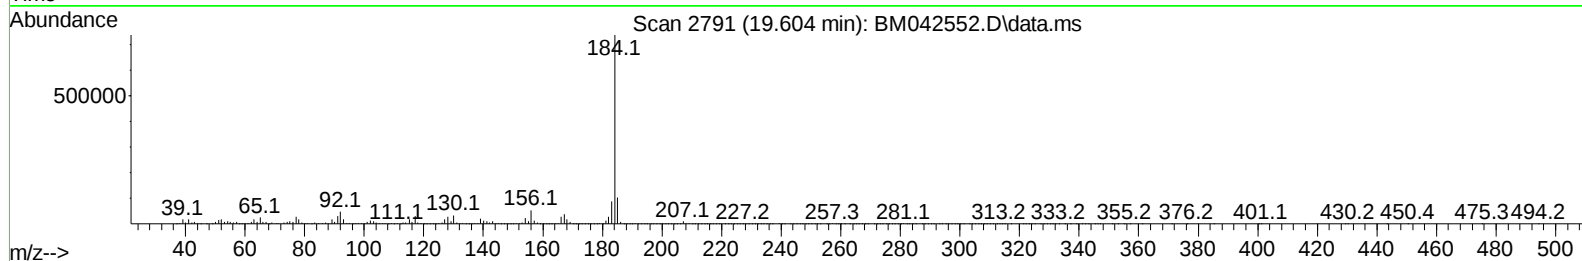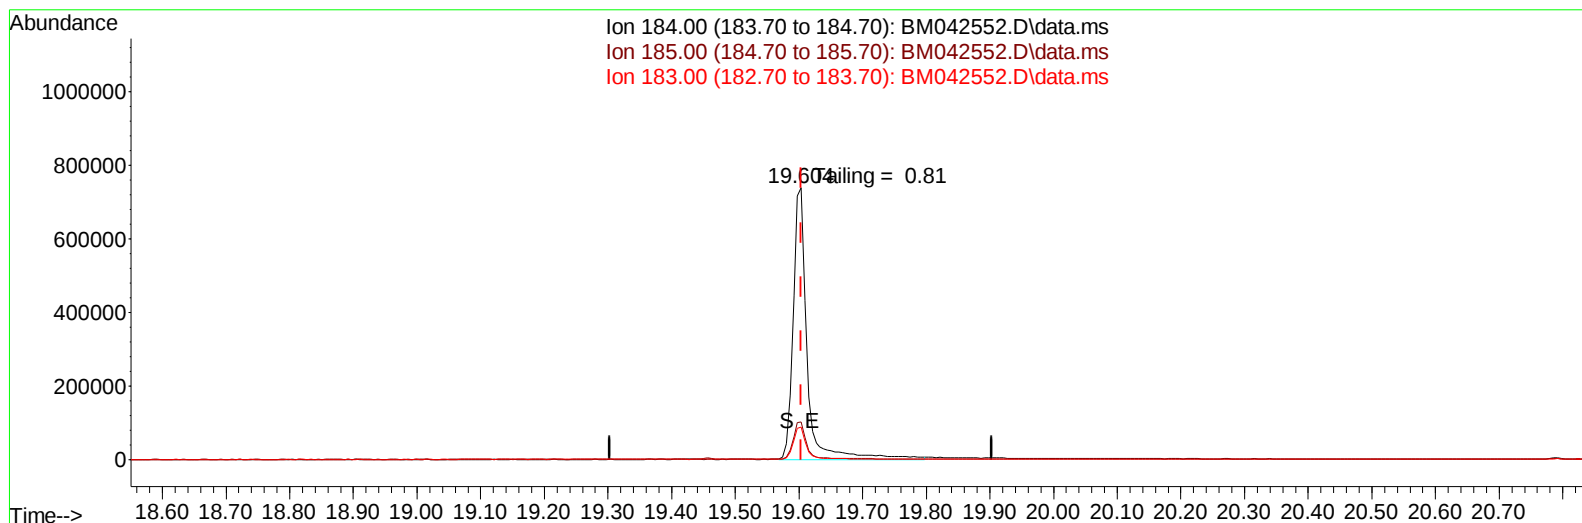

TIC: BM042552.D\data.ms

(77) Benzidine**19.604min (-0.000) 94164.56 ng****response 1150744**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.92
183.00	11.20	11.84
0.00	0.00	0.00