

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110223\
 Data File : BM042565.D
 Acq On : 02 Nov 2023 17:25
 Operator : MA/JU
 Sample : 04938-18DL2 100X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0-3(5-10)DL2

Quant Time: Nov 02 22:42:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 31 02:55:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	50344	20.000	ng	0.00
21) Naphthalene-d8	10.739	136	193314	20.000	ng	-0.01
39) Acenaphthene-d10	14.569	164	114484	20.000	ng	-0.01
64) Phenanthrene-d10	17.321	188	246542	20.000	ng	# 0.00
76) Chrysene-d12	21.503	240	262363	20.000	ng	0.00
86) Perylene-d12	23.927	264	309249	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.457	112	2706	0.867	ng	0.00
7) Phenol-d6	7.093	99	3610	0.844	ng	0.00
23) Nitrobenzene-d5	9.134	82	2734	0.659	ng	0.00
42) 2,4,6-Tribromophenol	16.080	330	773	0.517	ng	0.00
45) 2-Fluorobiphenyl	13.192	172	6762	0.795	ng	0.00
79) Terphenyl-d14	19.939	244	11329	0.732	ng	0.00
Target Compounds						
31) Naphthalene	10.786	128	130858	13.102	ng	99
37) 2-Methylnaphthalene	12.398	142	19660	2.795	ng	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110223\
Data File : BM042565.D
Acq On : 02 Nov 2023 17:25
Operator : MA/JU
Sample : 04938-18DL2 100X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0-3(5-10)DL2

Quant Time: Nov 02 22:42:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 31 02:55:18 2023
Response via : Initial Calibration




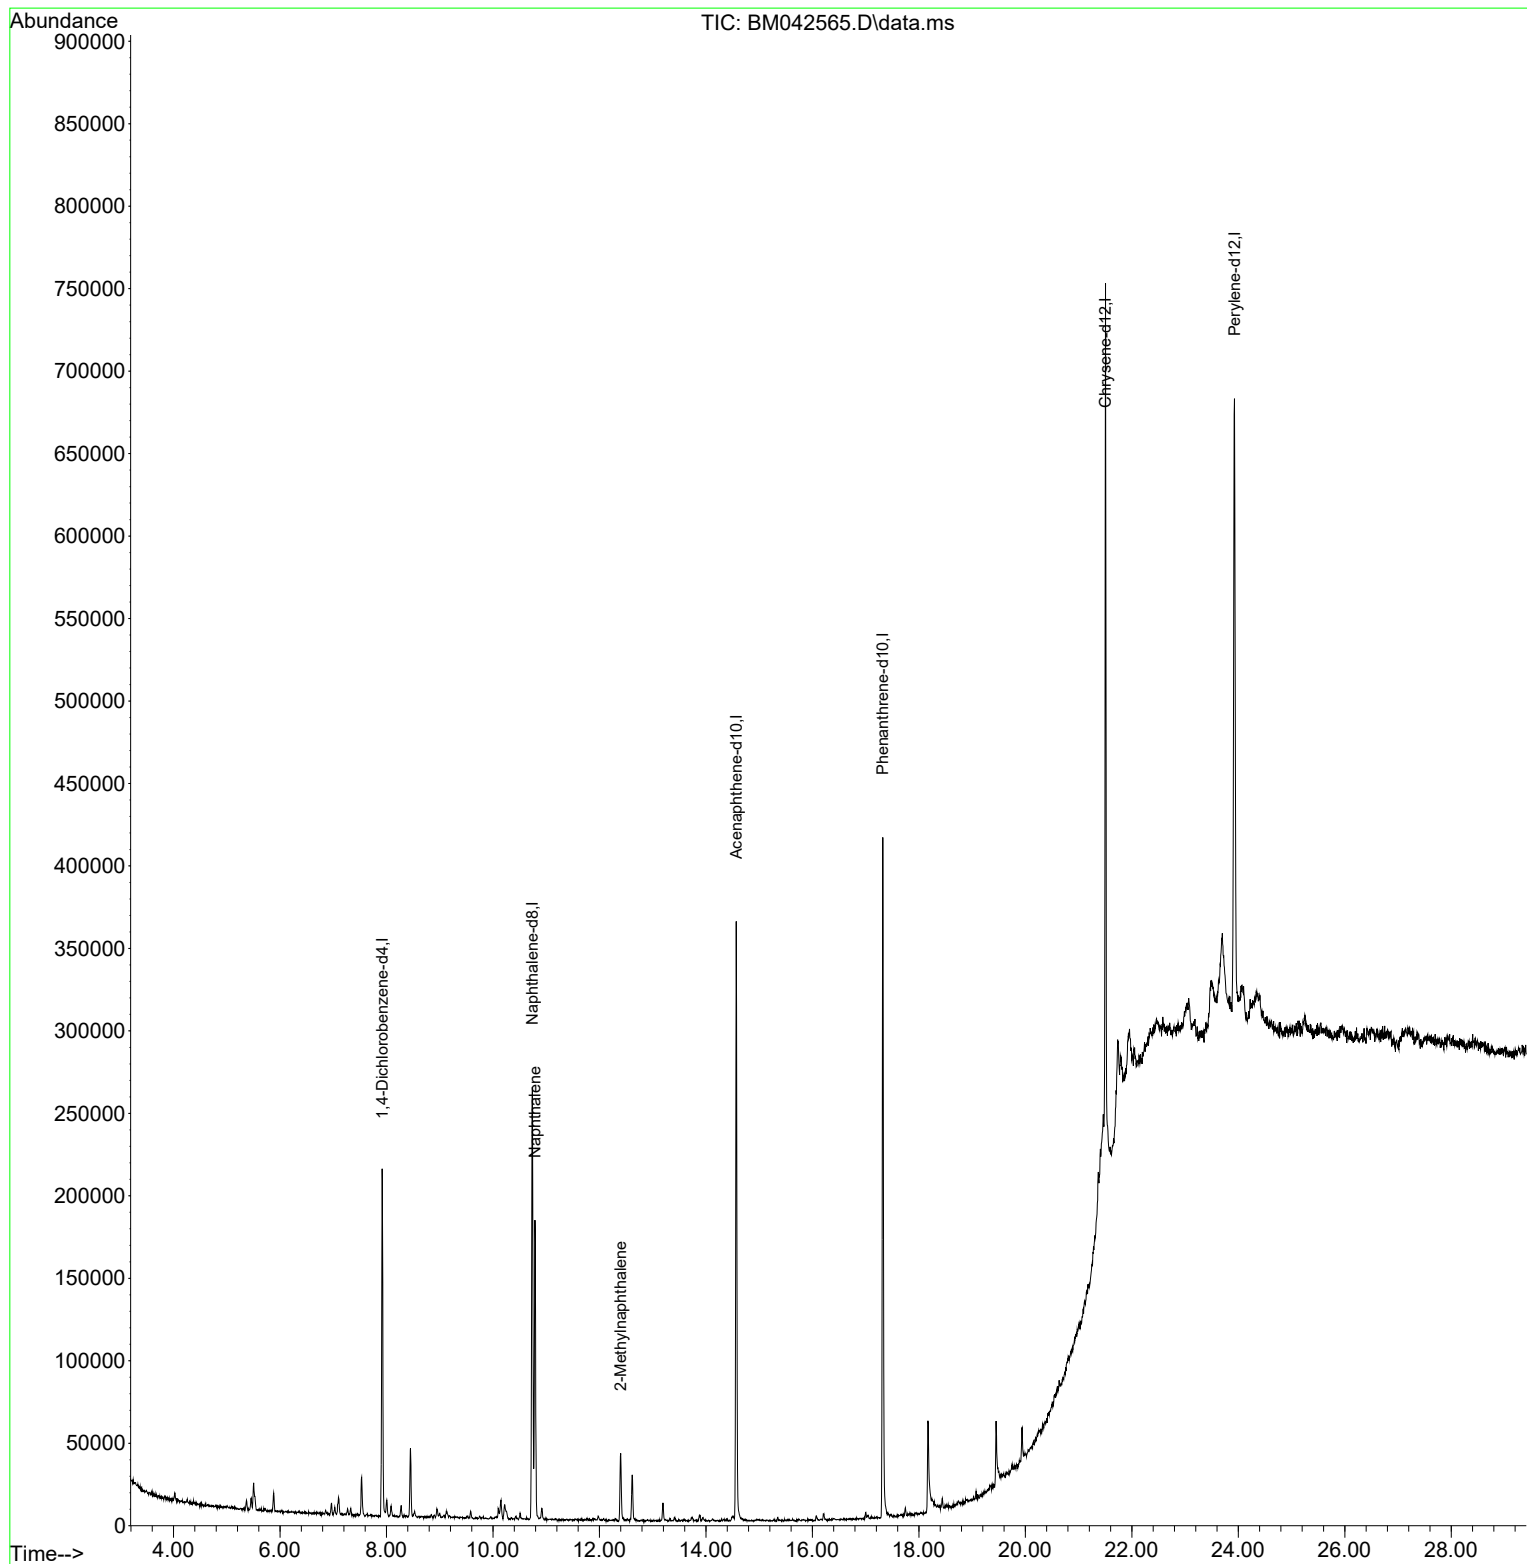




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.922 min Scan# 806
Delta R.T. -0.006 min
Lab File: BM042565.D
Acq: 02 Nov 2023 17:25




Instrument :
BNA_M
ClientSampleId :
0-3(5-10)DL2


Tgt Ion:152 Resp: 50344
Ion Ratio Lower Upper
152 100
150 152.1 127.4 191.0
115 57.6 47.9 71.9

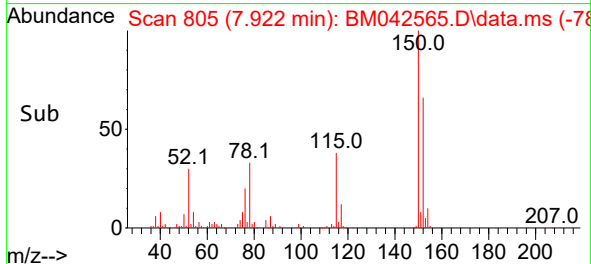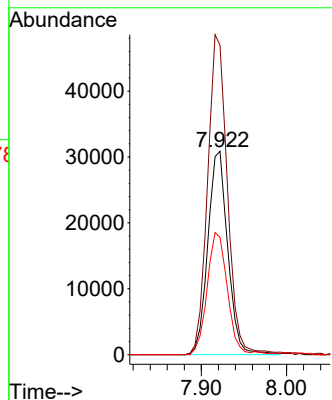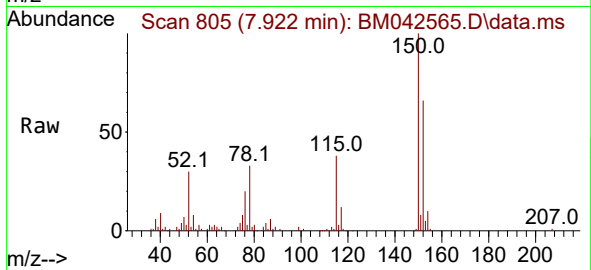

#5
2-Fluorophenol
Concen: 0.867 ng
RT: 5.457 min Scan# 386
Delta R.T. -0.006 min
Lab File: BM042565.D
Acq: 02 Nov 2023 17:25

Tgt Ion:112 Resp: 2706
Ion Ratio Lower Upper
112 100
64 63.5 52.1 78.1
63 32.1 28.3 42.5


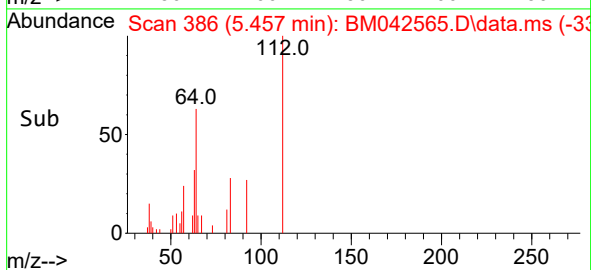
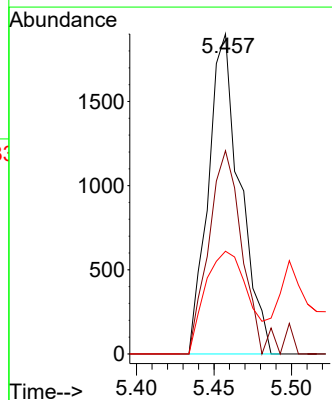
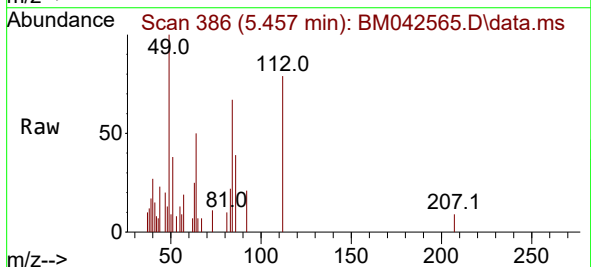




#7
Phenol-d6
Concen: 0.844 ng
RT: 7.093 min Scan# 61
Delta R.T. -0.006 min
Lab File: BM042565.D
Acq: 02 Nov 2023 17:25




Instrument :
BNA_M
ClientSampleId :
0-3(5-10)DL2


Tgt Ion: 99 Resp: 3610
Ion Ratio Lower Upper
99 100
42 34.6 18.7 28.1#
71 30.9 29.1 43.7

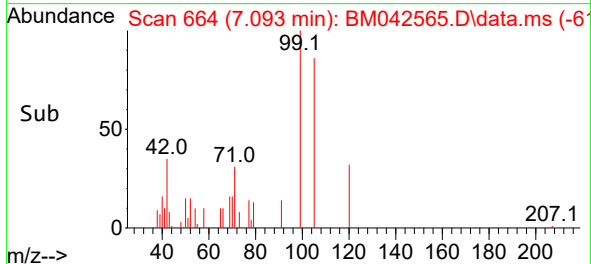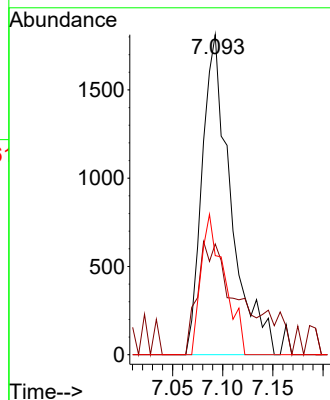

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.739 min Scan# 1284
Delta R.T. -0.012 min
Lab File: BM042565.D
Acq: 02 Nov 2023 17:25

Tgt Ion:136 Resp: 193314
Ion Ratio Lower Upper
136 100
137 10.6 9.0 13.6
54 10.6 8.0 12.0
68 6.6 5.7 8.5

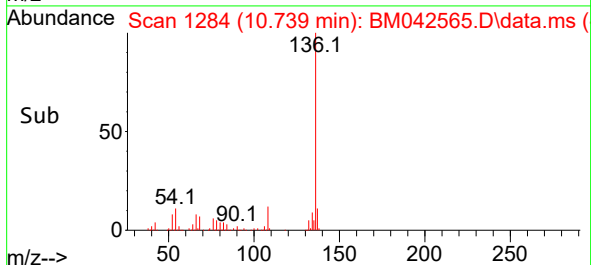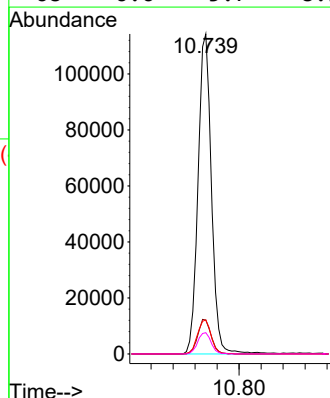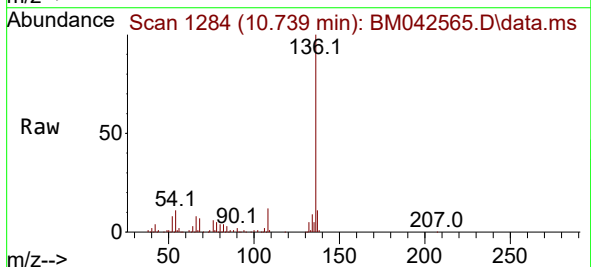

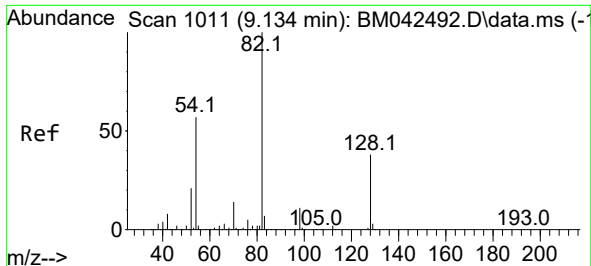

#23

Nitrobenzene-d5

Concen: 0.659 ng

RT: 9.134 min Scan# 1011

Delta R.T. -0.000 min

Lab File: BM042565.D

Acq: 02 Nov 2023 17:25

Instrument :

BNA_M

ClientSampleId :

0-3(5-10)DL2





Tgt Ion: 82 Resp: 2734

Ion Ratio Lower Upper

82 100

128 27.5 30.7 46.1#

54 55.9 45.3 67.9

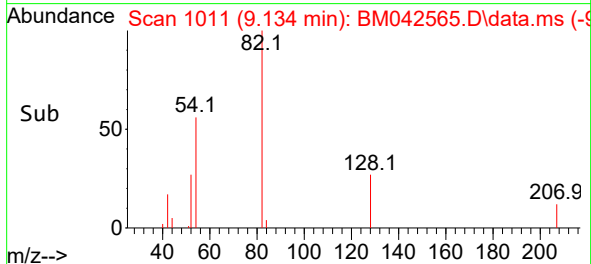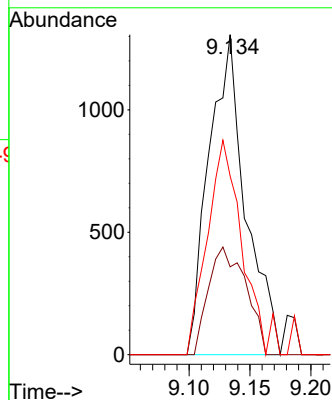

#31

Naphthalene

Concen: 13.102 ng

RT: 10.786 min Scan# 1292

Delta R.T. -0.012 min

Lab File: BM042565.D

Acq: 02 Nov 2023 17:25




Tgt Ion: 128 Resp: 130858


Ion Ratio Lower Upper

128 100

129 11.2 8.8 13.2

127 13.6 10.6 15.8


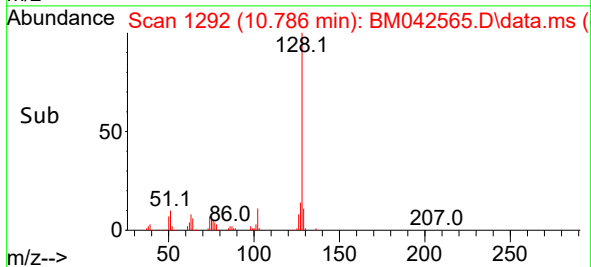
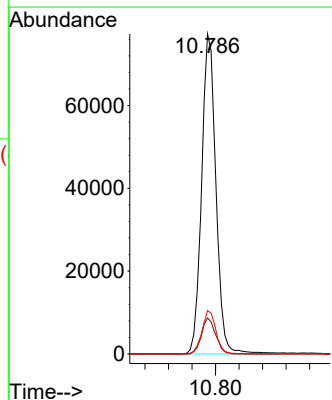
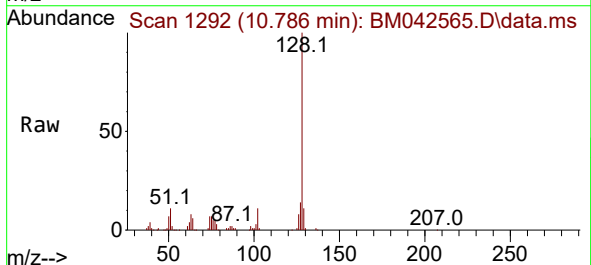




#37
2-Methylnaphthalene
Concen: 2.795 ng
RT: 12.398 min Scan# 1
Delta R.T. -0.006 min
Lab File: BM042565.D
Acq: 02 Nov 2023 17:25




Instrument :
BNA_M
ClientSampleId :
0-3(5-10)DL2


Tgt Ion:142 Resp: 19660
Ion Ratio Lower Upper
142 100
141 94.2 70.9 106.3
115 43.3 30.2 45.2

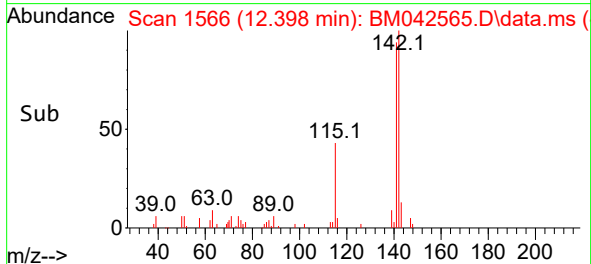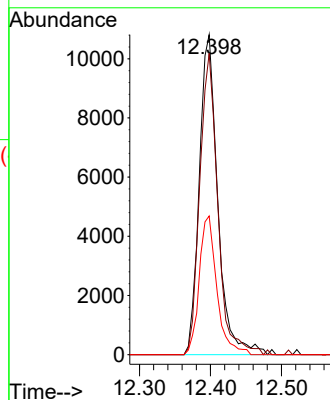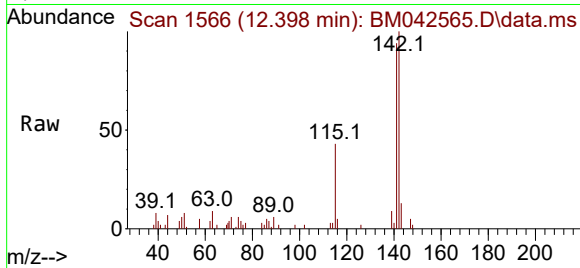

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.569 min Scan# 1935
Delta R.T. -0.011 min
Lab File: BM042565.D
Acq: 02 Nov 2023 17:25

Tgt Ion:164 Resp: 114484
Ion Ratio Lower Upper
164 100
162 103.2 81.6 122.4
160 46.5 36.2 54.4



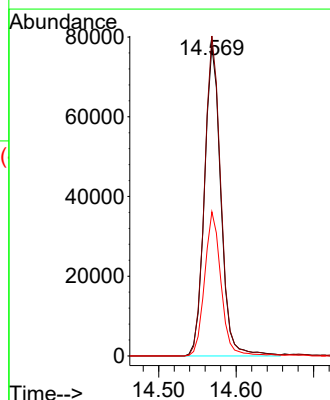
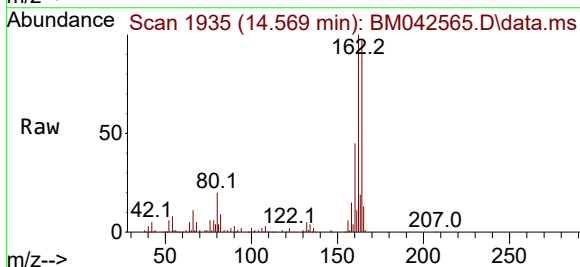


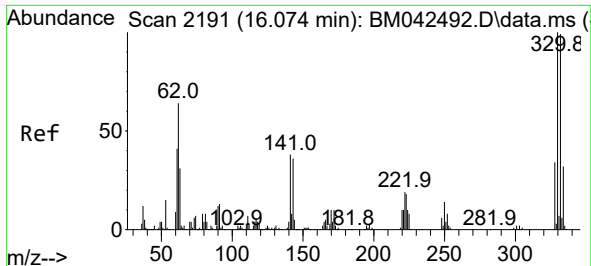

#42
2,4,6-Tribromophenol
Concen: 0.517 ng
RT: 16.080 min Scan# 2191
Delta R.T. 0.006 min
Lab File: BM042565.D
Acq: 02 Nov 2023 17:25




Instrument :
BNA_M
ClientSampleId :
0-3(5-10)DL2


Tgt Ion:330 Resp: 773
Ion Ratio Lower Upper
330 100
332 97.4 78.8 118.2
141 27.0 31.1 46.7#

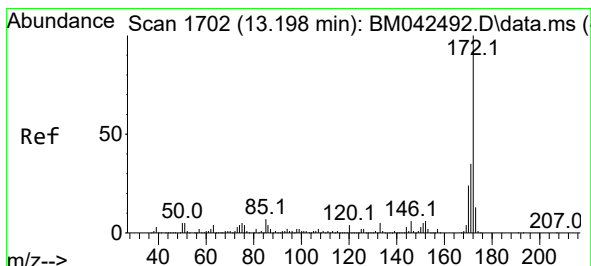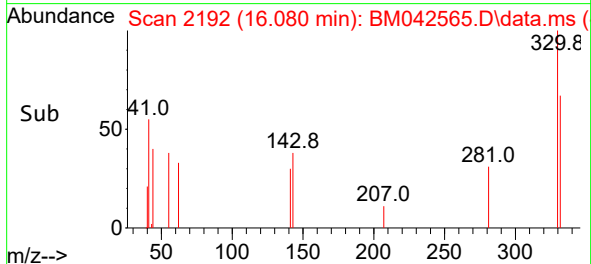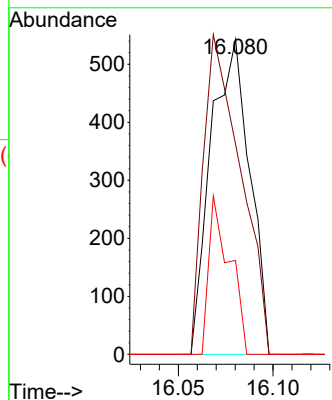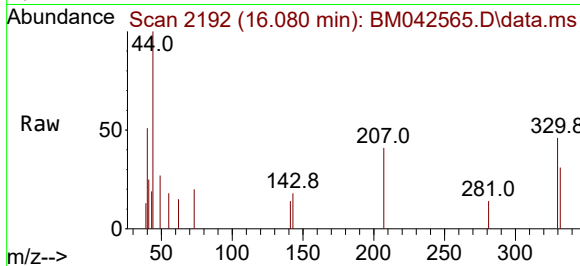

#45
2-Fluorobiphenyl
Concen: 0.795 ng
RT: 13.192 min Scan# 1701
Delta R.T. -0.006 min
Lab File: BM042565.D
Acq: 02 Nov 2023 17:25

Tgt Ion:172 Resp: 6762
Ion Ratio Lower Upper
172 100
171 34.0 28.2 42.2
170 23.8 19.0 28.4

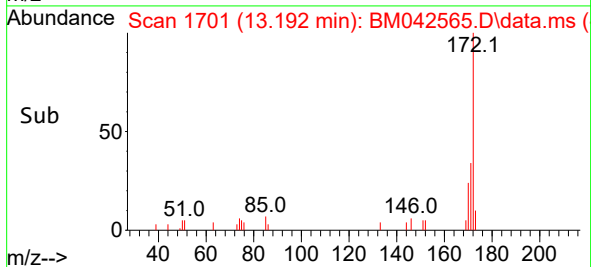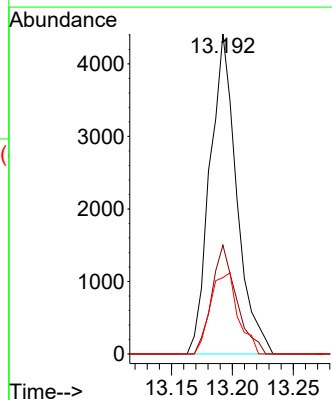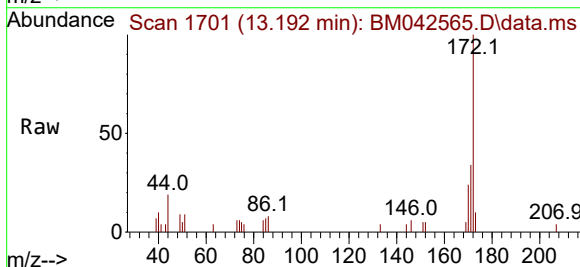



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.321 min Scan# 24

Delta R.T. -0.006 min

Lab File: BM042565.D

Acq: 02 Nov 2023 17:25

Instrument :

BNA_M

ClientSampleId :

0-3(5-10)DL2





Tgt Ion:188 Resp: 246542

Ion Ratio Lower Upper

188 100

94 8.2 8.2 12.4#

80 10.0 9.4 14.2

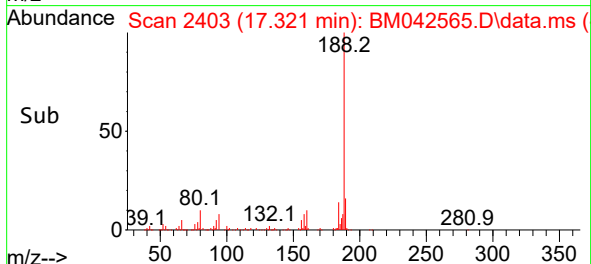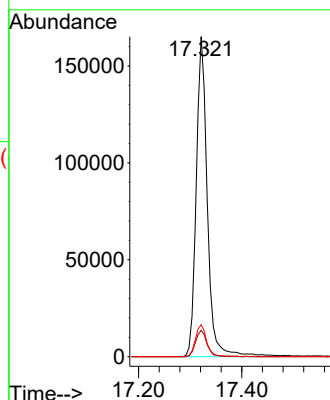

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.503 min Scan# 3114

Delta R.T. -0.006 min

Lab File: BM042565.D

Acq: 02 Nov 2023 17:25




Tgt Ion:240 Resp: 262363


Ion Ratio Lower Upper

240 100

120 9.4 8.3 12.5

236 26.2 20.8 31.2

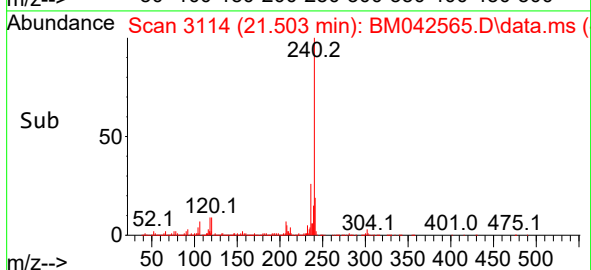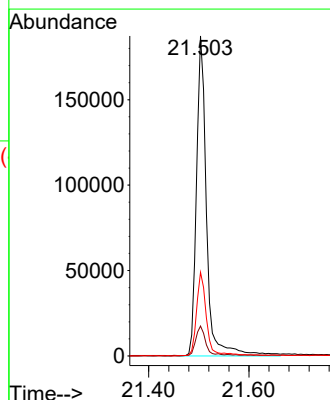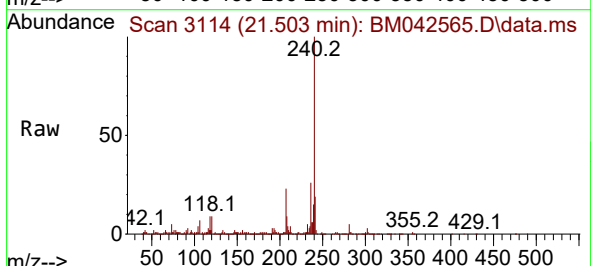



#79

Terphenyl-d14

Concen: 0.732 ng

RT: 19.939 min Scan# 21

Delta R.T. -0.006 min

Lab File: BM042565.D

Acq: 02 Nov 2023 17:25

Instrument :

BNA_M

ClientSampleId :

0-3(5-10)DL2





Tgt Ion:244 Resp: 11329

Ion Ratio Lower Upper

244 100

212 6.6 5.4 8.2

122 10.3 7.2 10.8

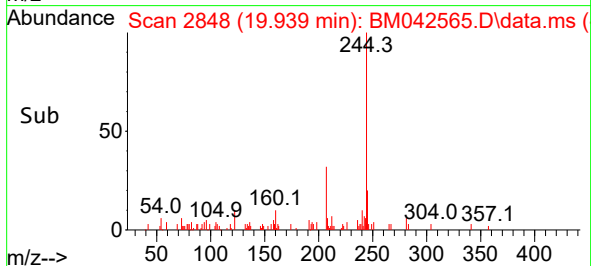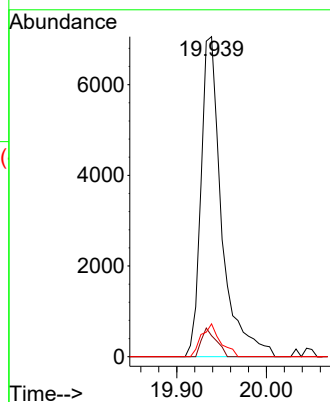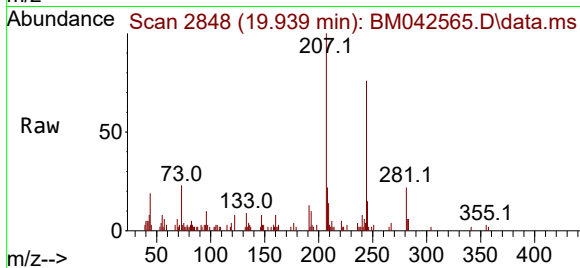

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.927 min Scan# 3526

Delta R.T. -0.006 min

Lab File: BM042565.D

Acq: 02 Nov 2023 17:25

Tgt Ion:264 Resp: 309249

Ion Ratio Lower Upper

264 100

260 24.1 19.0 28.4

265 21.9 18.7 28.1

