


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110223\
Data File : BM042552.D
Acq On : 02 Nov 2023 09:27
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 31 02:55:18 2023

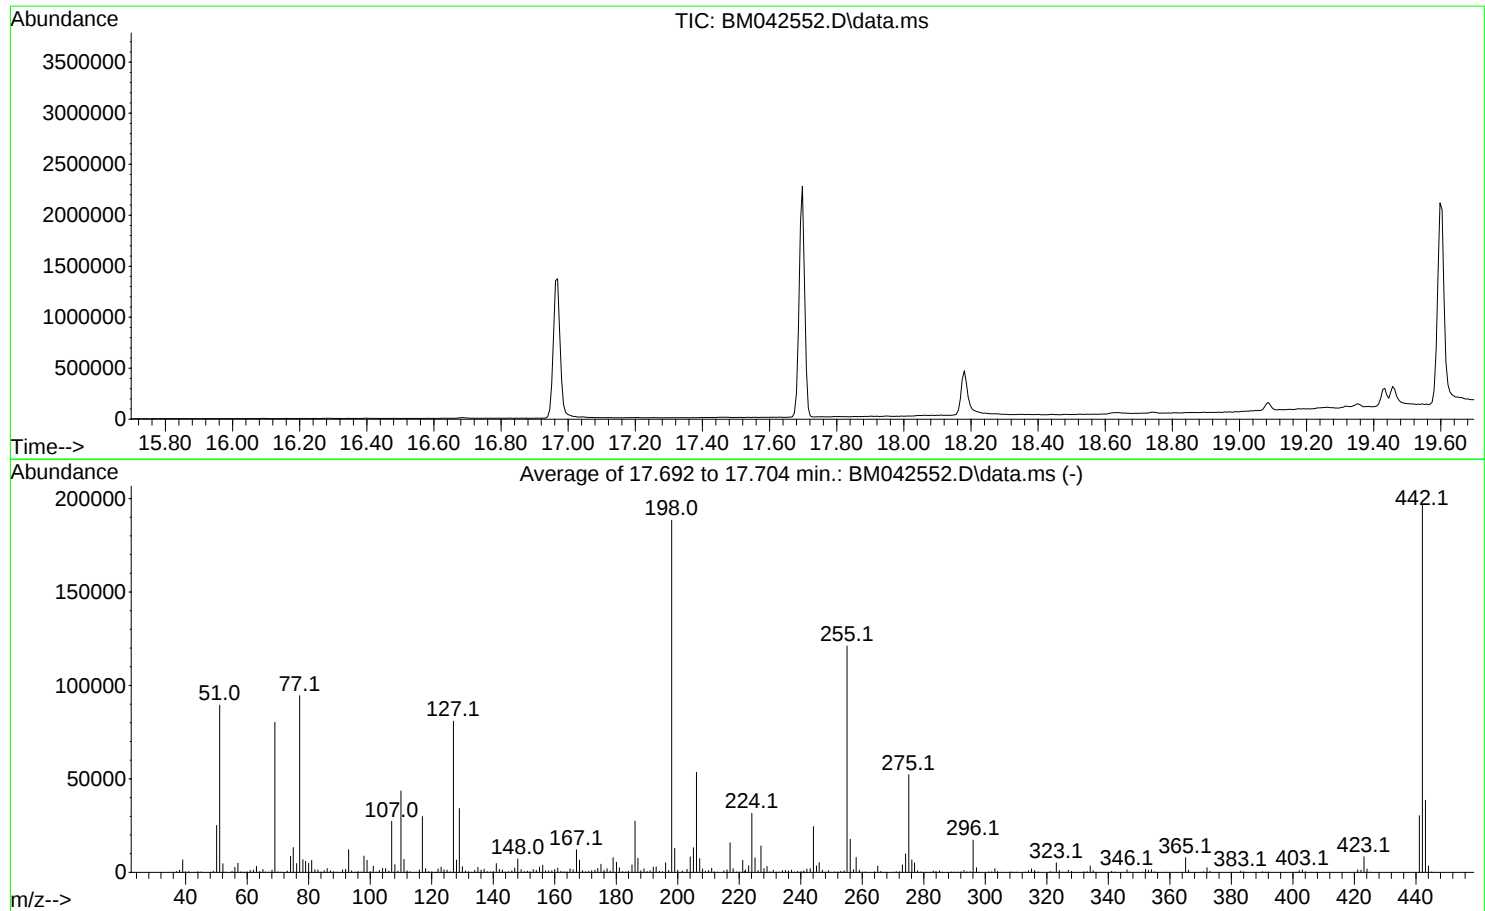




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.5	89483	PASS
68	69	0.00	2	1.6	1312	PASS
69	198	0.00	100	42.6	80302	PASS
70	69	0.00	2	0.4	352	PASS
127	198	10	80	42.9	80893	PASS
197	198	0.00	2	0.6	1055	PASS
198	198	100	100	100.0	188352	PASS
199	198	5	9	6.8	12875	PASS
275	198	10	60	27.7	52192	PASS
365	198	1	100	4.2	7904	PASS
441	198	0.01	100	16.1	30325	PASS
442	442	50	100	100.0	196800	PASS
443	442	15	24	19.6	38549	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110223\
Data File : BM042552.D
Acq On : 02 Nov 2023 09:27
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 02 23:00:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 31 02:55:18 2023
Response via : Initial Calibration

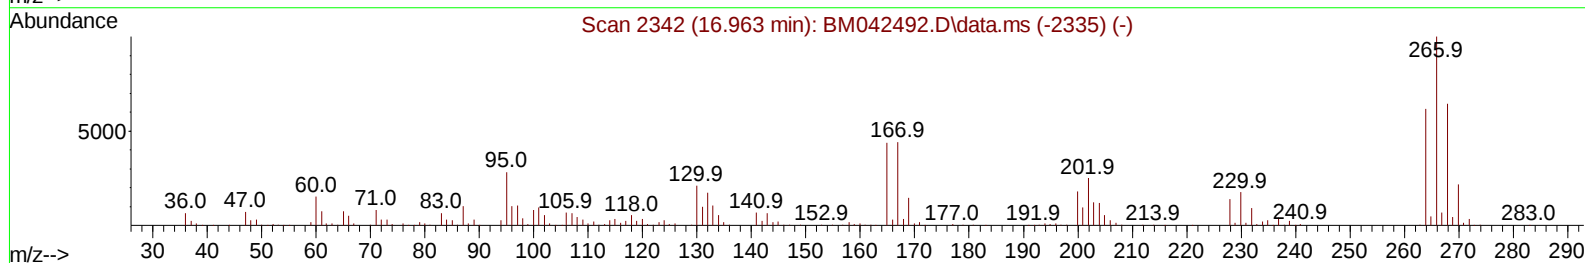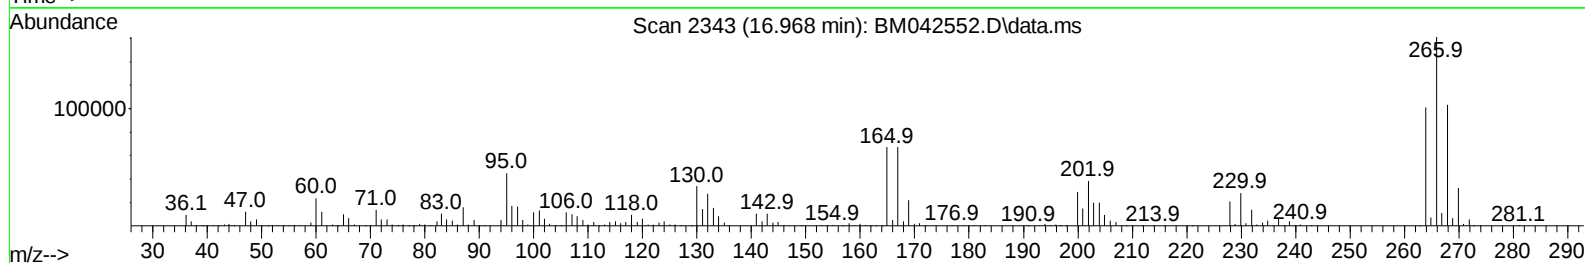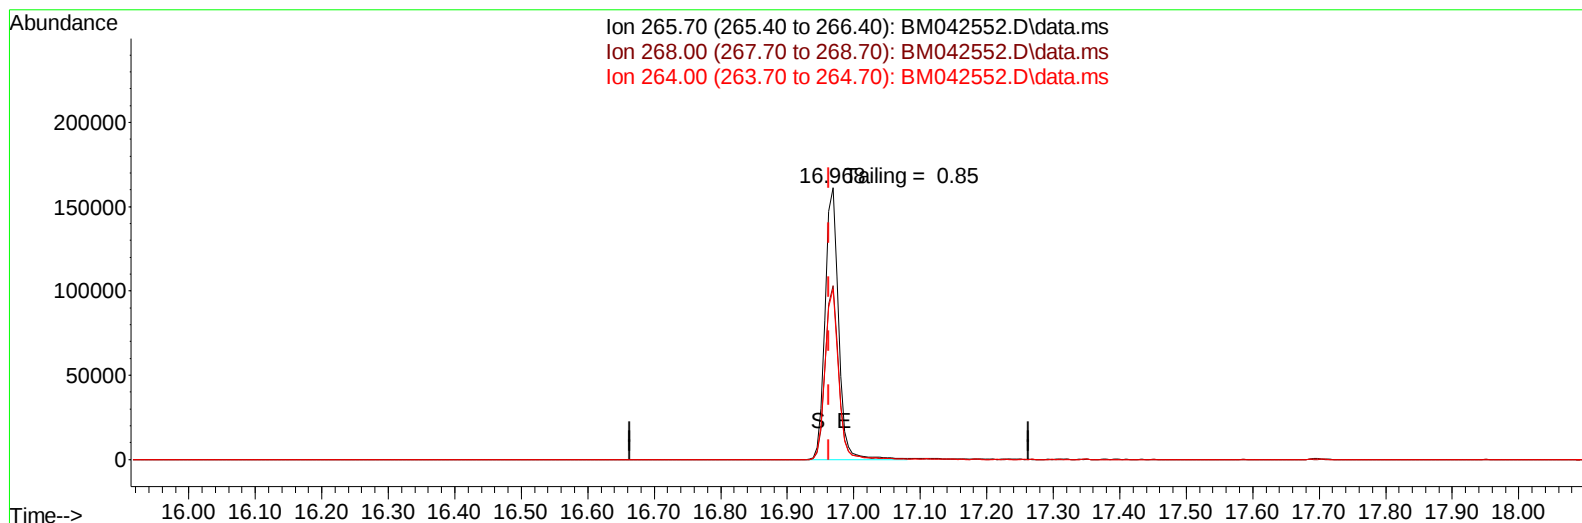

TIC: BM042552.D\data.ms

(70) Pentachlorophenol (C)

16.968min (+ 0.005) 324615.78 ng




response 224400

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	64.02
264.00	61.80	62.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110223\
Data File : BM042552.D
Acq On : 02 Nov 2023 09:27
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 02 23:00:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 31 02:55:18 2023
Response via : Initial Calibration

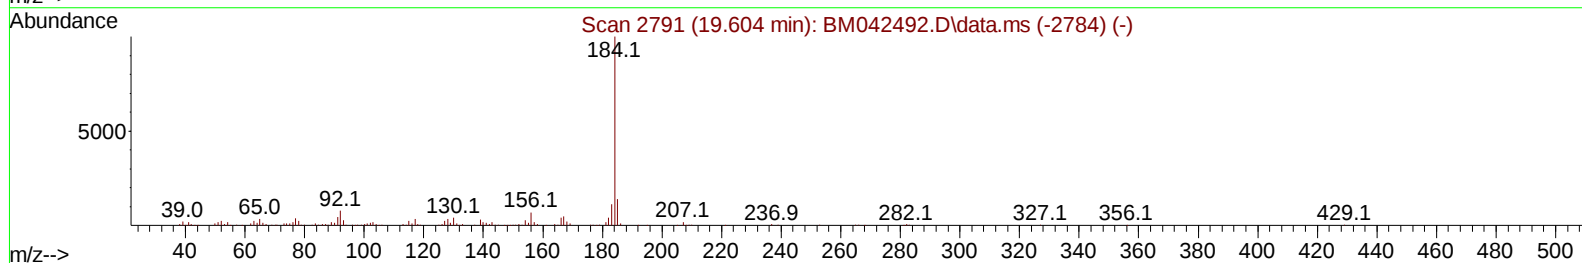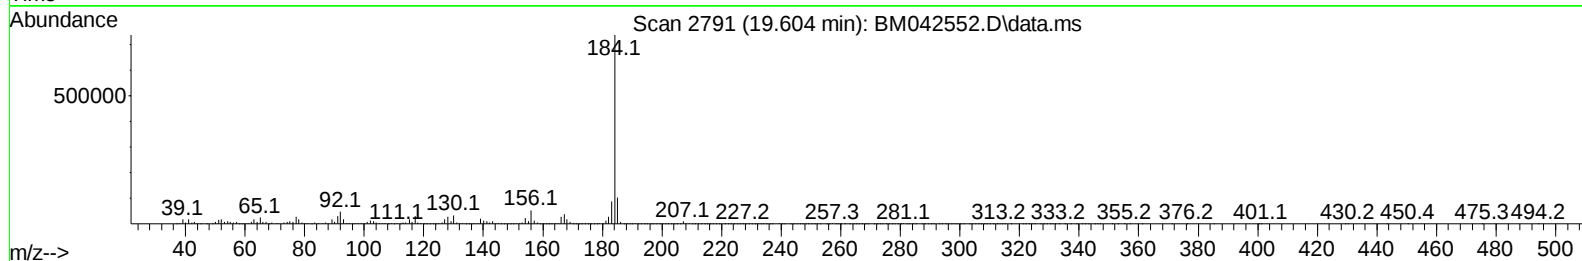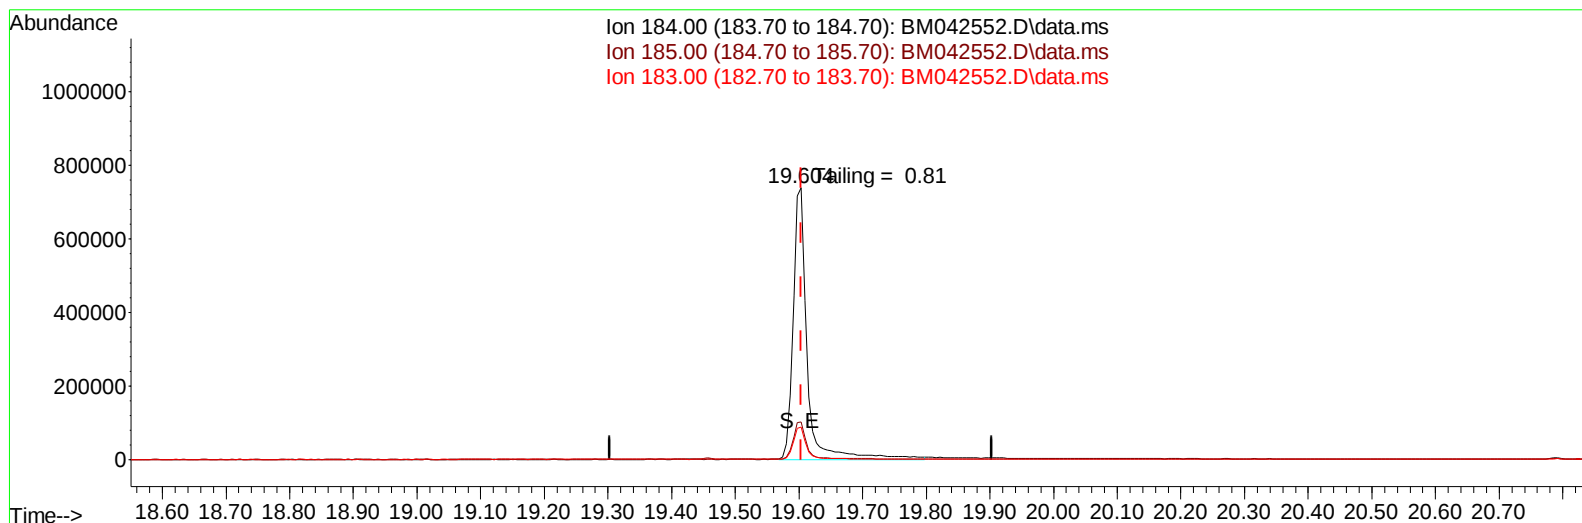

TIC: BM042552.D\data.ms

(77) Benzidine

19.604min (-0.000) 94164.56 ng

response 1150744

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.92
183.00	11.20	11.84
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/2/2023	BNA_M	<u>BM042552.D</u>
Compound Name	Response	Retention Time
DDT	681631	20.786
DDD	13863	20.392
DDE	0	19.833
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13863	695494	1.99

Instrument :
BNA_M
ClientSampleId :
DFTPP