
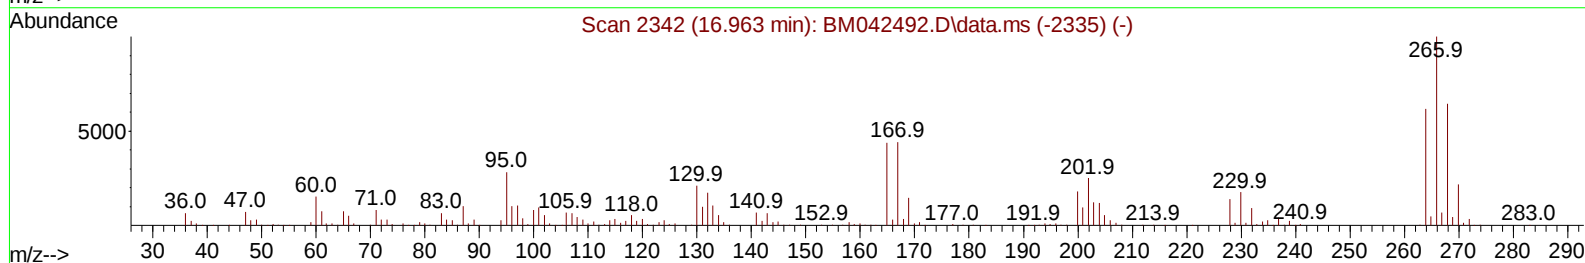
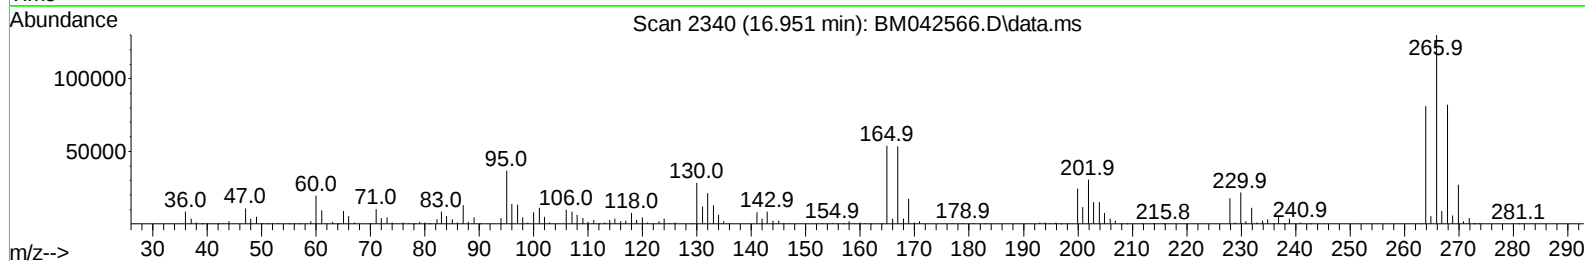


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110323\
Data File : BM042566.D
Acq On : 03 Nov 2023 12:16
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 20:30:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 03 15:52:20 2023
Response via : Initial Calibration

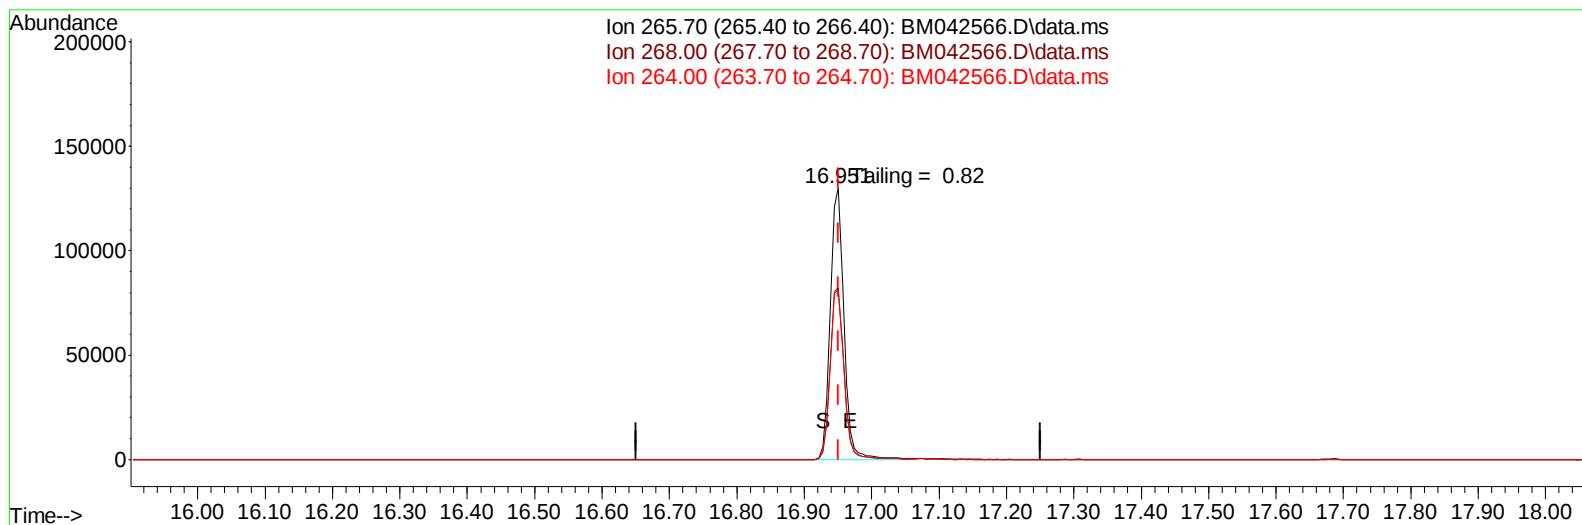




TIC: BM042566.D\data.ms

(70) Pentachlorophenol (C)**16.951min (-0.000) 45158.86 ng****response 182897**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	63.20
264.00	61.80	62.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110323\
Data File : BM042566.D
Acq On : 03 Nov 2023 12:16
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 03 20:30:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 03 15:52:20 2023
Response via : Initial Calibration

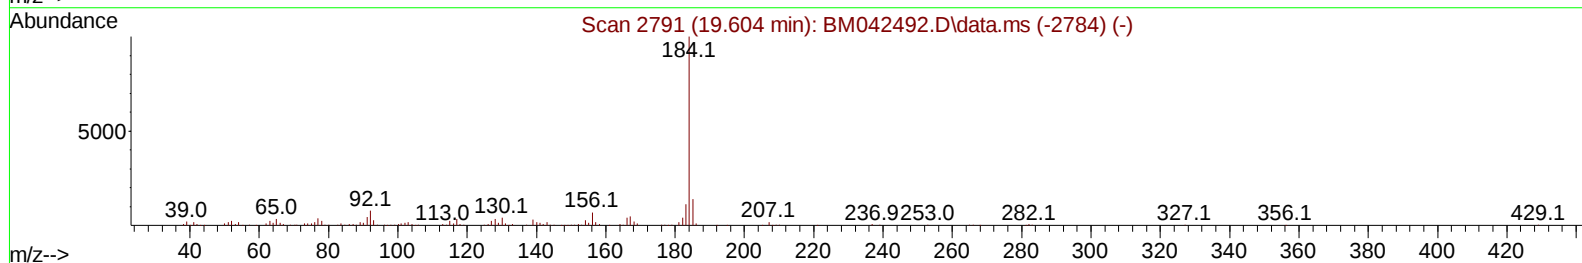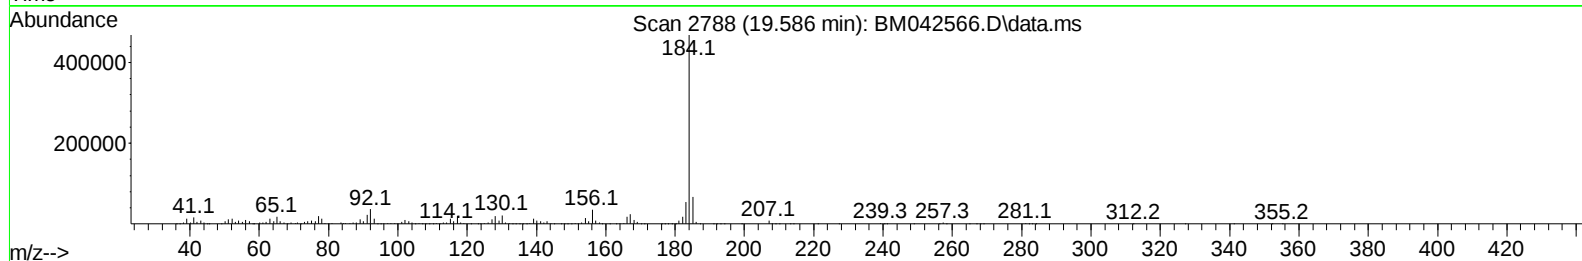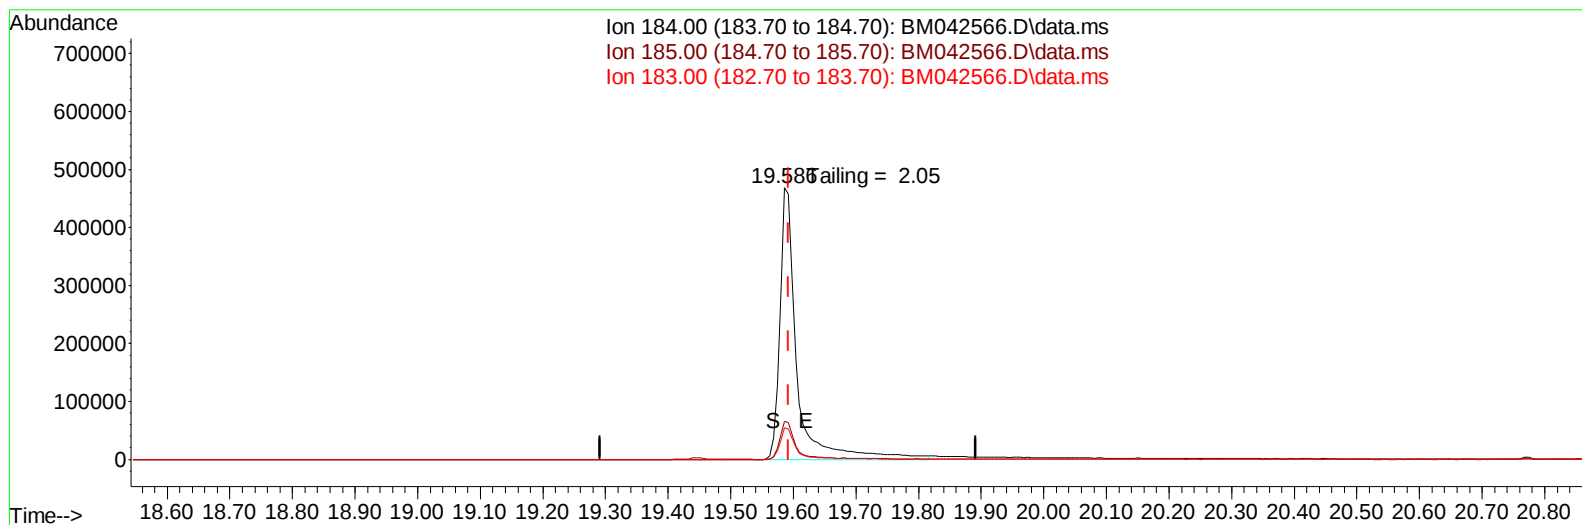

TIC: BM042566.D\data.ms

(77) Benzidine**19.586min (-0.006) 73980.28 ng****response 905500**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.17
183.00	11.20	11.65
0.00	0.00	0.00