
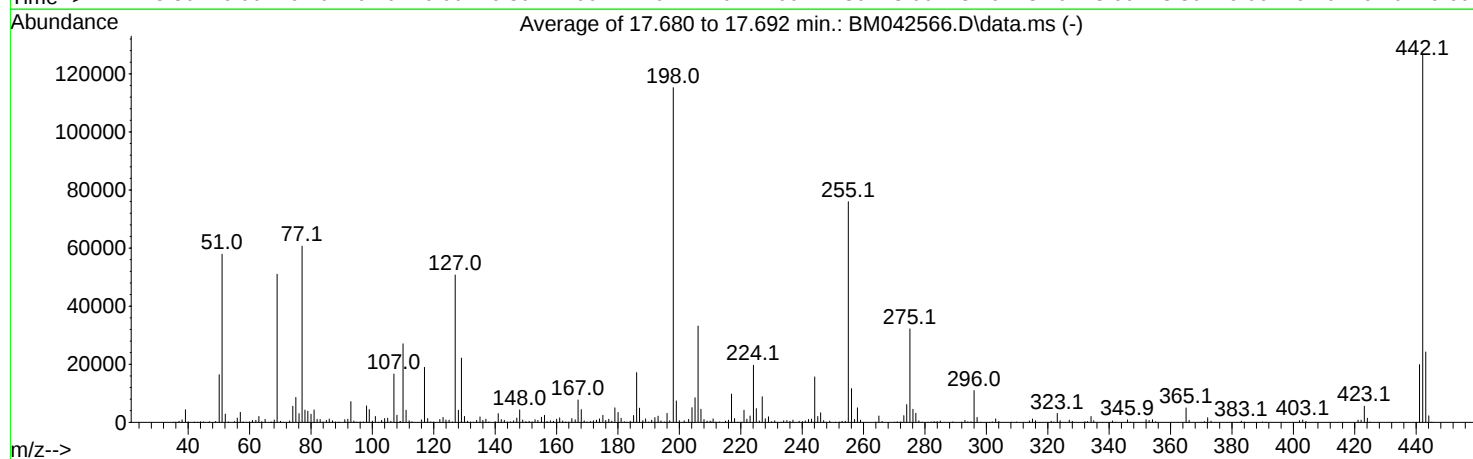


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110323\
 Data File : BM042566.D
 Acq On : 03 Nov 2023 12:16
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 03 15:52:20 2023

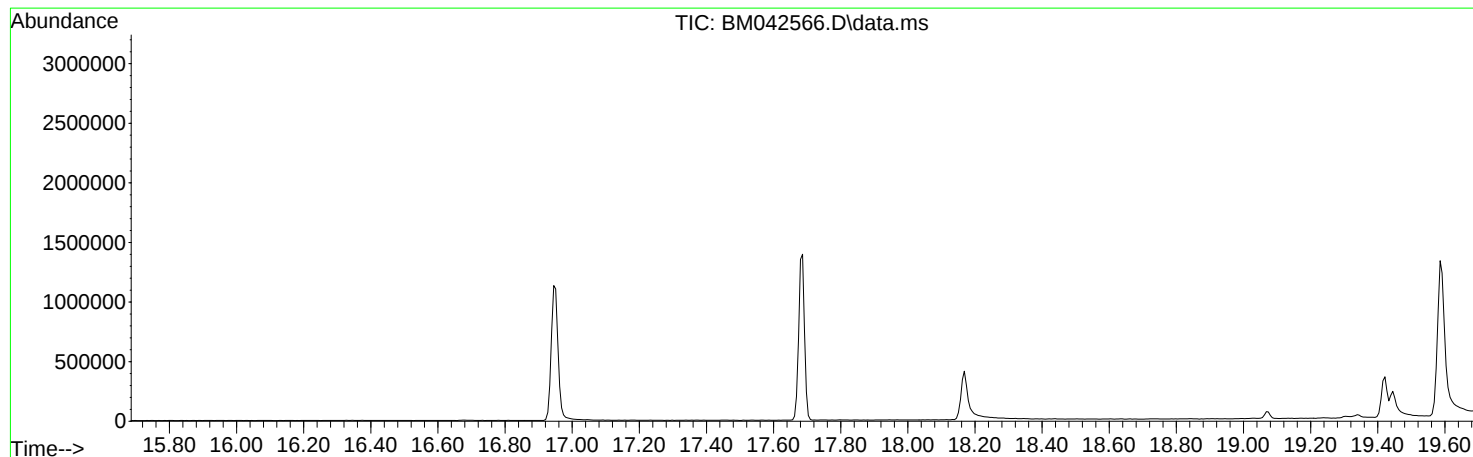




AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.2	57888	PASS
68	69	0.00	2	1.7	848	PASS
69	198	0.00	100	44.3	51045	PASS
70	69	0.00	2	0.8	411	PASS
127	198	10	80	44.0	50741	PASS
197	198	0.00	2	0.5	555	PASS
198	198	100	100	100.0	115227	PASS
199	198	5	9	6.4	7368	PASS
275	198	10	60	27.9	32152	PASS
365	198	1	100	4.3	4978	PASS
441	198	0.01	100	17.3	19917	PASS
442	442	50	100	100.0	126651	PASS
443	442	15	24	19.1	24224	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110323\
Data File : BM042566.D
Acq On : 03 Nov 2023 12:16
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 03 20:30:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 03 15:52:20 2023
Response via : Initial Calibration

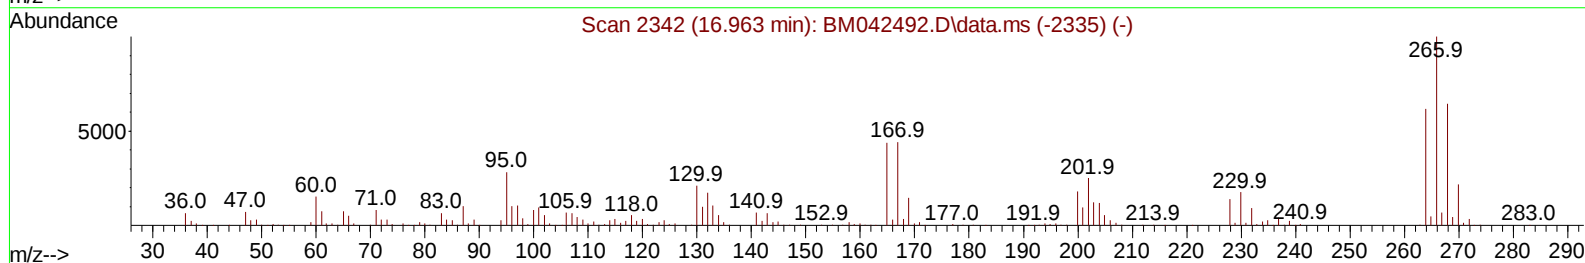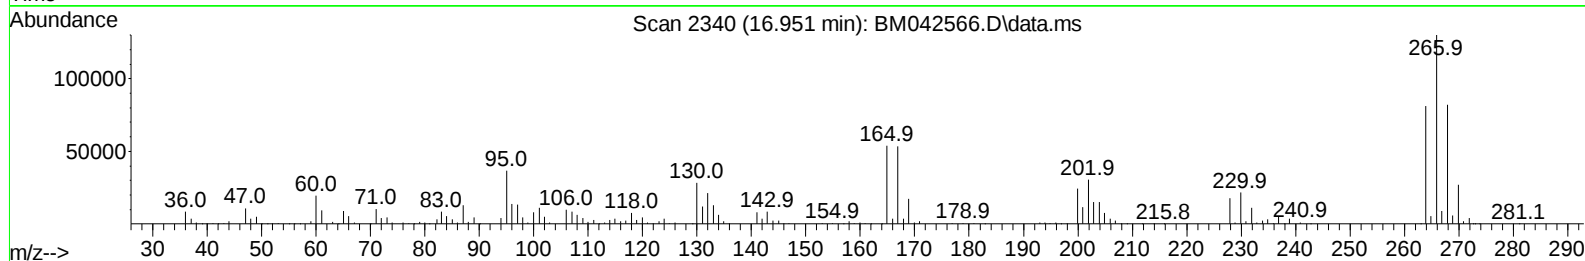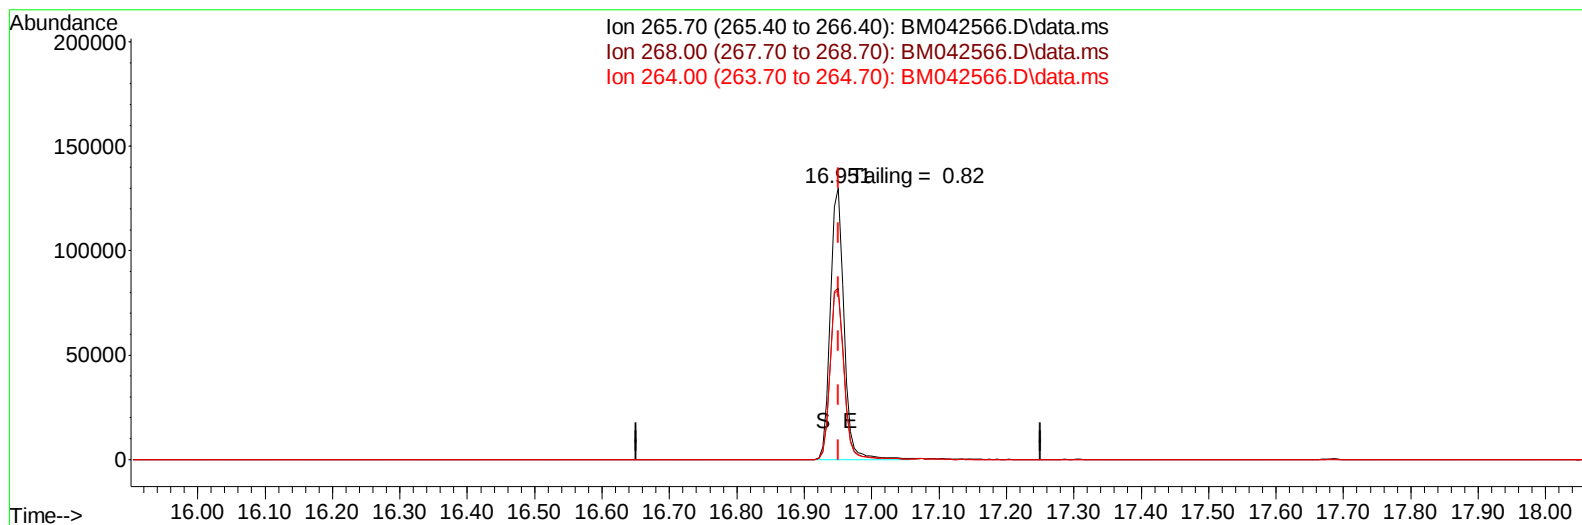

TIC: BM042566.D\data.ms

(70) Pentachlorophenol (C)

16.951min (-0.000) 45158.86 ng




response 182897

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	63.20
264.00	61.80	62.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110323\
Data File : BM042566.D
Acq On : 03 Nov 2023 12:16
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 03 20:30:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 03 15:52:20 2023
Response via : Initial Calibration

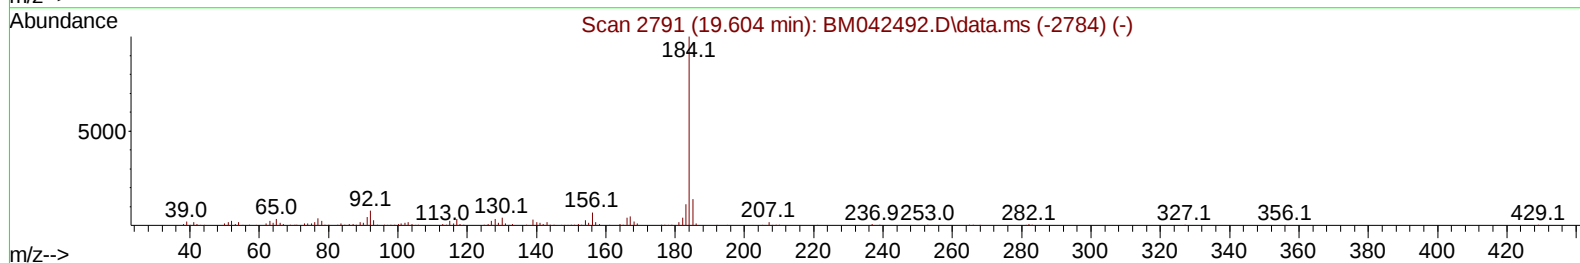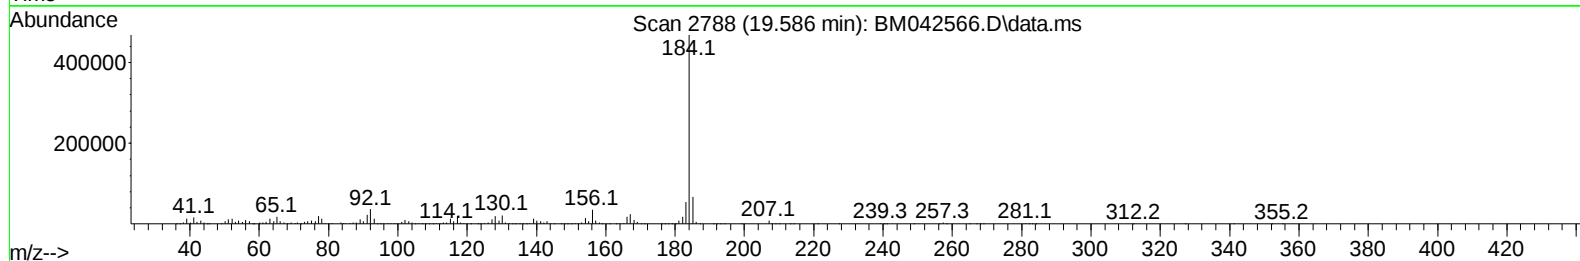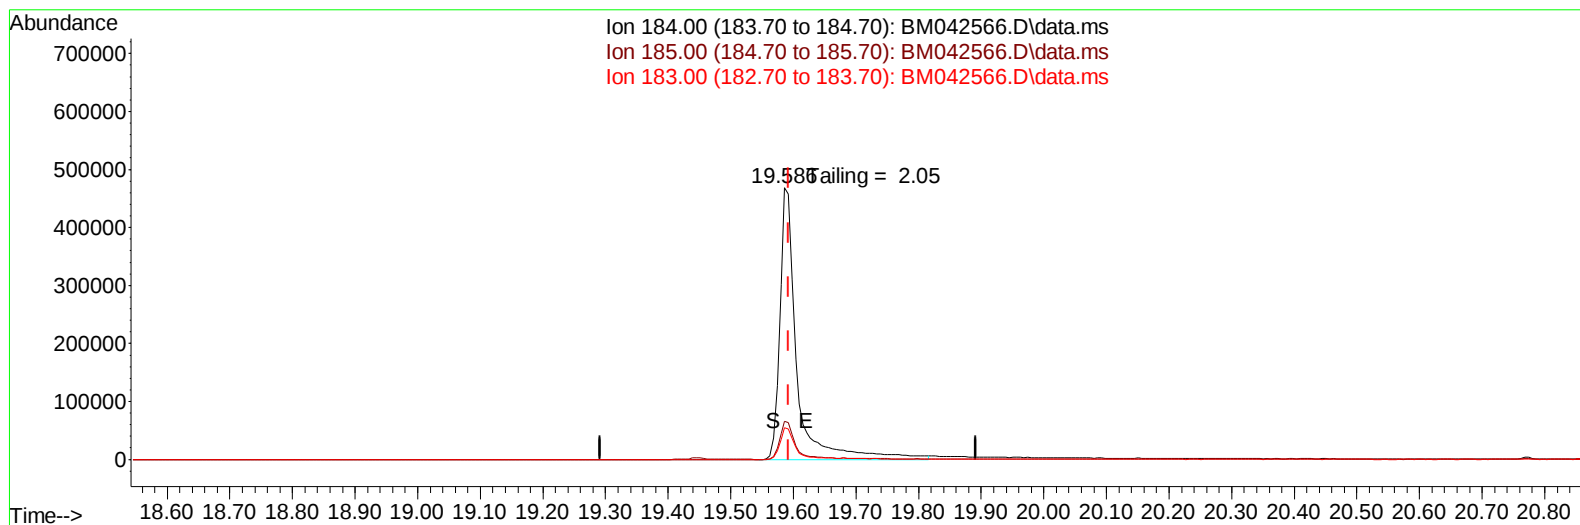

TIC: BM042566.D\data.ms

(77) Benzidine

19.586min (-0.006) 73980.28 ng

response 905500

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.17
183.00	11.20	11.65
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/3/2023	BNA_M	<u>BM042566.D</u>
Compound Name	Response	Retention Time
DDT	608762	20.774
DDD	9466	20.38
DDE	77	19.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9543	618305	1.54

Instrument :
BNA_M
ClientSampleId :
DFTPP