

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110419\
 Data File : BM023580.D
 Acq On : 04 Nov 2019 14:37
 Operator : JU
 Sample : K5511-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEJN1

Quant Time: Nov 04 15:24:18 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 04 01:07:42 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	312163	20.00	ng/ul	0.00
18) Naphthalene-d8	10.38	136	1271668	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.25	164	784290	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.00	188	1787272	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	1898143	20.00	ng/ul	0.00
86) Perylene-d12	23.39	264	2234237	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.15	96	45212	6.88	ng/uL	0.00
5) Phenol-d5	6.79	99	207951	7.93	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	521481	33.94	ng/ul	0.00
9) 2-Chlorophenol-d4	7.14	132	564280	27.53	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	370053	17.38	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	338325	35.34	ng/ul	0.00
22) 2-Nitrophenol-d4	9.47	143	347939	32.76	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.01	165	638107	30.57	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	52602	2.19	ng/ul	0.00
44) Dimethylphthalate-d6	13.67	166	2292952	38.50	ng/ul	0.00
47) Acenaphthylene-d8	13.94	160	2577641	37.78	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	65117	6.31	ng/ul	0.00
58) Fluorene-d10	15.25	176	2012552	39.90	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.38	200	295886	26.59	ng/ul	0.00
71) Anthracene-d10	17.10	188	3424225	40.54	ng/ul	0.00
79) Pyrene-d10	19.40	212	3940121	37.74	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.24	264	4817991	42.33	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.72	163	101465	1.697	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110419\
Data File : BM023580.D
Acq On : 04 Nov 2019 14:37
Operator : JU
Sample : K5511-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEJN1

Quant Time: Nov 04 15:24:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 04 01:07:42 2019
Response via : Initial Calibration

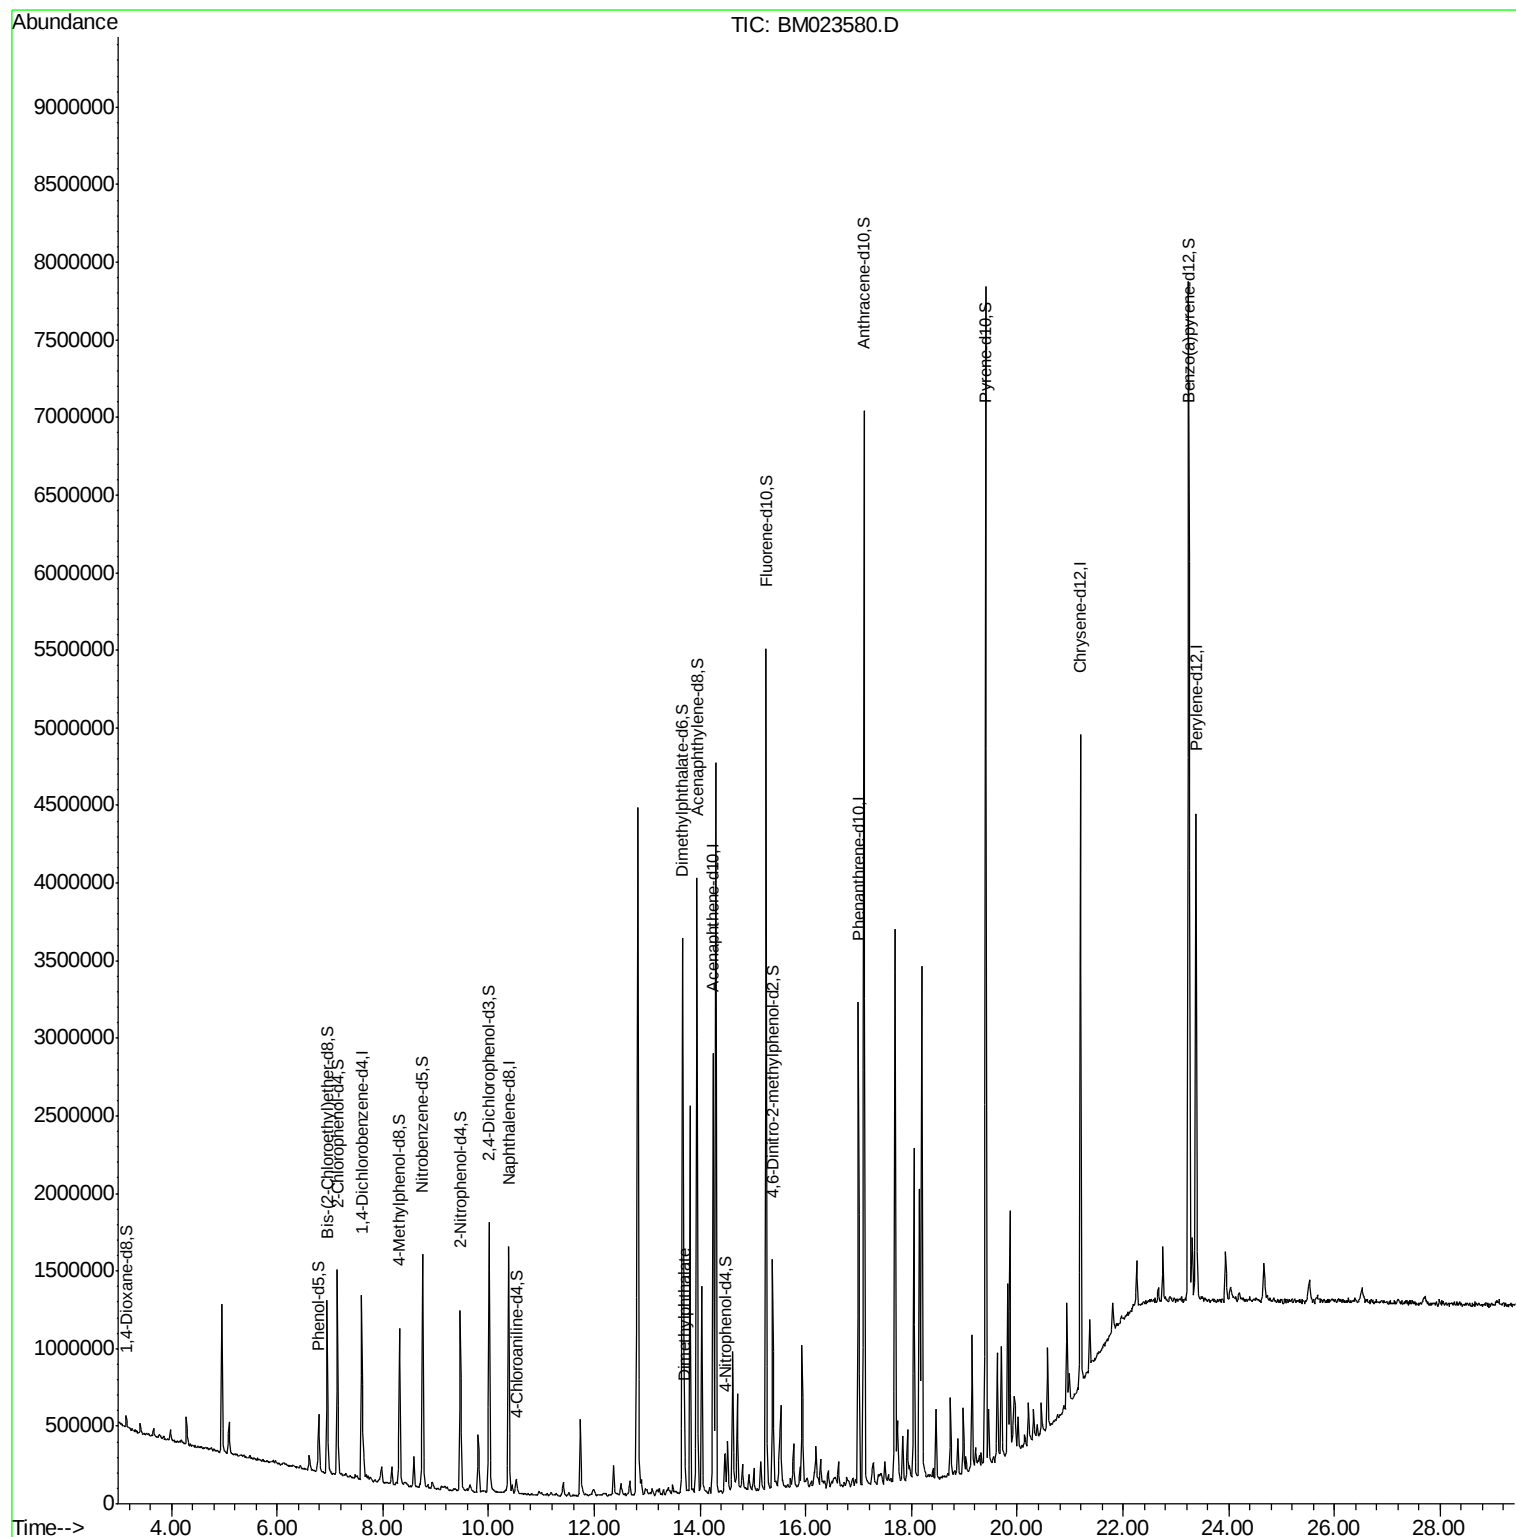

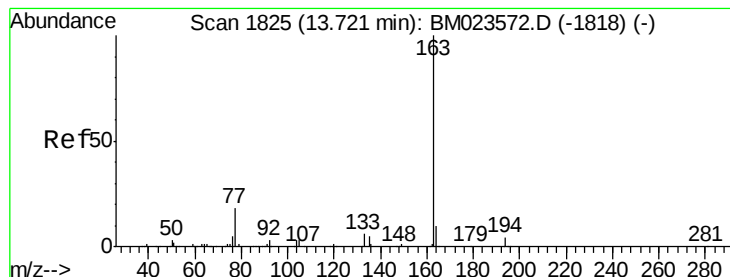

#45
 Dimethylphthalate
 Concen: 1.697 ng/ul
 RT: 13.72 min Scan# 1824
 Delta R.T. -0.01 min
 Lab File: BM023580.D
 Acq: 04 Nov 2019 14:37

Instrument :
 BNA_M
 ClientSampleId :
 BEJN1

Tot Ion:	163	Resp:	101465
Ion	Ratio	Lower	Upper
163	100		
194	3.9	3.3	4.9
164	10.2	7.9	11.9

