

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110419\
 Data File : BM023581.D
 Acq On : 04 Nov 2019 15:12
 Operator : JU
 Sample : K5511-15
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEJN2

Quant Time: Nov 04 15:46:37 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 04 01:07:42 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	327786	20.00	ng/ul	0.00
18) Naphthalene-d8	10.38	136	1343826	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.25	164	829965	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.00	188	1837542	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	1868518	20.00	ng/ul	0.00
86) Perylene-d12	23.39	264	2268351	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.15	96	42175	6.11	ng/uL	0.00
5) Phenol-d5	6.79	99	205086	7.45	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	511782	31.72	ng/ul	0.00
9) 2-Chlorophenol-d4	7.14	132	554215	25.75	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	373983	16.73	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	337519	33.36	ng/ul	0.00
22) 2-Nitrophenol-d4	9.47	143	349580	31.14	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.01	165	644085	29.20	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	44329	1.75	ng/ul	0.00
44) Dimethylphthalate-d6	13.67	166	2401290	38.10	ng/ul	0.00
47) Acenaphthylene-d8	13.94	160	2724286	37.73	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	60541	5.54	ng/ul	0.00
58) Fluorene-d10	15.25	176	2054418	38.49	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.38	200	289754	25.33	ng/ul	0.00
71) Anthracene-d10	17.10	188	3386629	39.00	ng/ul	0.00
79) Pyrene-d10	19.40	212	3891121	37.87	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.24	264	4704019	40.71	ng/ul	-0.01
Target Compounds						
45) Dimethylphthalate	13.72	163	228648	3.613	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110419\
Data File : BM023581.D
Acq On : 04 Nov 2019 15:12
Operator : JU
Sample : K5511-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEJN2

Quant Time: Nov 04 15:46:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 04 01:07:42 2019
Response via : Initial Calibration

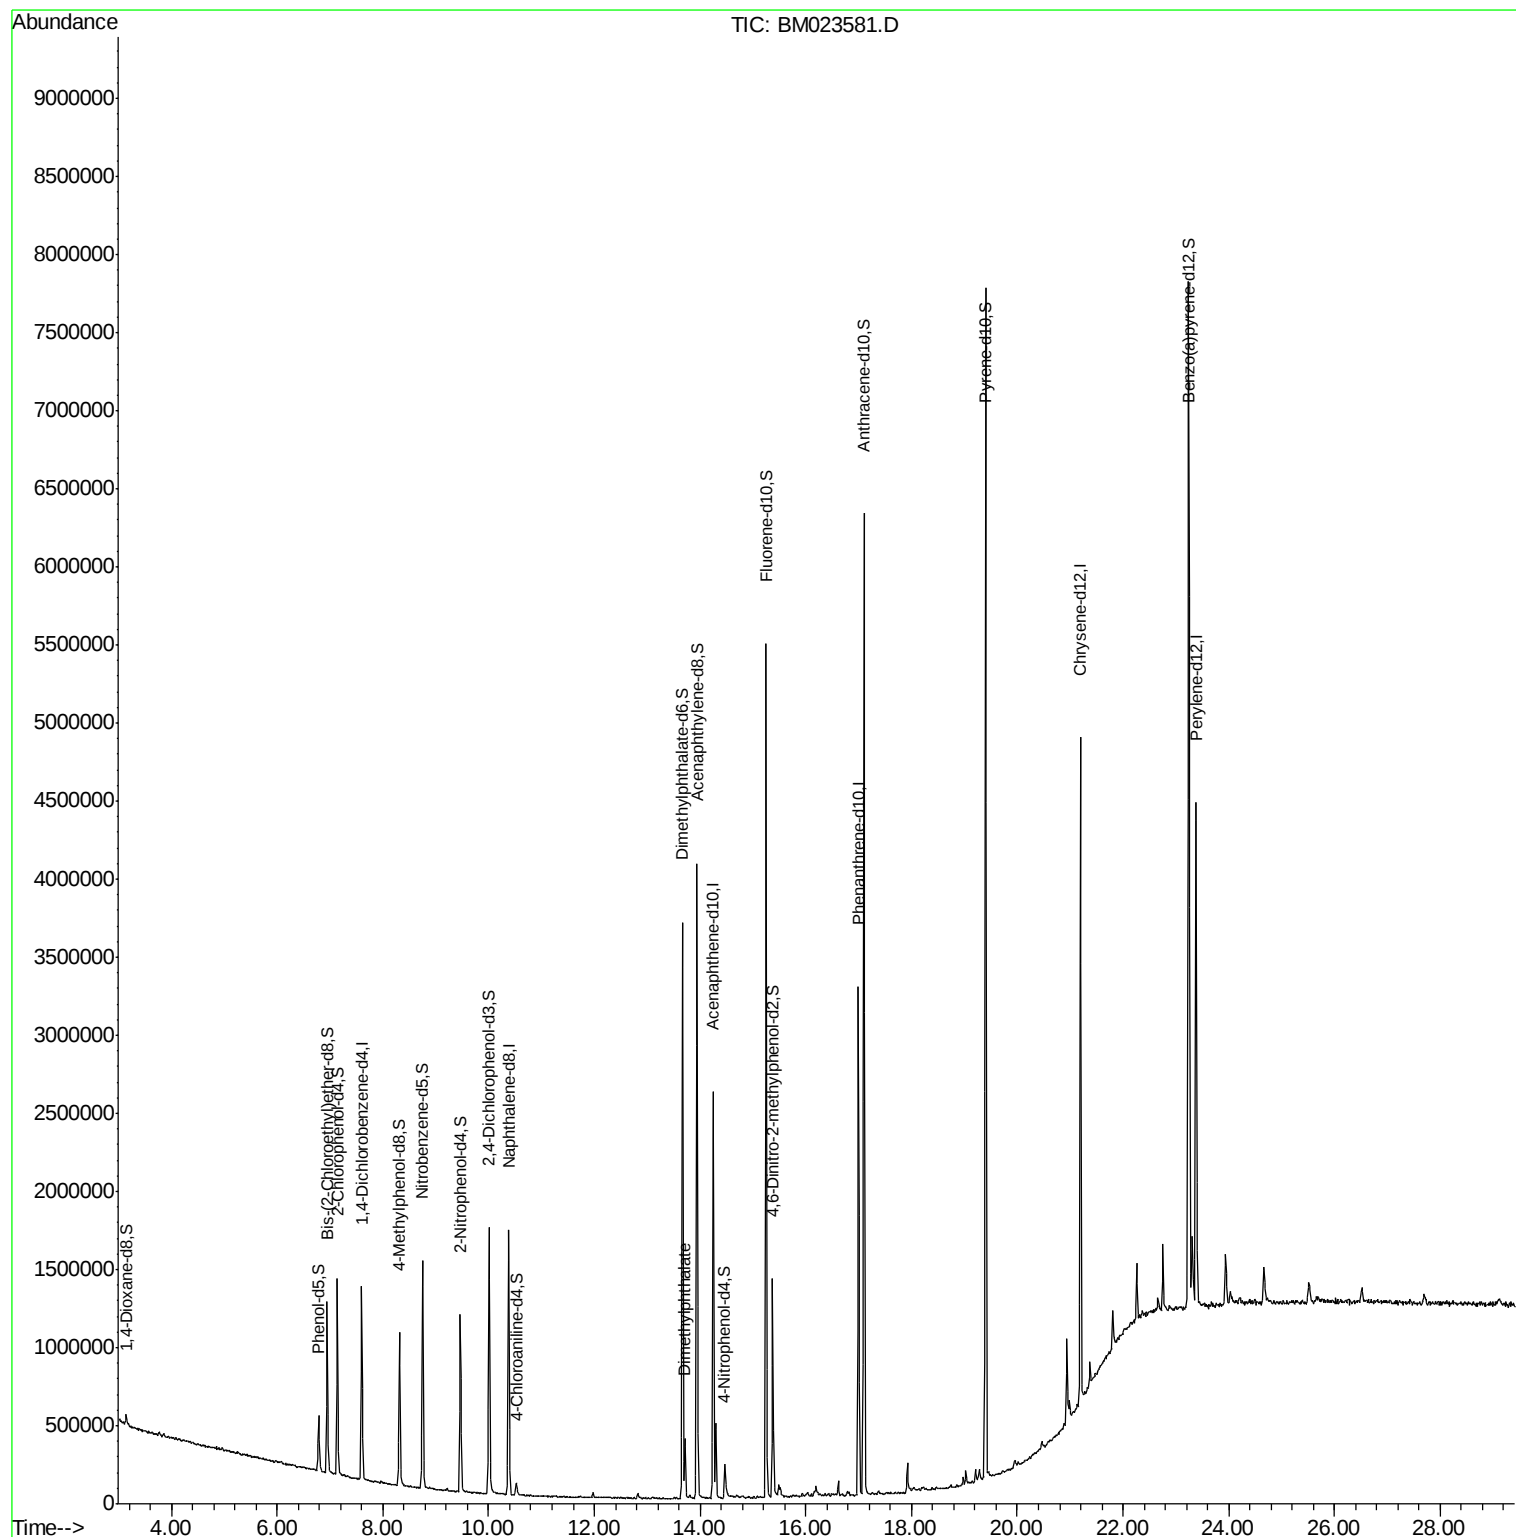

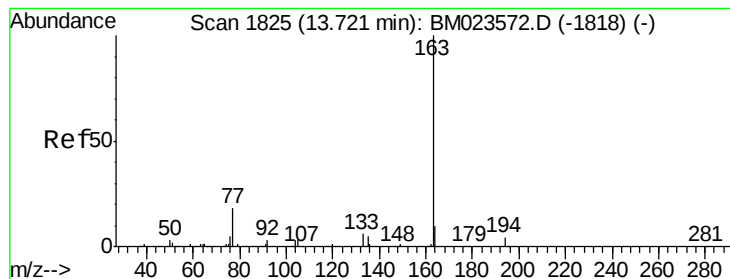

#45

Dimethylphthalate

Concen: 3.613 ng/ul

RT: 13.72 min Scan# 1824

Delta R.T. -0.01 min

Lab File: BM023581.D

Acq: 04 Nov 2019 15:12

Instrument :

BNA_M

ClientSampleId :

BEJN2



Tot Ion:163 Resp: 228648

Ion Ratio Lower Upper

163 100

194 4.1 3.3 4.9

164 9.9 7.9 11.9

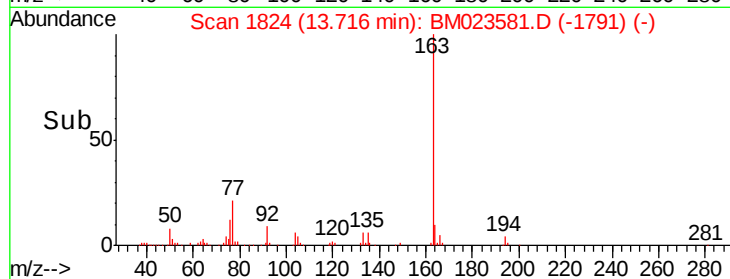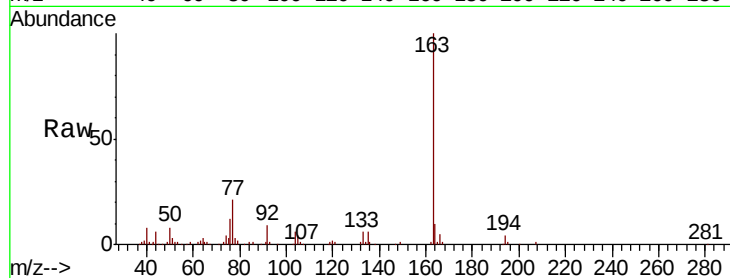

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

