

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110419\
 Data File : BM023585.D
 Acq On : 04 Nov 2019 18:11
 Operator : JU
 Sample : K5511-17
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEJN4

Quant Time: Nov 05 03:18:23 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 05 03:15:52 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	296244	20.00	ng/ul	0.00
18) Naphthalene-d8	10.38	136	1190236	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.25	164	729811	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.00	188	1567234	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	1569868	20.00	ng/ul	0.00
86) Perylene-d12	23.39	264	1917559	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.15	96	42712	6.85	ng/uL	0.00
5) Phenol-d5	6.79	99	206049	8.28	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	527453	36.17	ng/ul	0.00
9) 2-Chlorophenol-d4	7.14	132	560369	28.81	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	351310	17.38	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	335564	37.45	ng/ul	0.00
22) 2-Nitrophenol-d4	9.47	143	346501	34.85	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.01	165	596227	30.52	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	50744	2.26	ng/ul	0.01
44) Dimethylphthalate-d6	13.67	166	2155883	38.90	ng/ul	0.00
47) Acenaphthylene-d8	13.94	160	2499407	39.37	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	51575	5.37	ng/ul	0.00
58) Fluorene-d10	15.25	176	1925894	41.03	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.37	200	263116	26.97	ng/ul	0.00
71) Anthracene-d10	17.10	188	3297765	44.53	ng/ul	0.00
79) Pyrene-d10	19.40	212	3720780	43.10	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.25	264	4448726	45.54	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.72	163	177334	3.187	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110419\
Data File : BM023585.D
Acq On : 04 Nov 2019 18:11
Operator : JU
Sample : K5511-17
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEJN4

Quant Time: Nov 05 03:18:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 05 03:15:52 2019
Response via : Initial Calibration

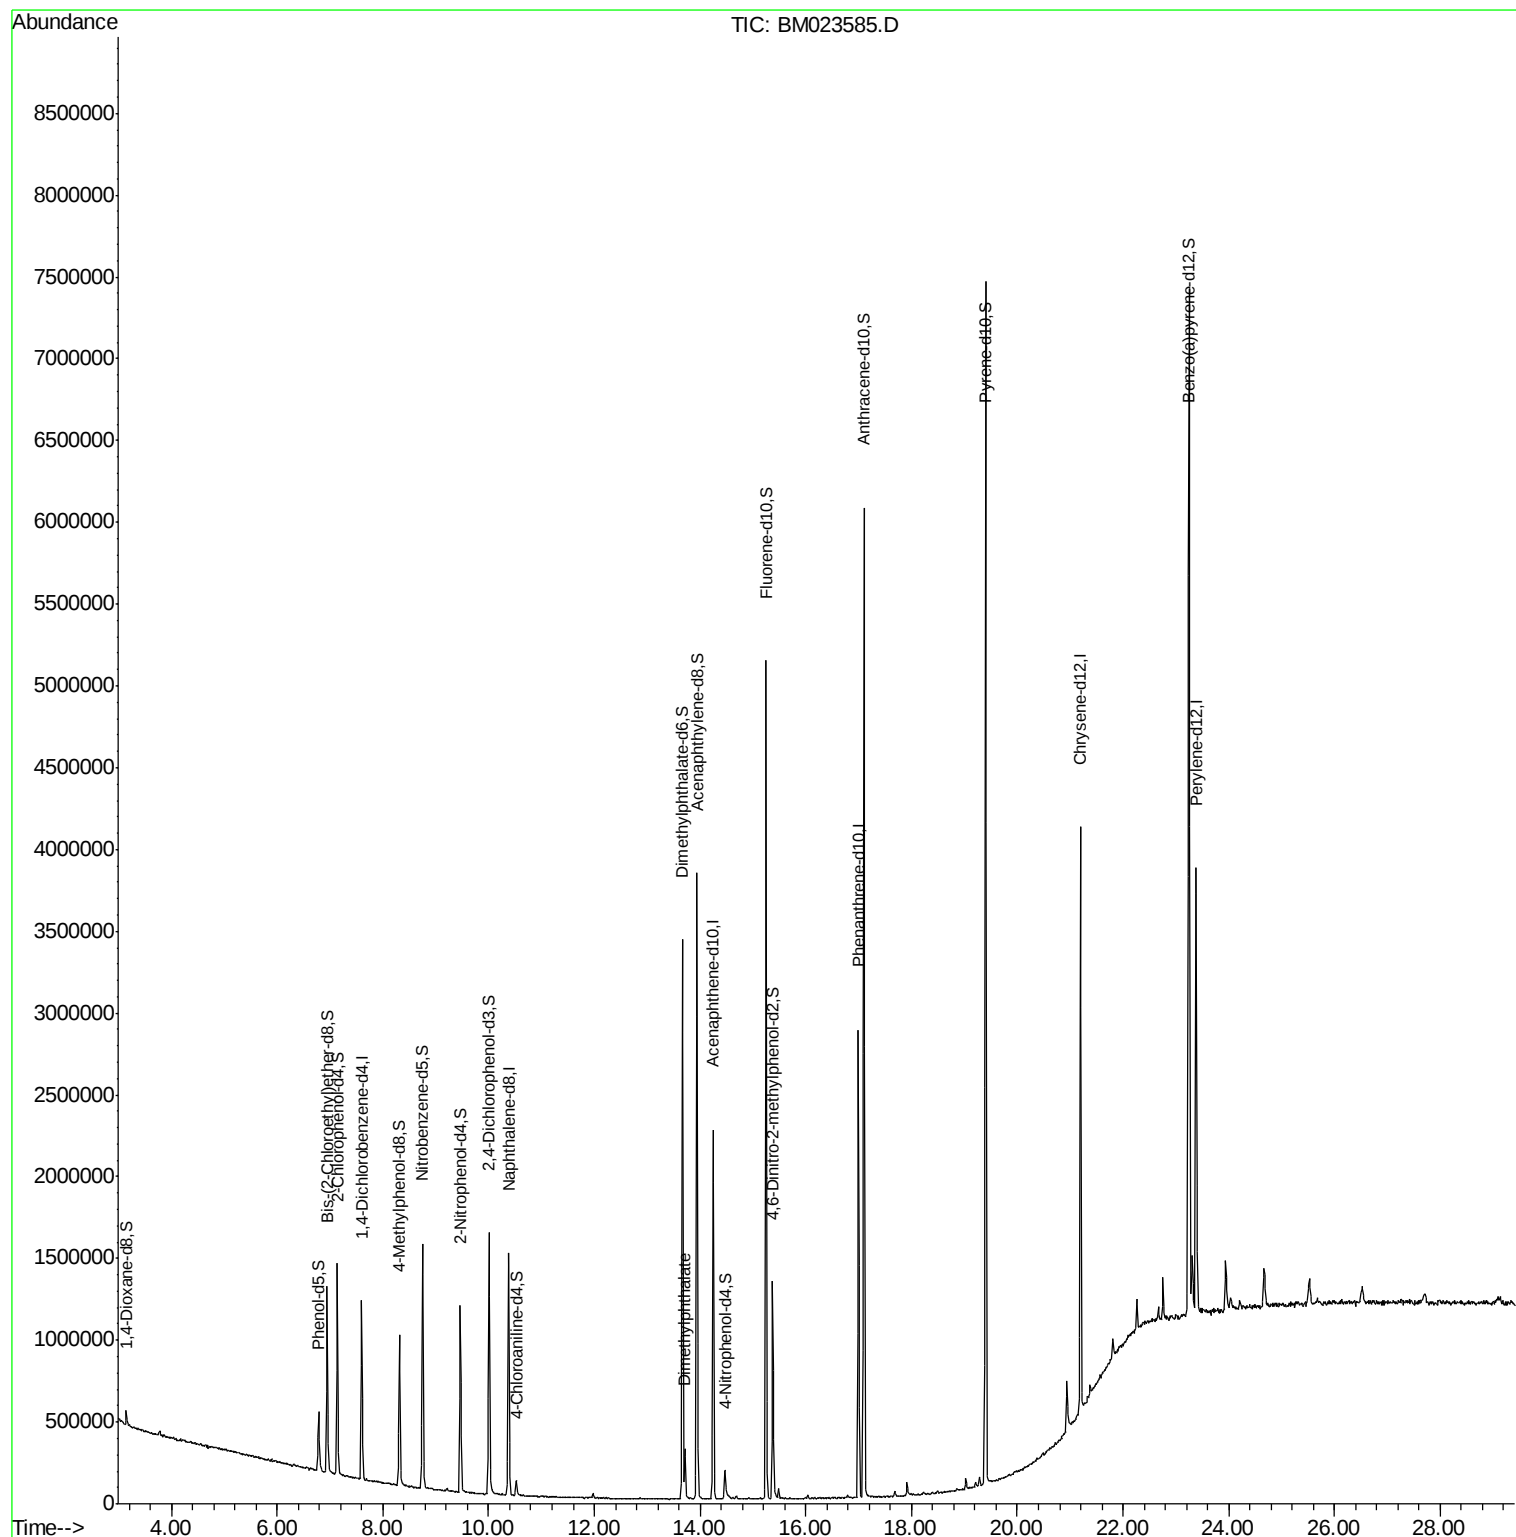


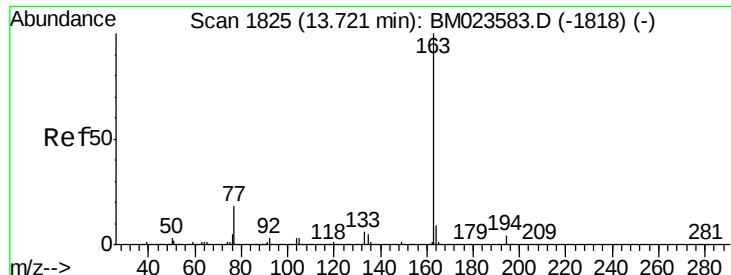

#45
 Dimethylphthalate
 Concen: 3.187 ng/ul
 RT: 13.72 min Scan# 1824
 Delta R.T. -0.01 min
 Lab File: BM023585.D
 Acq: 04 Nov 2019 18:11

Instrument :
 BNA_M
 ClientSampleId :
 BEJN4

Tot Ion	Ratio	Lower	Upper
163	100		
194	3.7	3.3	4.9
164	10.5	7.9	11.9

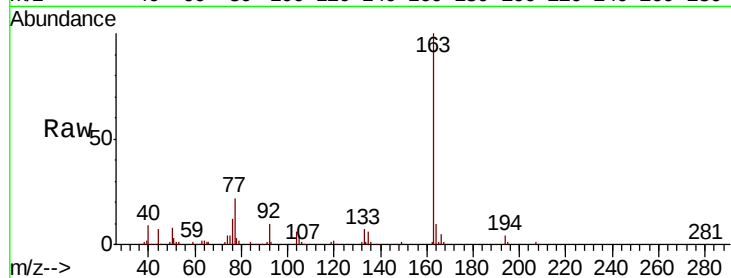

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

