
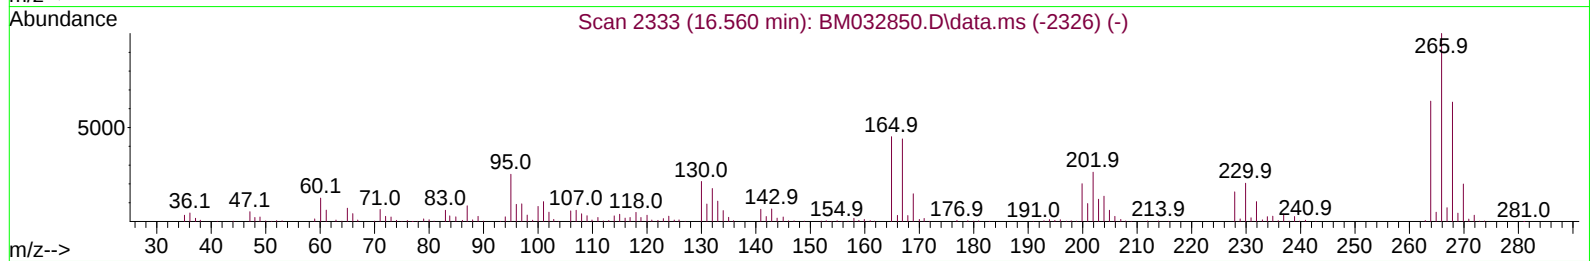
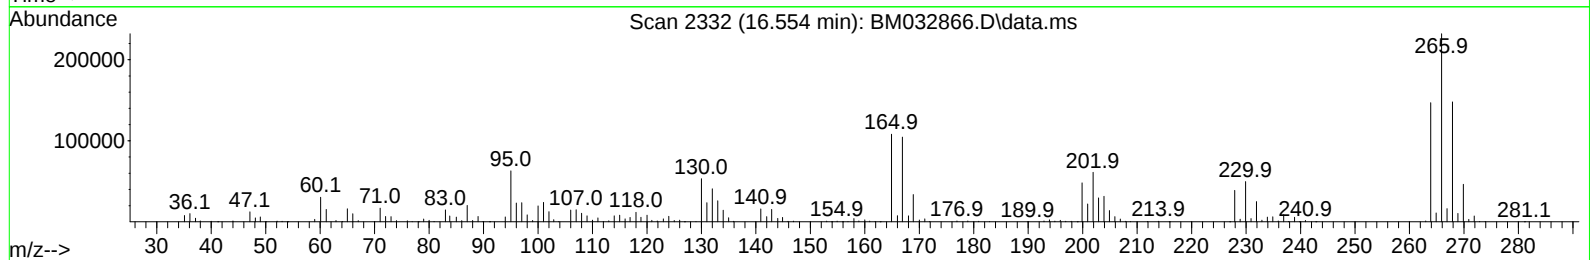


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110421\
Data File : BM032866.D
Acq On : 04 Nov 2021 09:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 14:59:28 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 02 16:07:18 2021
Response via : Initial Calibration

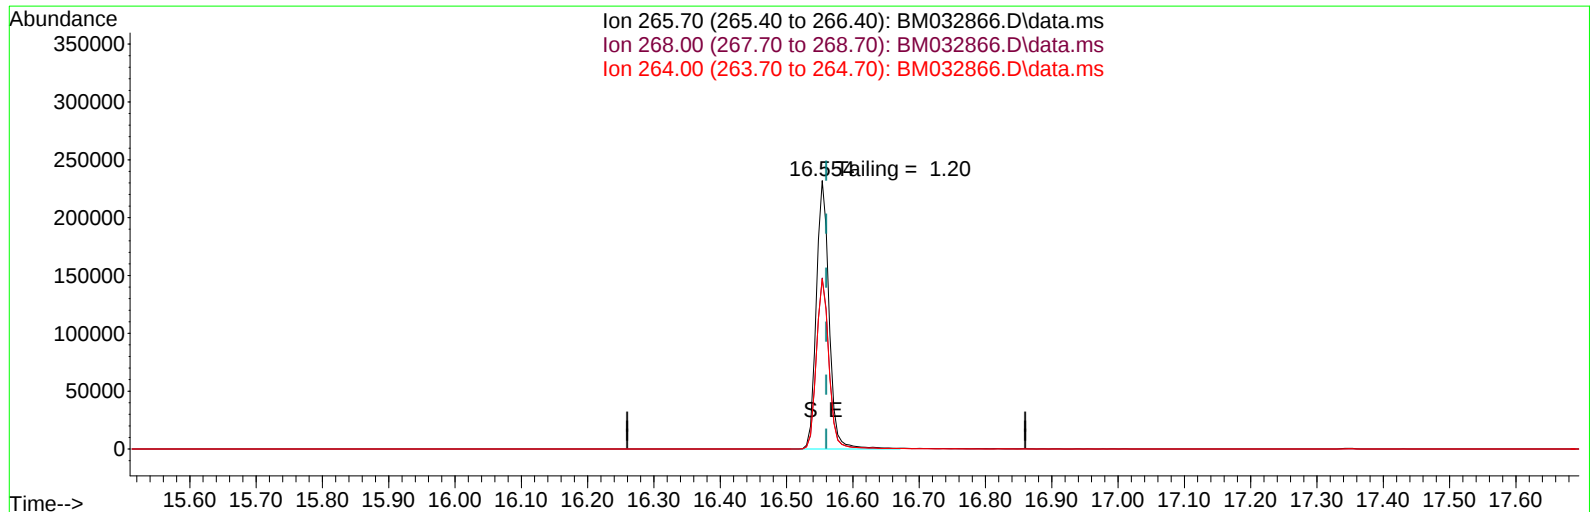

TIC: BM032866.D\data.ms

(70) Pentachlorophenol (C)




16.554min (-0.006) 0.00 ng

response 313931

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	63.75
264.00	65.10	63.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110421\
 Data File : BM032866.D
 Acq On : 04 Nov 2021 09:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 14:59:28 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 02 16:07:18 2021
 Response via : Initial Calibration

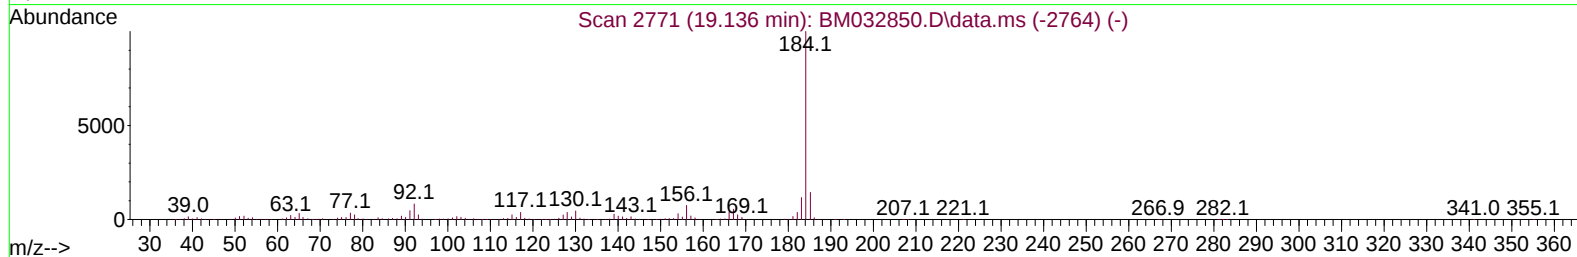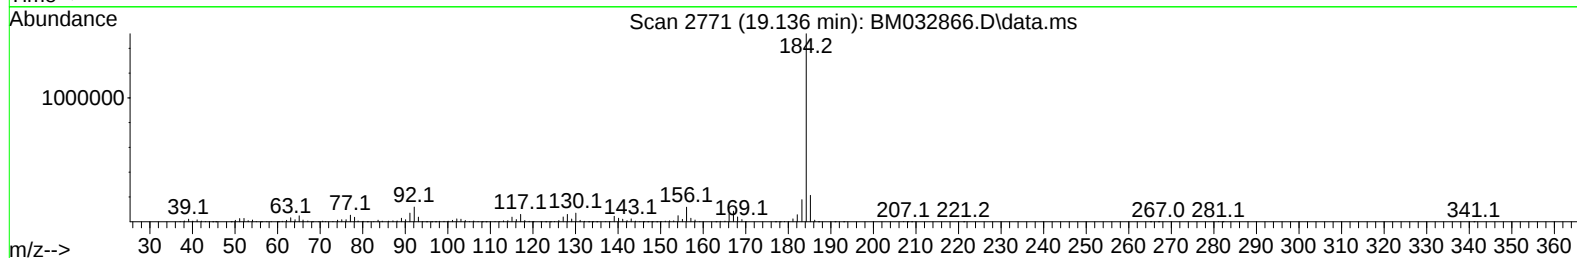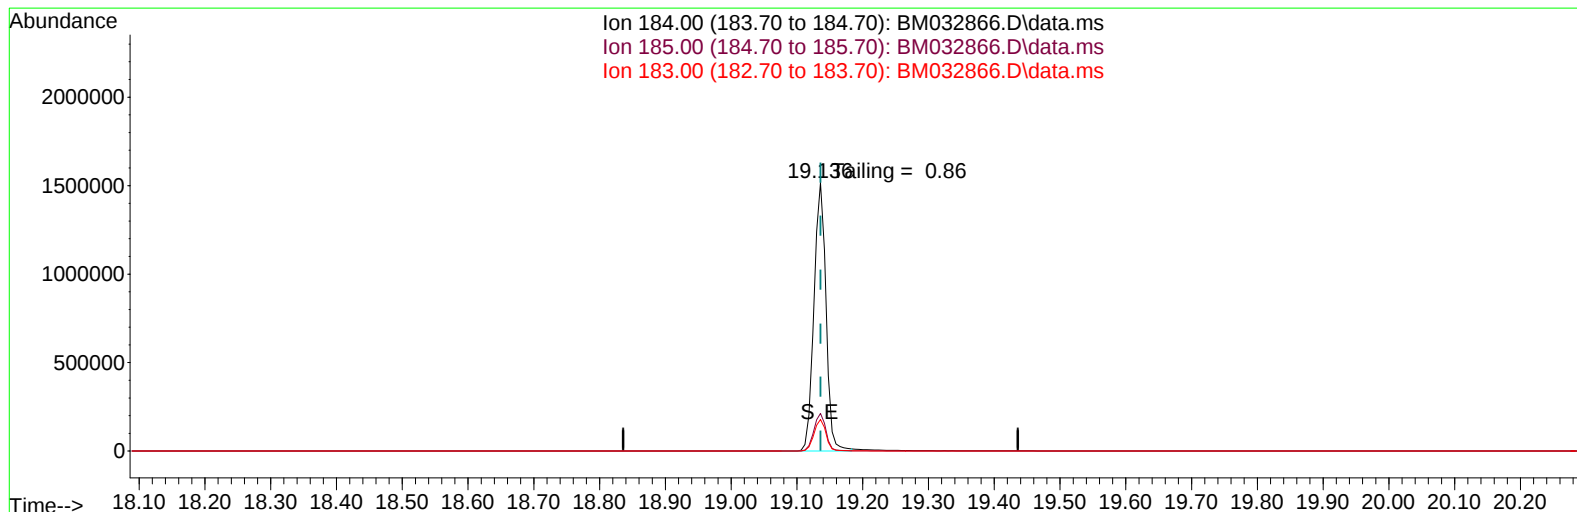

TIC: BM032866.D\data.ms

(77) Benzidine**19.136min (-0.000) 608796.38 ng****response 1952047**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	14.03
183.00	11.20	11.79
0.00	0.00	0.00