

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110421\
Data File : BM032868.D
Acq On : 04 Nov 2021 10:45
Operator : CG/JU
Sample : PB140471BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB140471BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM032868.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.078	375	381	398	rBV	2333668	3363622	45.25%	9.901%
2	6.695	648	656	668	rBV	2305256	3535267	47.56%	10.406%
3	7.490	784	791	804	rBV	391212	627146	8.44%	1.846%
4	8.642	980	987	1009	rBV	1410296	2230686	30.01%	6.566%
5	10.272	1257	1264	1282	rBV	558929	945236	12.72%	2.782%
6	12.760	1680	1687	1704	rBV	3457386	5259550	70.76%	15.481%
7	14.148	1917	1923	1934	rBV	983689	1369578	18.42%	4.031%
8	15.642	2171	2177	2193	rBV	2736803	3887791	52.30%	11.444%
9	16.883	2382	2388	2401	rBV	1174541	1660861	22.34%	4.889%
10	19.518	2830	2836	2848	rBV	5709101	7433457	100.00%	21.880%
11	21.065	3094	3099	3105	rBV	1532134	1835923	24.70%	5.404%
12	23.177	3453	3458	3467	rVB2	1056910	1824376	24.54%	5.370%




Sum of corrected areas: 33973493

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110421\
Data File : BM032868.D
Acq On : 04 Nov 2021 10:45
Operator : CG/JU
Sample : PB140471BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB140471BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

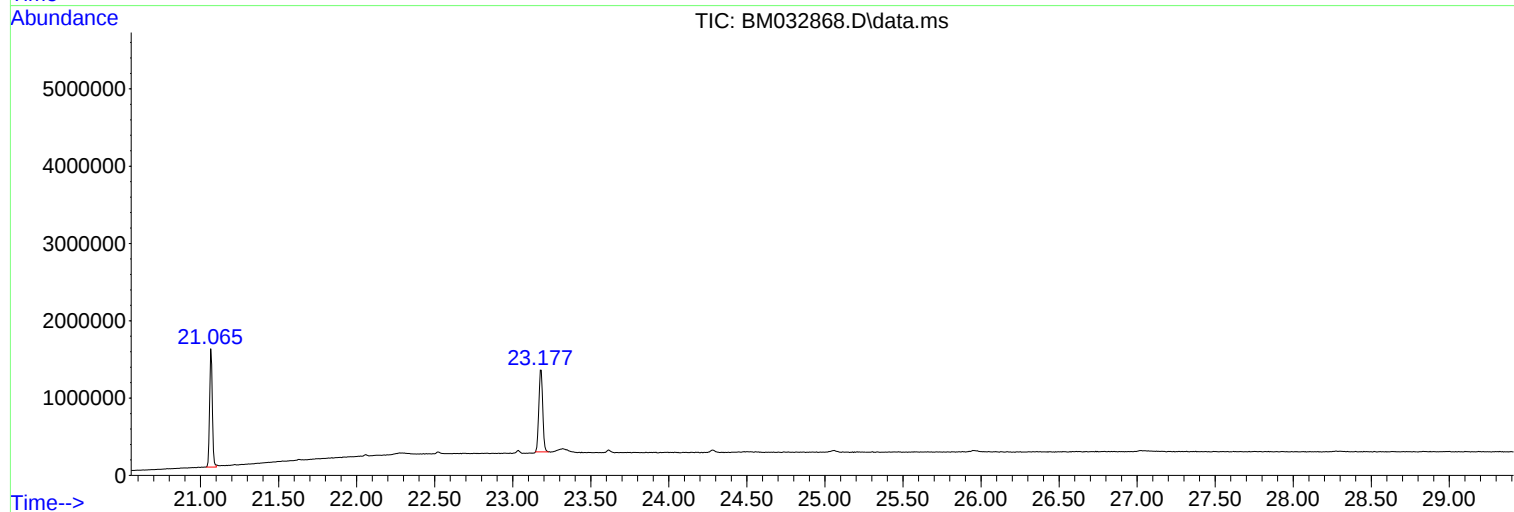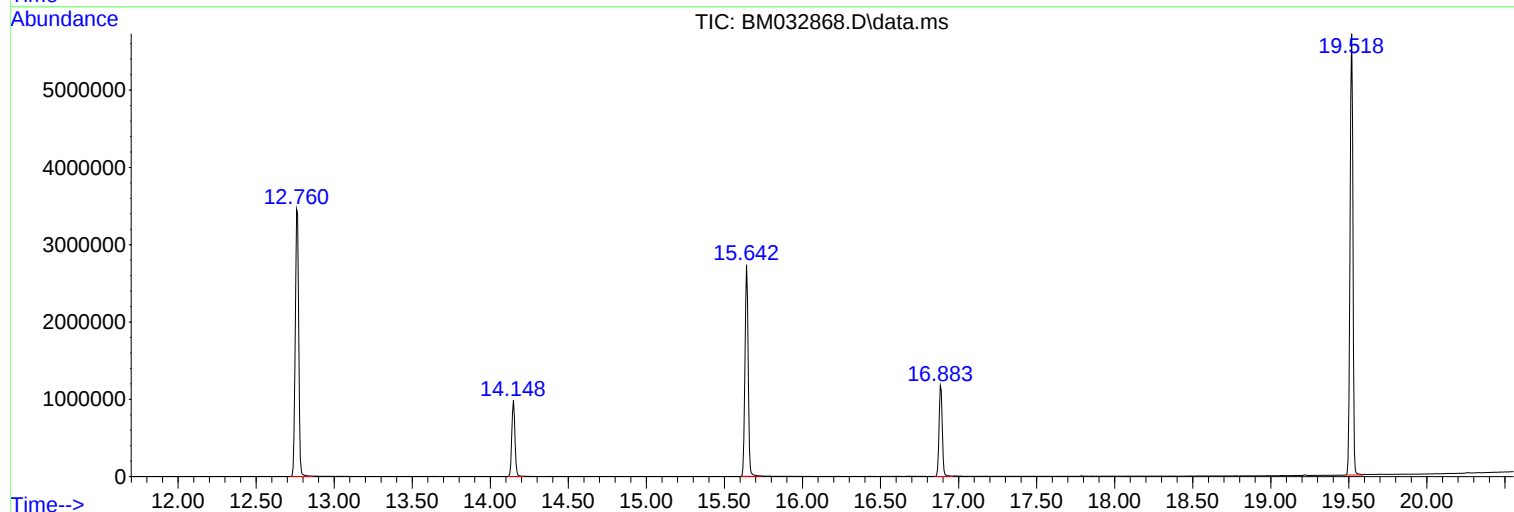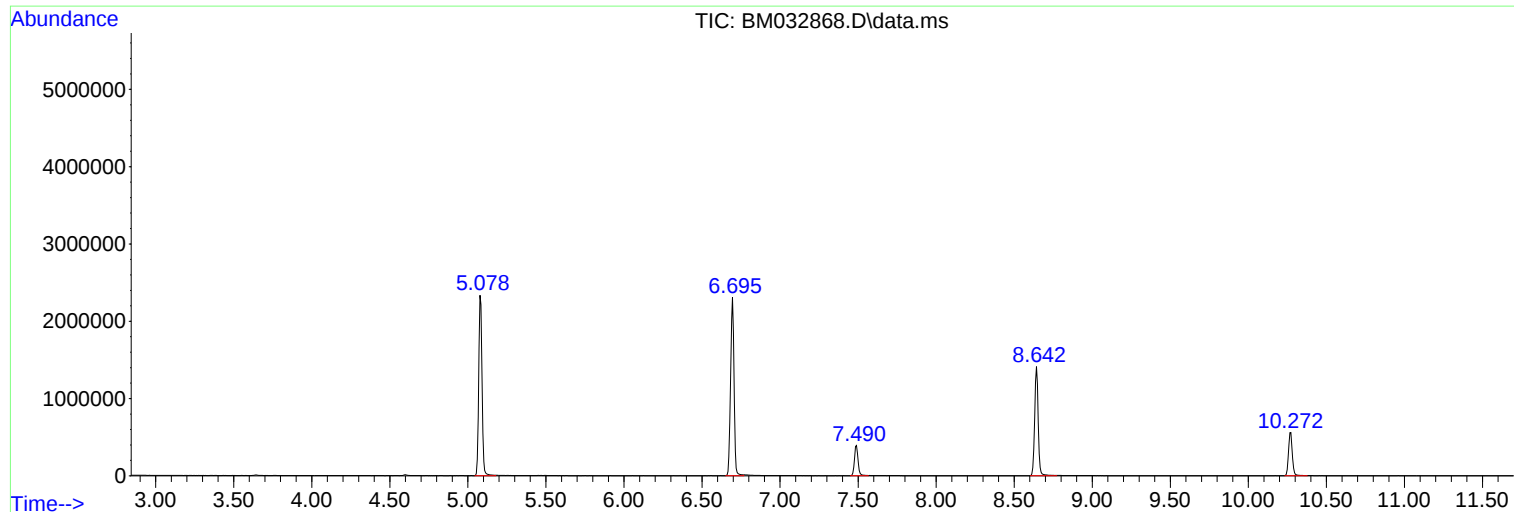

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110421\
Data File : BM032868.D
Acq On : 04 Nov 2021 10:45
Operator : CG/JU
Sample : PB140471BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB140471BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110421\
Data File : BM032868.D
Acq On : 04 Nov 2021 10:45
Operator : CG/JU
Sample : PB140471BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB140471BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------