
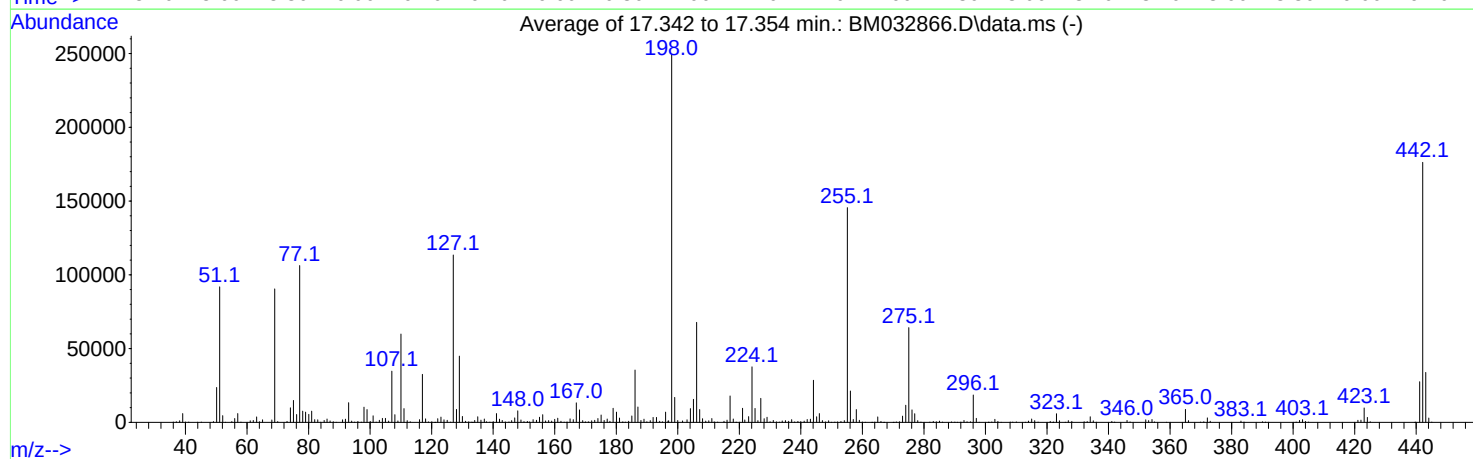


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110421\
 Data File : BM032866.D
 Acq On : 04 Nov 2021 09:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 02 16:07:18 2021

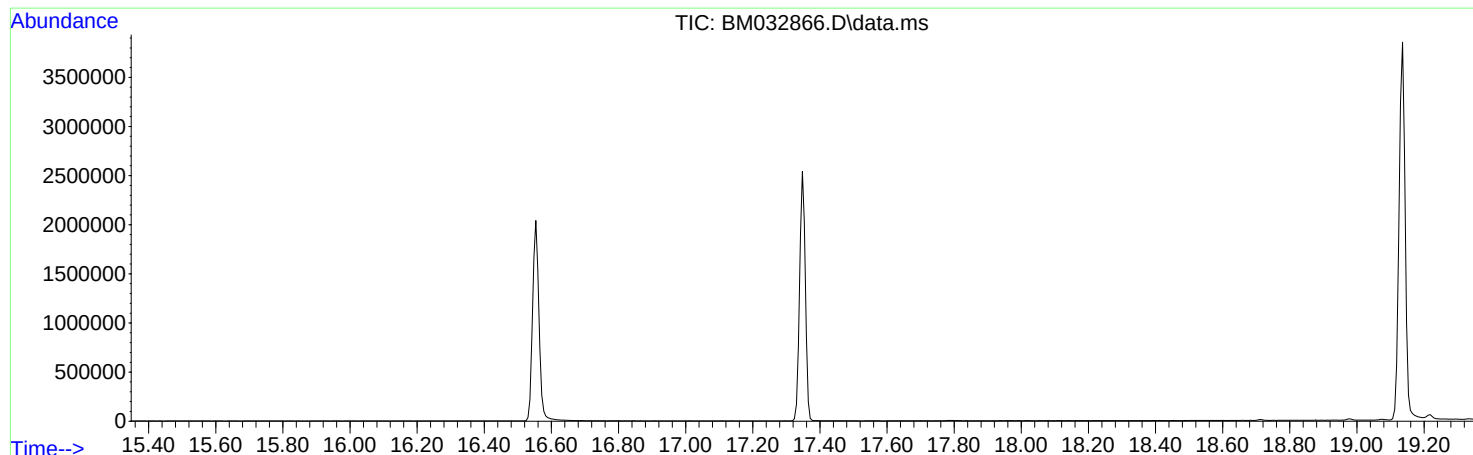




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	91883	PASS
68	69	0.00	2	1.8	1637	PASS
69	198	0.00	100	36.3	90485	PASS
70	69	0.00	2	0.6	550	PASS
127	198	10	80	45.5	113459	PASS
197	198	0.00	2	0.4	1075	PASS
198	198	100	100	100.0	249344	PASS
199	198	5	9	6.8	16977	PASS
275	198	10	60	25.8	64248	PASS
365	198	1	100	3.5	8820	PASS
441	198	0.01	100	11.1	27587	PASS
442	442	50	100	100.0	176269	PASS
443	442	15	24	19.2	33877	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110421\
 Data File : BM032866.D
 Acq On : 04 Nov 2021 09:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Nov 04 14:59:28 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 02 16:07:18 2021
 Response via : Initial Calibration

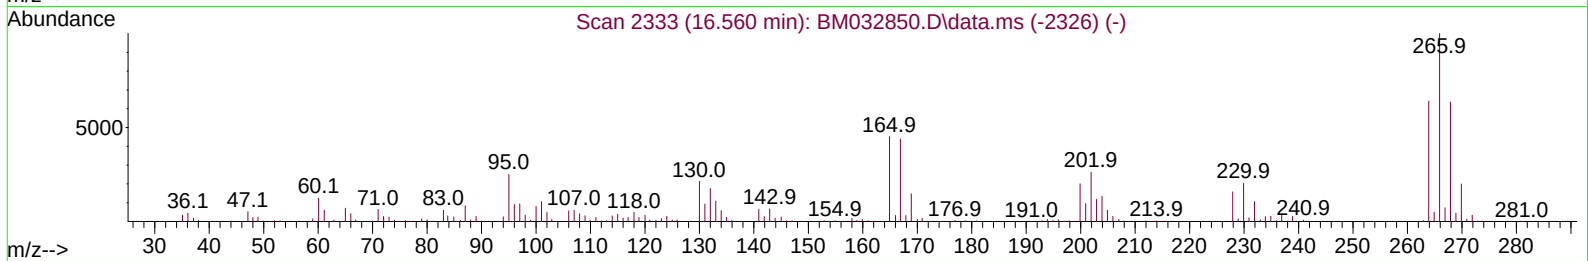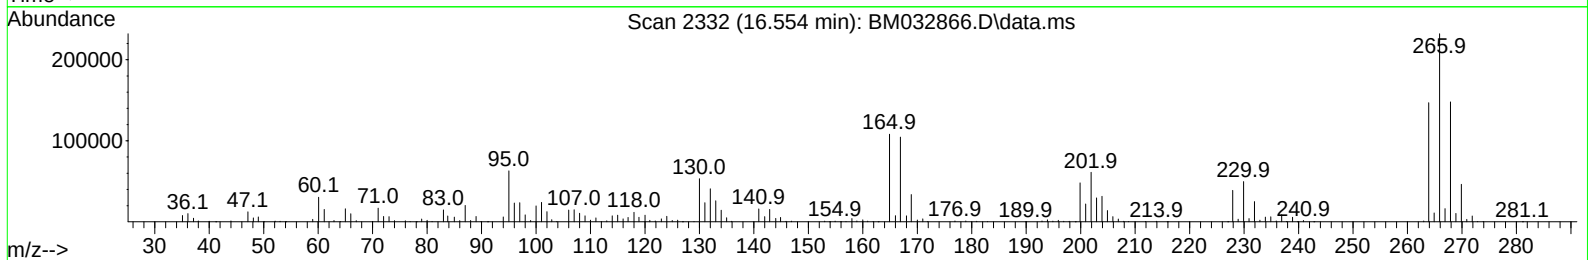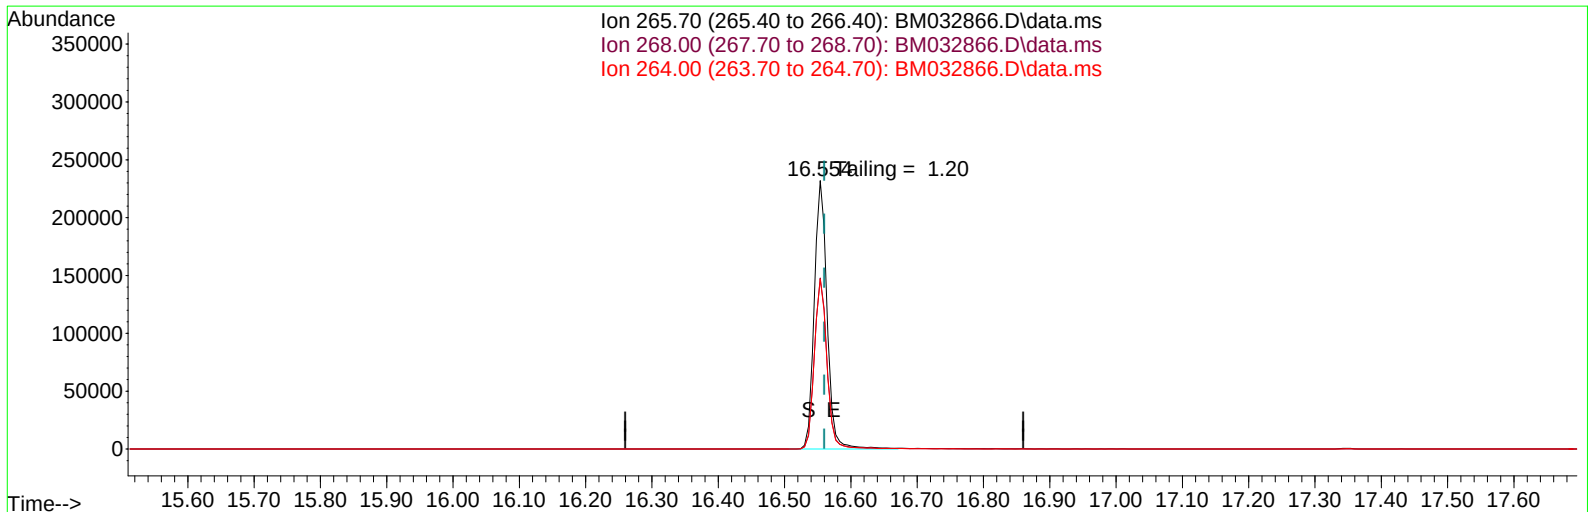

TIC: BM032866.D\data.ms

(70) Pentachlorophenol (C)

16.554min (-0.006) 0.00 ng




response 313931

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	63.75
264.00	65.10	63.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110421\
Data File : BM032866.D
Acq On : 04 Nov 2021 09:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 04 14:59:28 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 02 16:07:18 2021
Response via : Initial Calibration

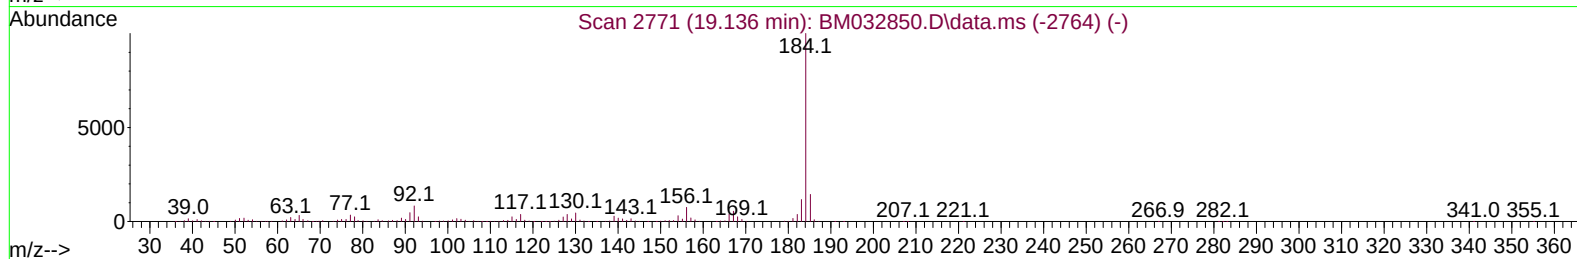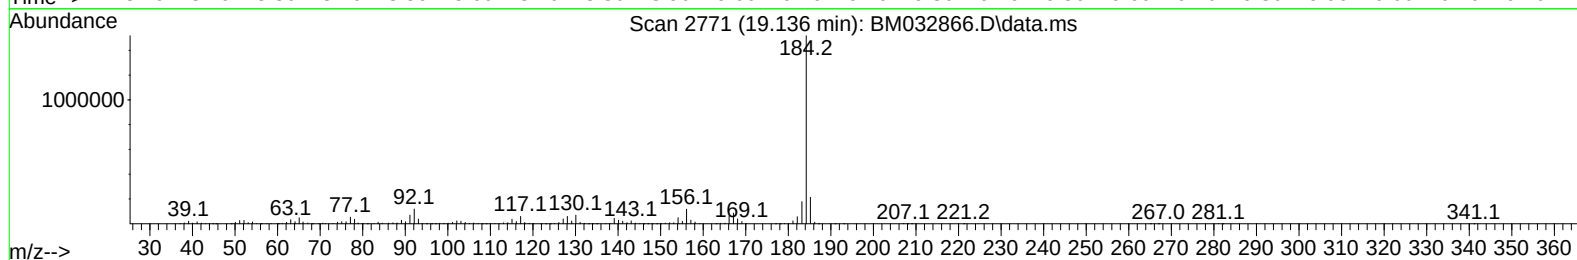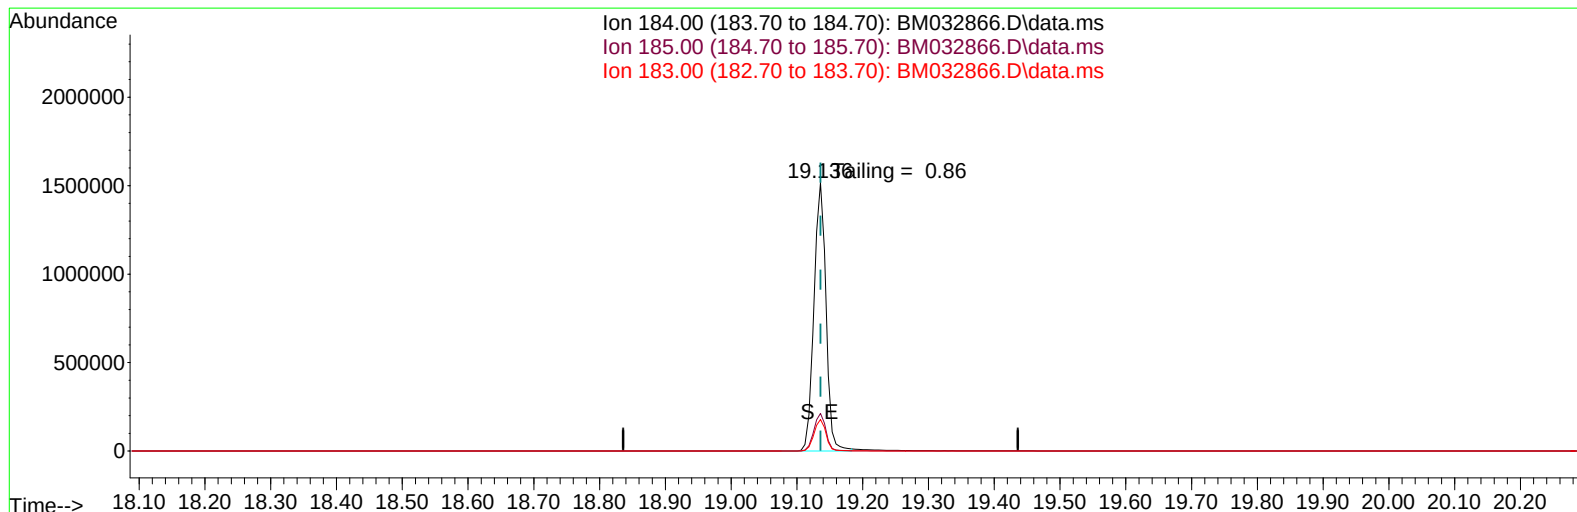

TIC: BM032866.D\data.ms

(77) Benzidine

19.136min (-0.000) 608796.38 ng

response 1952047

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	14.03
183.00	11.20	11.79
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_M
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
11/4/2021	BNA_M	<u>BM032866.D</u>
Compound Name	Response	Retention Time
DDT	864712	20.37
DDD	8185	19.93
DDE	545	19.43
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8730	873442	1.00