
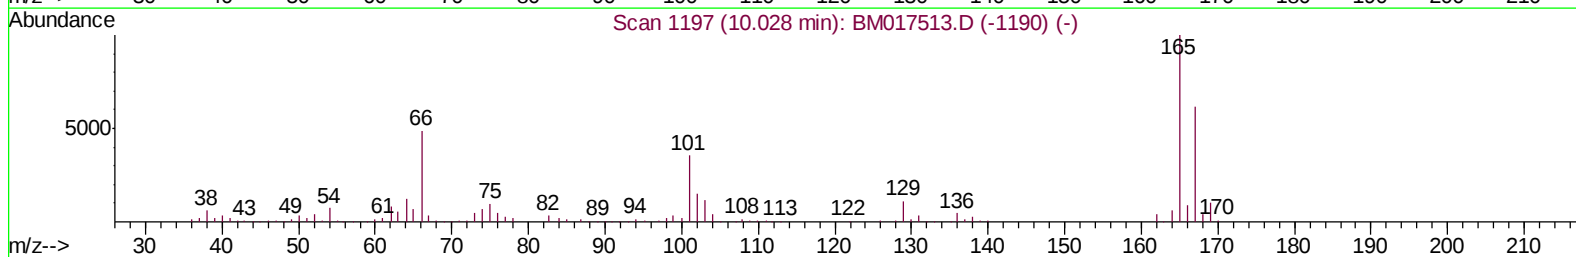
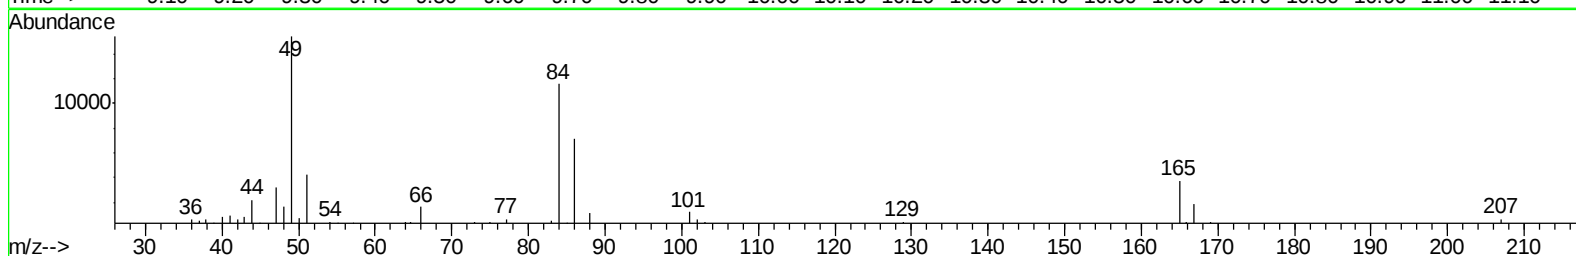


Data File : BM017514.D
Acq On : 05 Nov 2018 14:05
Operator : MJ/SJ
Sample : J5701-11DL 10X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Nov 06 00:37:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 06 00:34:52 2018
Response via : Initial Calibration

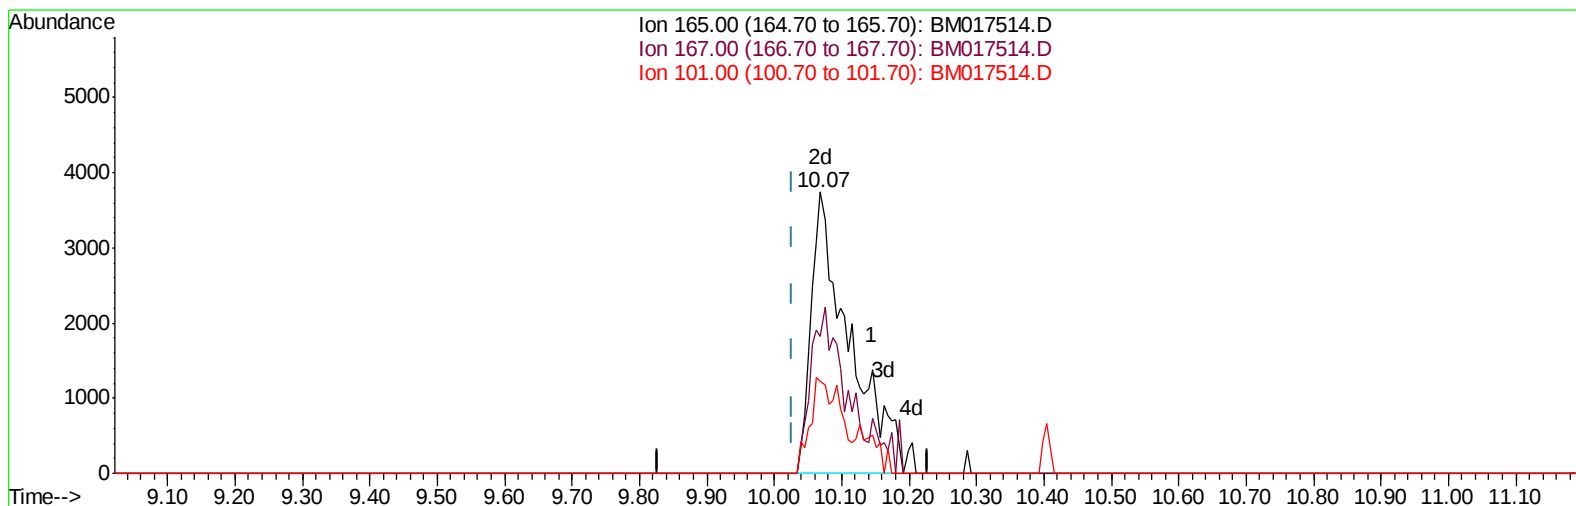

TIC: BM017514.D

(26) 2,4-Dichlorophenol-d3 (S)

10.069min (+0.041) 1.15ng/ul m

response 14600

Ion	Exp%	Act%
165.00	100	100
167.00	63.60	48.47#
101.00	34.30	32.85
0.00	0.00	0.00