
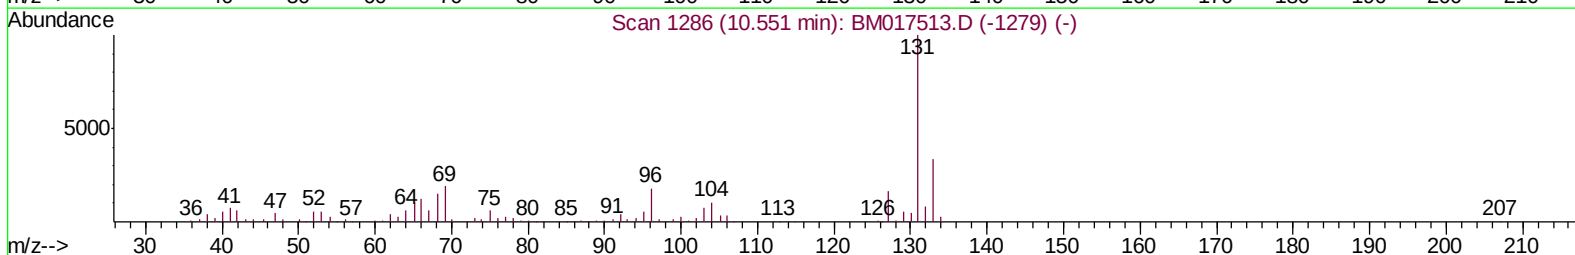
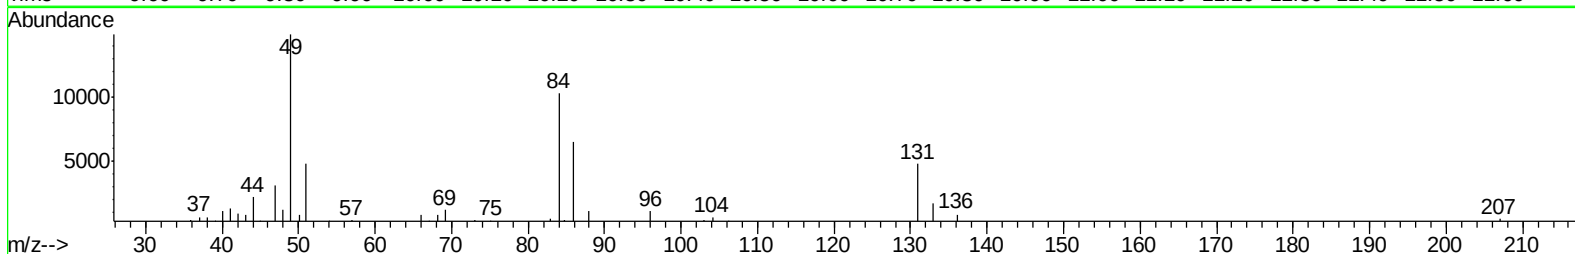


Data File : BM017514.D
Acq On : 05 Nov 2018 14:05
Operator : MJ/SJ
Sample : J5701-11DL 10X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Nov 06 00:37:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 06 00:34:52 2018
Response via : Initial Calibration

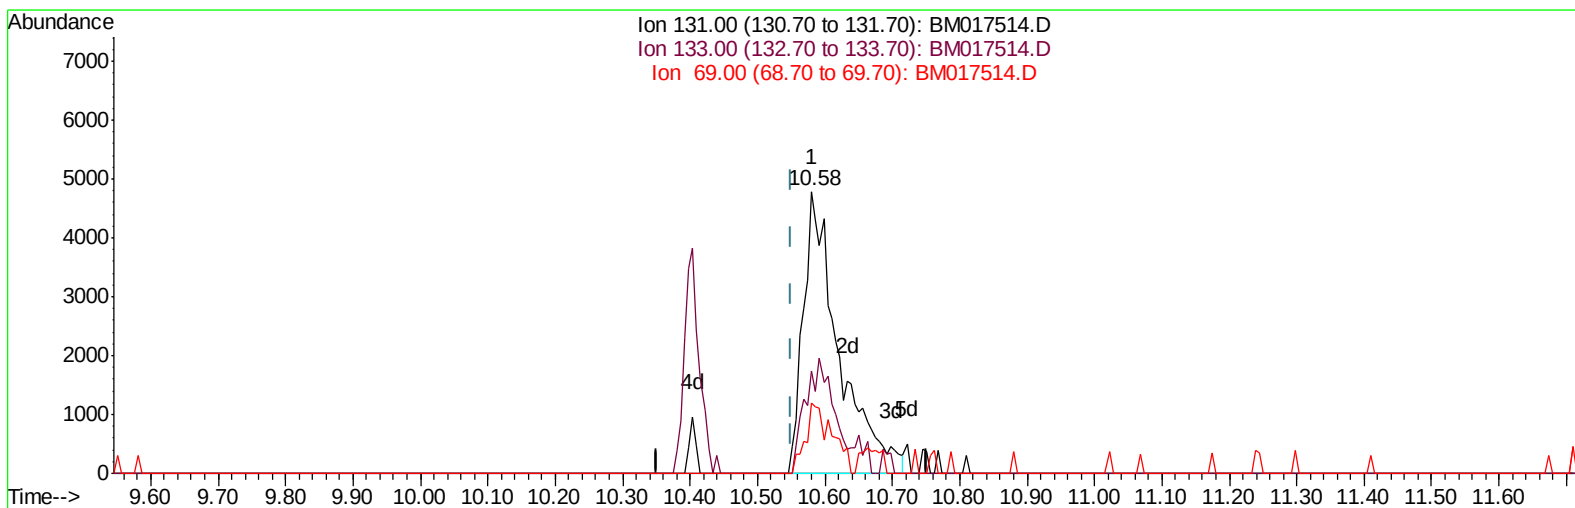

TIC: BM017514.D

(29) 4-Chloroaniline-d4 (S)

10.580min (+0.029) 1.69ng/ul m

response 17468

Ion	Exp%	Act%
131.00	100	100
133.00	33.60	36.16
69.00	17.60	24.80#
0.00	0.00	0.00